

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022498.D
 Acq On : 12 Apr 2022 11:33
 Operator : SY/VA
 Sample : N2262-12
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Apr 12 23:31:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	355293	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	342553	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	175291	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	148780	18.942	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.760%
7) Chloroethane-d5	2.885	69	99554	20.224	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.880%
11) 1,1-Dichloroethene-d2	4.019	63	153967	15.113	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.440%
21) 2-Butanone-d5	7.074	46	80211	58.493	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.980%
24) Chloroform-d	7.647	84	285901	25.745	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.960%
26) 1,2-Dichloroethane-d4	8.305	65	165433	26.072	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.280%
32) Benzene-d6	8.275	84	514523	24.585	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.320%
36) 1,2-Dichloropropane-d6	9.274	67	157091	25.937	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.760%
41) Toluene-d8	10.323	98	484613	23.643	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.560%
43) trans-1,3-Dichloroprop...	10.579	79	67945	23.771	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.080%
47) 2-Hexanone-d5	10.921	63	67719	60.097	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.200%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	143920	27.947	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.800%
66) 1,2-Dichlorobenzene-d4	13.853	152	179361	28.888	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.560%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	6357	0.719	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
Data File : VW022498.D
Acq On : 12 Apr 2022 11:33
Operator : SY/VA
Sample : N2262-12
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Apr 12 23:31:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 12 23:30:19 2022
Response via : Initial Calibration

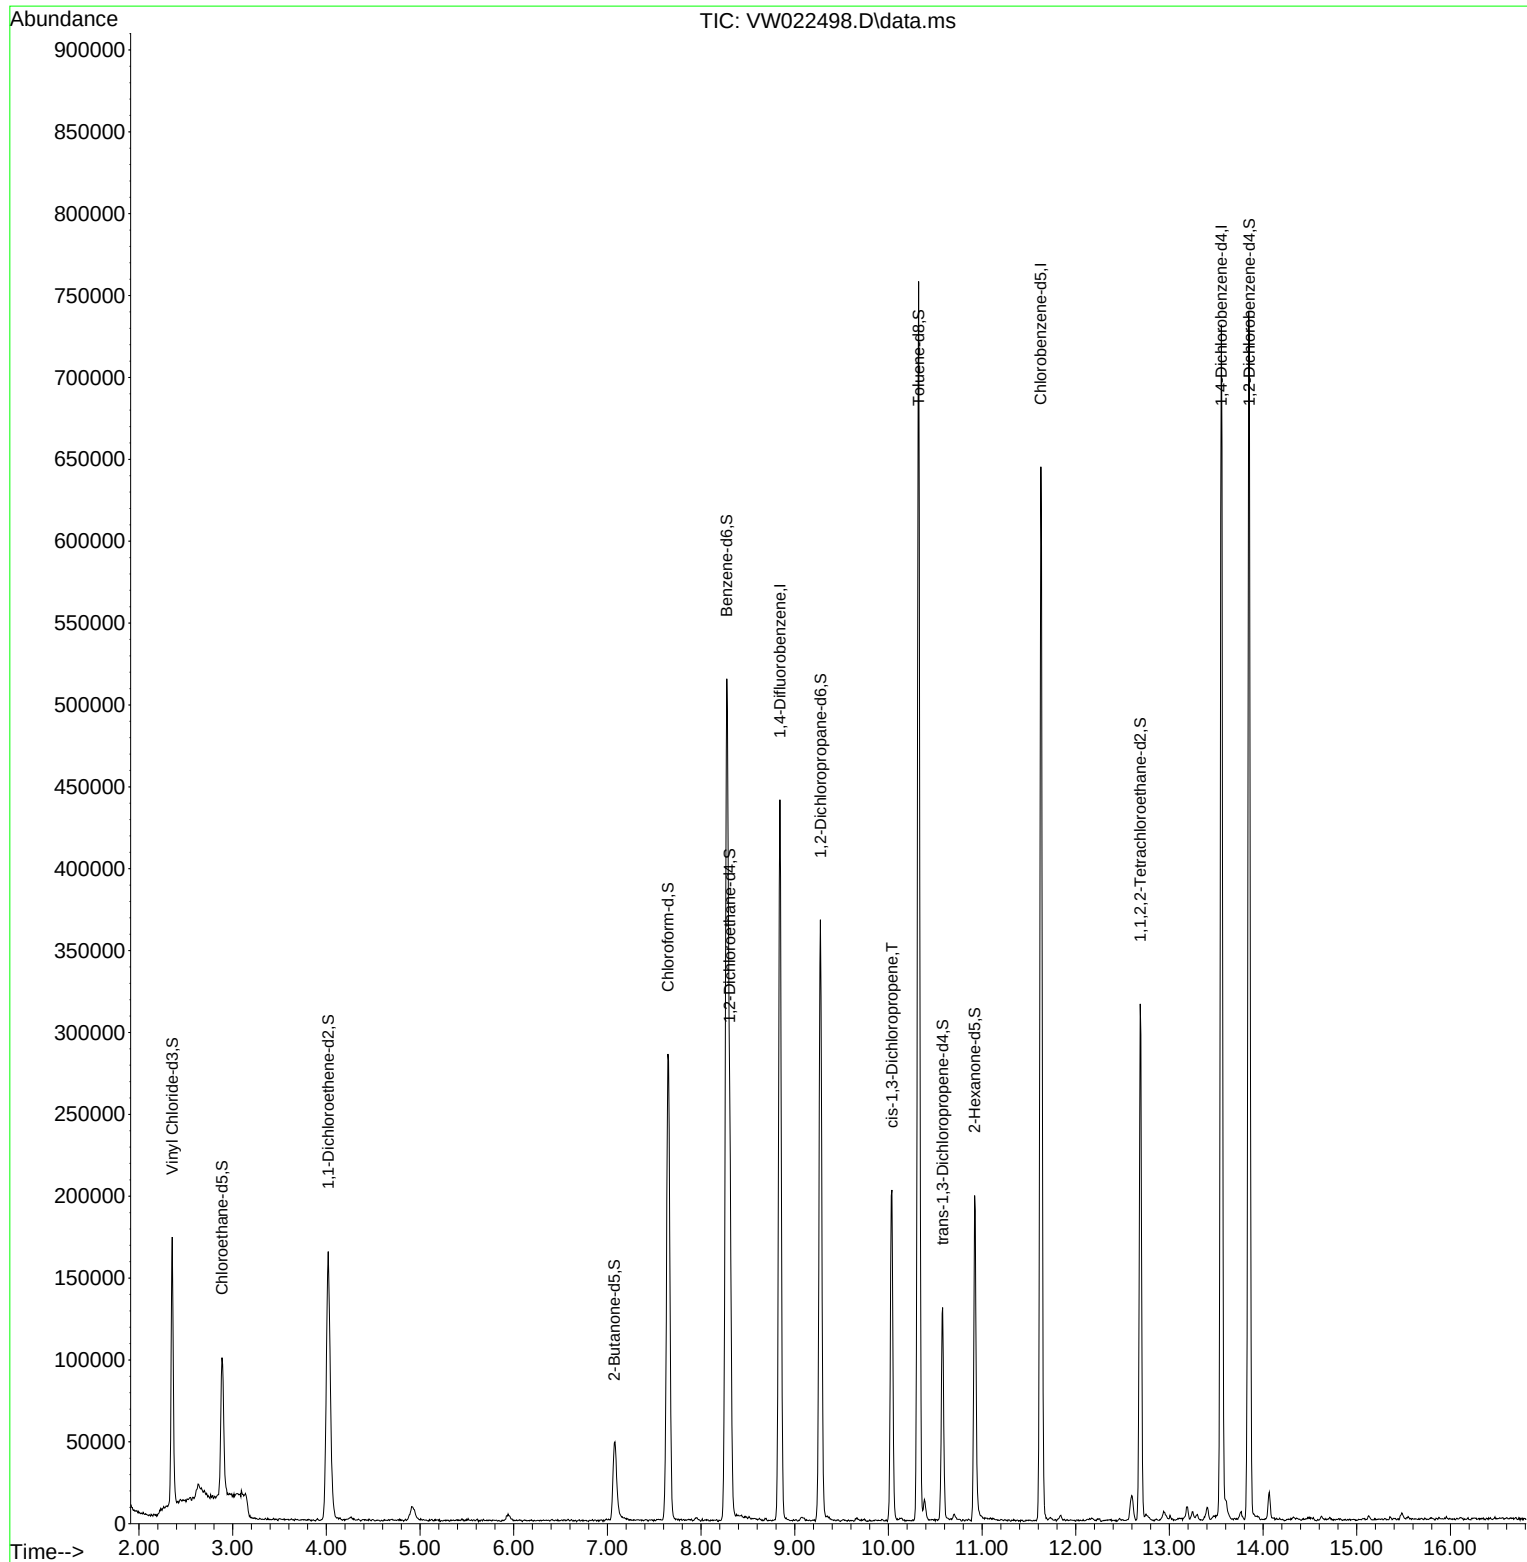

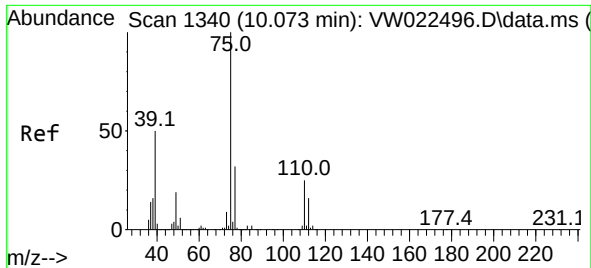

#39
 cis-1,3-Dichloropropene
 Concen: 0.719 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022498.D
 Acq: 12 Apr 2022 11:33

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 6357
 Ion Ratio Lower Upper
 75 100
 77 41.0 22.6 42.0

