

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022518.D
 Acq On : 12 Apr 2022 19:35
 Operator : SY/VA
 Sample : N2373-02
 Misc : 5.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD3

Quant Time: Apr 12 23:35:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	341151	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	263181	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	82746	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	132004	17.503	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.000%
7) Chloroethane-d5	2.886	69	99539	21.059	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.240%
11) 1,1-Dichloroethene-d2	4.013	63	135328	13.835	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.320%
21) 2-Butanone-d5	7.080	46	78229	59.413	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.820%
24) Chloroform-d	7.653	84	256733	24.076	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.320%
26) 1,2-Dichloroethane-d4	8.305	65	152869	25.091	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.360%
32) Benzene-d6	8.275	84	430830	26.794	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.160%
36) 1,2-Dichloropropane-d6	9.275	67	141139	30.332	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	121.320%#
41) Toluene-d8	10.323	98	356913	22.664	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.640%
43) trans-1,3-Dichloroprop...	10.579	79	45000	20.491	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.960%
47) 2-Hexanone-d5	10.927	63	61280	70.784	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.560%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	121793	30.783	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	123.120%#
66) 1,2-Dichlorobenzene-d4	13.847	152	73673	25.137	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.560%
Target Compounds						Qvalue
68) 1,2-Dibromo-3-chloropr...	14.463	75	2460	6.026	ug/L #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
Data File : VW022518.D
Acq On : 12 Apr 2022 19:35
Operator : SY/VA
Sample : N2373-02
Misc : 5.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFD3

Quant Time: Apr 12 23:35:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 12 23:30:19 2022
Response via : Initial Calibration

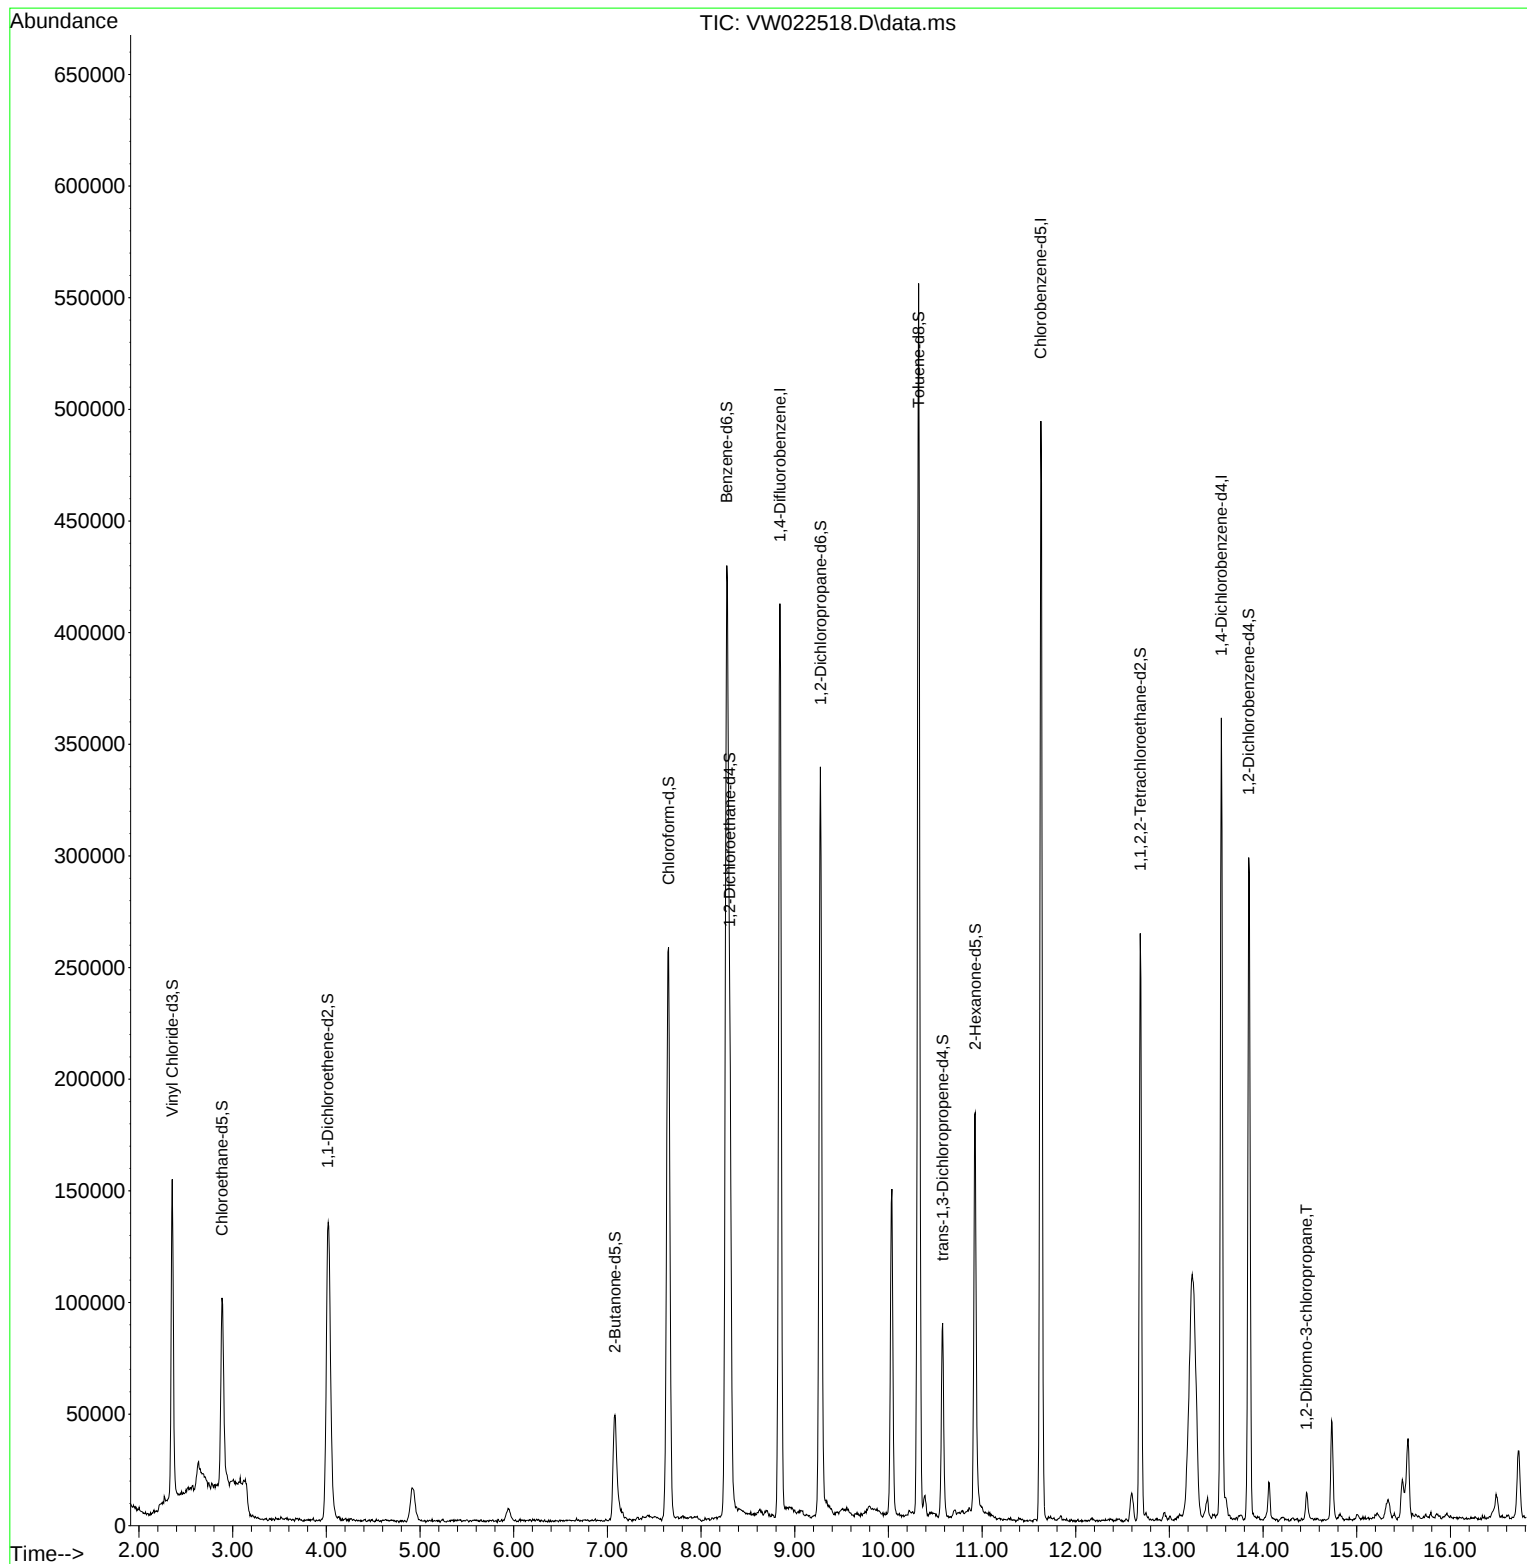

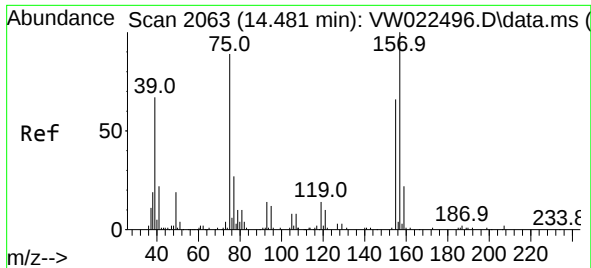

#68
 1,2-Dibromo-3-chloropropane
 Concen: 6.026 ug/L
 RT: 14.463 min Scan# 2060
 Delta R.T. -0.018 min
 Lab File: VW022518.D
 Acq: 12 Apr 2022 19:35

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD3

Tgt Ion: 75 Resp: 2460
 Ion Ratio Lower Upper
 75 100
 155 0.0 55.6 83.4#
 157 0.0 69.8 104.6#

