




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022515.D
 Acq On : 12 Apr 2022 18:22
 Operator : SY/VA
 Sample : N2374-01
 Misc : 3.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 23:34:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

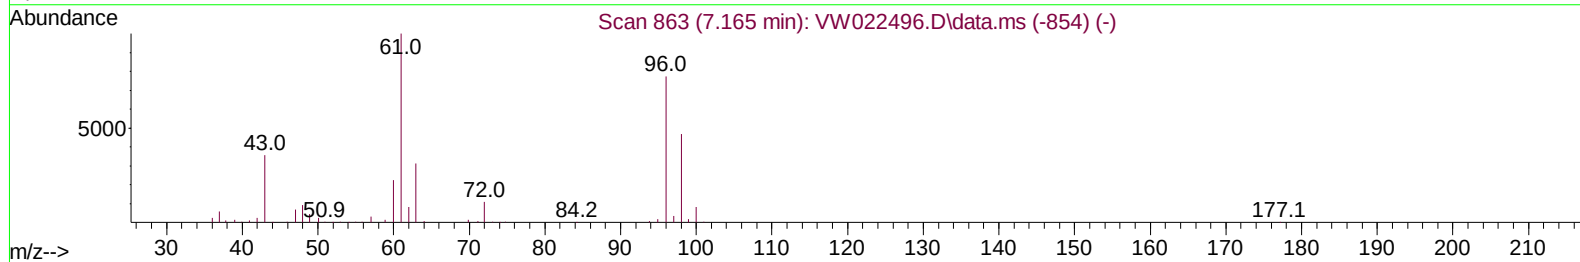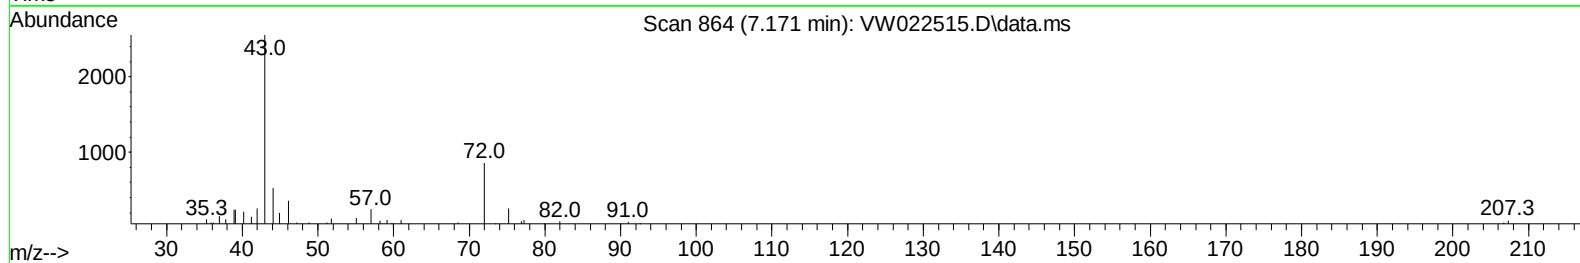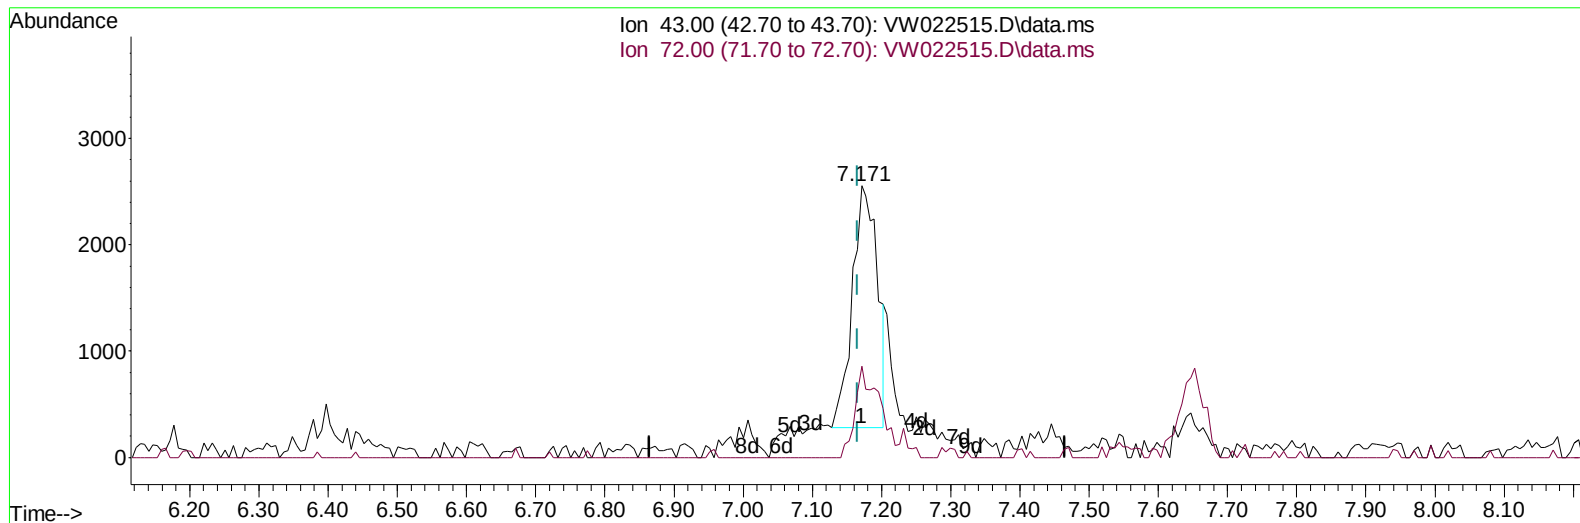

TIC: VW022515.D\data.ms

(22) 2-Butanone (T)

7.171min (+ 0.006) 4.59 ug/L

response 5684

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	28.00	21.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022515.D
 Acq On : 12 Apr 2022 18:22
 Operator : SY/VA
 Sample : N2374-01
 Misc : 3.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 23:34:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

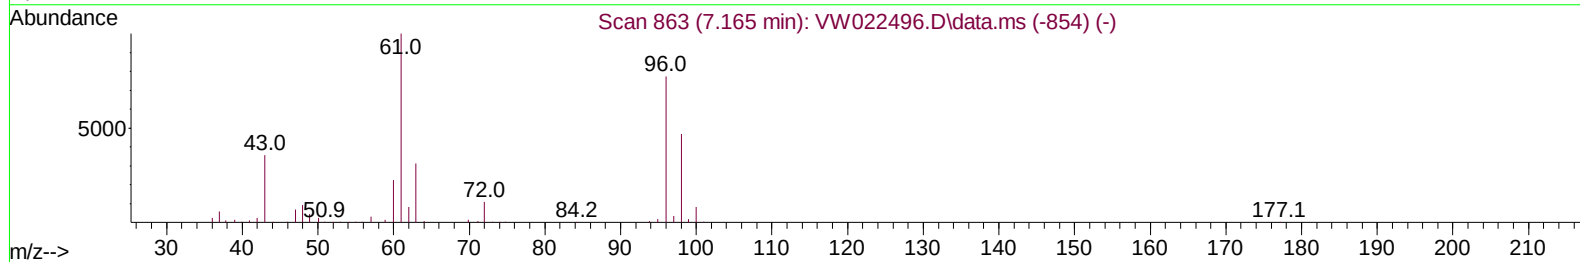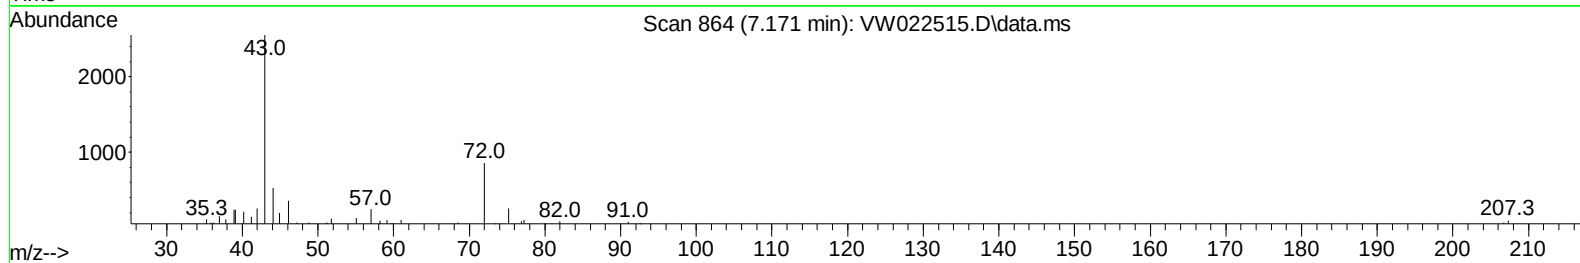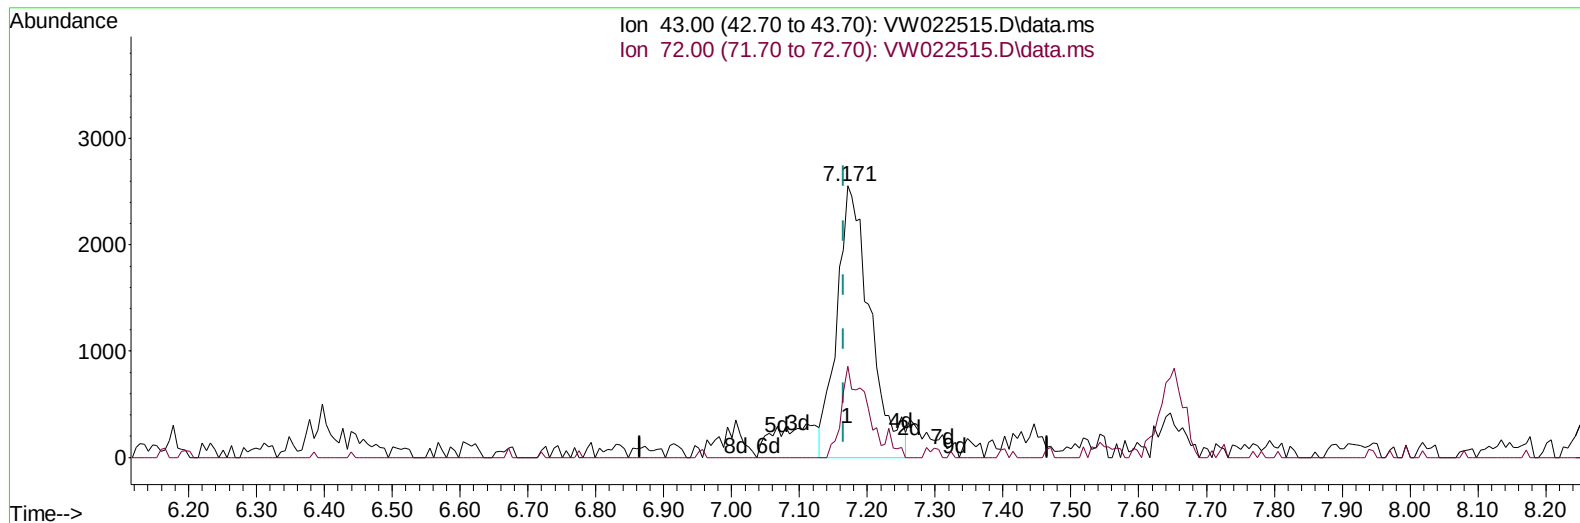

TIC: VW022515.D\data.ms

(22) 2-Butanone (T)

7.171min (+ 0.006) 6.97 ug/L m

response 8642

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	28.00	13.98#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022515.D
 Acq On : 12 Apr 2022 18:22
 Operator : SY/VA
 Sample : N2374-01
 Misc : 3.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 23:34:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

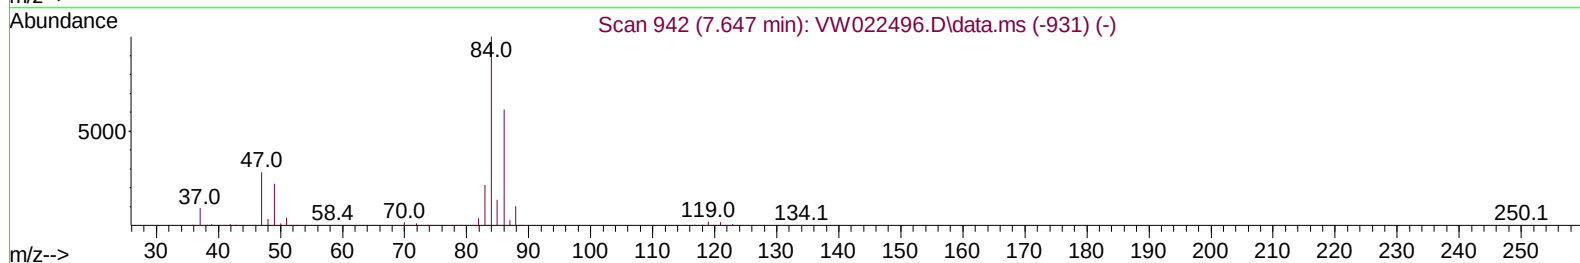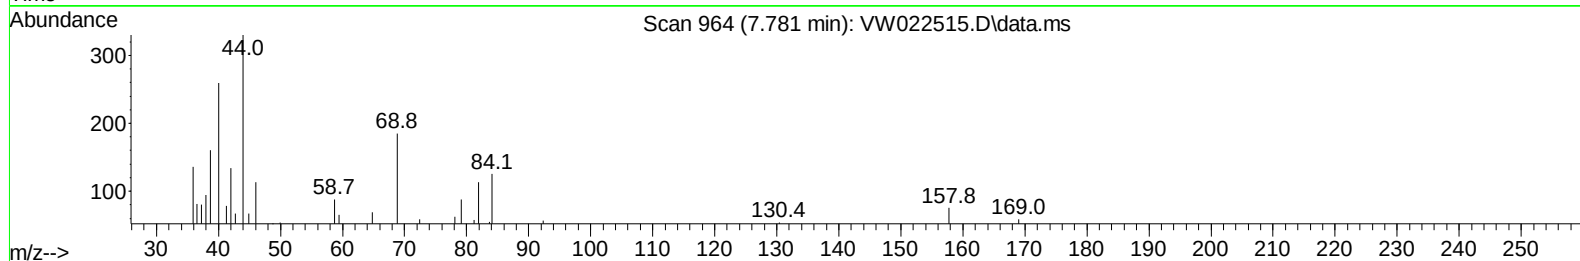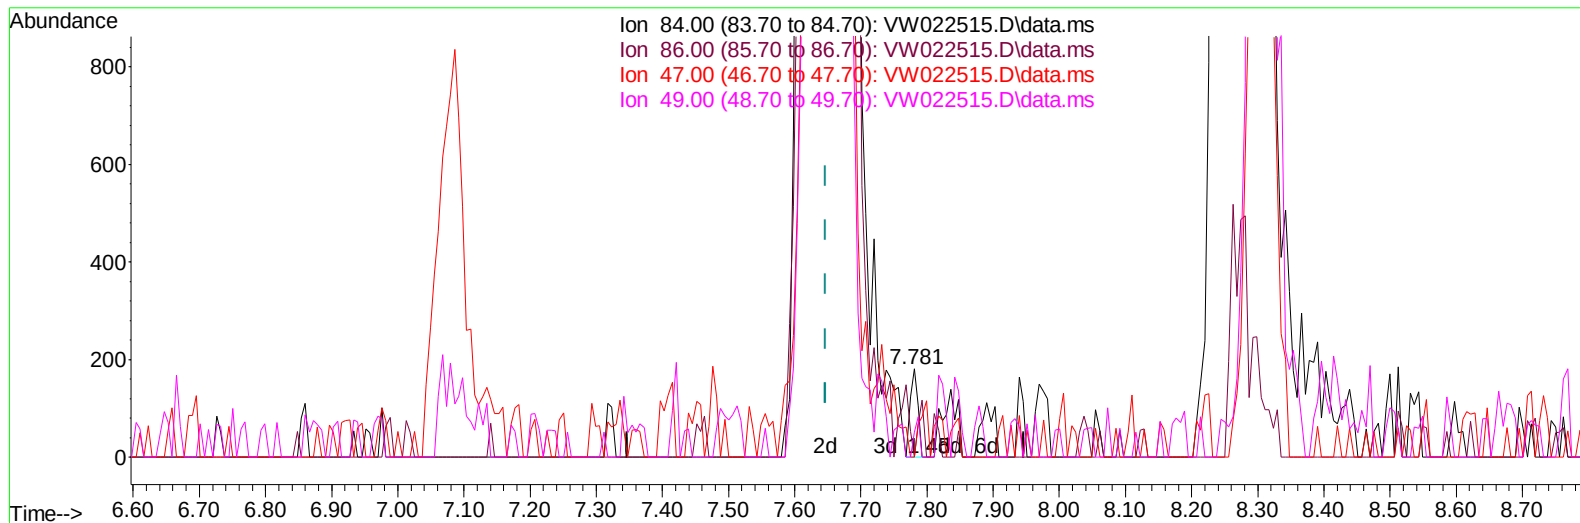

TIC: VW022515.D\data.ms

(24) Chloroform-d (S)

7.781min (+ 0.134) 0.02 ug/L

response 150

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	45.33
47.00	51.50	65.33
49.00	31.80	32.67




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022515.D
 Acq On : 12 Apr 2022 18:22
 Operator : SY/VA
 Sample : N2374-01
 Misc : 3.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 23:34:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

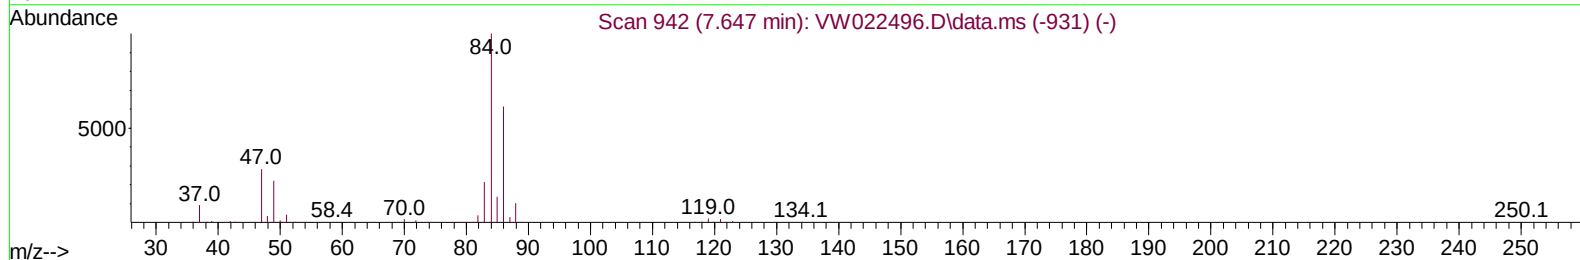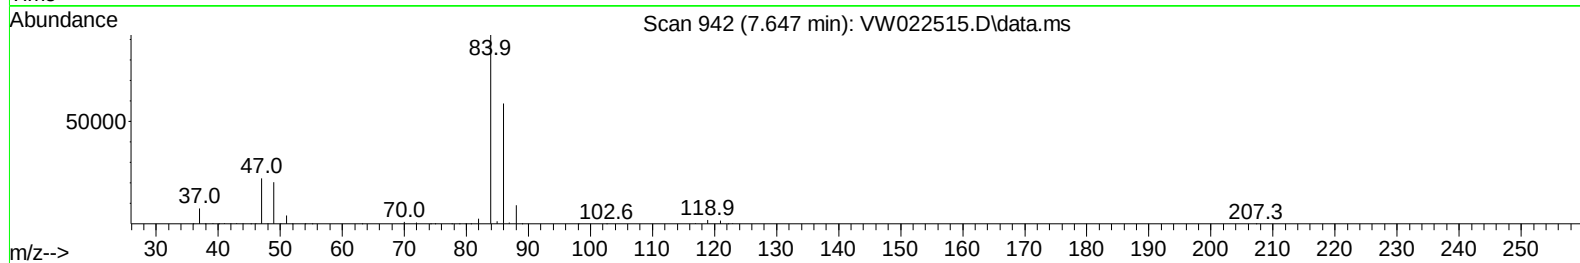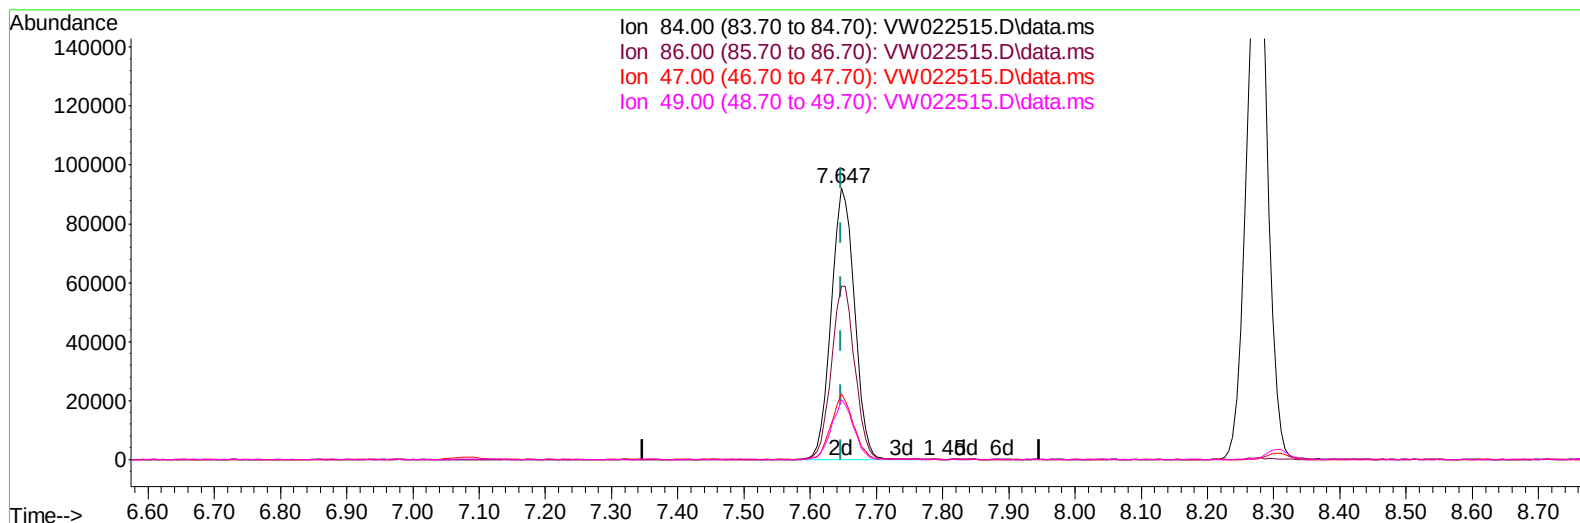

TIC: VW022515.D\data.ms

(24) Chloroform-d (S)

7.647min (0.000) 23.13 ug/L m

response 225806

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	0.03#
47.00	51.50	0.04#
49.00	31.80	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022515.D
 Acq On : 12 Apr 2022 18:22
 Operator : SY/VA
 Sample : N2374-01
 Misc : 3.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4

Manual IntegrationsAPPROVED

Quant Time: Apr 12 23:34:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	312271	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	222927	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	66309	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	124288	18.004	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.000%	
7) Chloroethane-d5	2.885	69	91335	21.111	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.440%	
11) 1,1-Dichloroethene-d2	4.019	63	125234	13.987	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.960%	
21) 2-Butanone-d5	7.080	46	78895	65.460	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	130.920%	
24) Chloroform-d	7.647	84	225806m	23.135	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.520%	
26) 1,2-Dichloroethane-d4	8.305	65	136258	24.433	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.720%	
32) Benzene-d6	8.275	84	405848	29.798	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	119.200%	
36) 1,2-Dichloropropane-d6	9.274	67	126605	32.121	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	128.480%#	
41) Toluene-d8	10.323	98	318036	23.842	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.360%	
43) trans-1,3-Dichloroprop...	10.579	79	44240	23.783	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.120%	
47) 2-Hexanone-d5	10.920	63	61760	84.220	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	168.440%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98822	29.487	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	117.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	58418	24.873	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.480%	
Target Compounds						
13) Acetone	4.123	43	16140	19.669	ug/L	87
22) 2-Butanone	7.171	43	8642m	6.973	ug/L	
42) Toluene	10.390	91	28666	1.653	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
Data File : VW022515.D
Acq On : 12 Apr 2022 18:22
Operator : SY/VA
Sample : N2374-01
Misc : 3.80g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFD4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/13/2022
Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 23:34:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 12 23:30:19 2022
Response via : Initial Calibration

