

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
 Data File : VW022517.D
 Acq On : 12 Apr 2022 19:11
 Operator : SY/VA
 Sample : N2373-01
 Misc : 3.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 23:35:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 12 23:30:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	229256	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	153594	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	44278	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	94559	18.657	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.640%		
7) Chloroethane-d5	2.891	69	70366	22.153	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.600%		
11) 1,1-Dichloroethene-d2	4.019	63	87423	13.299	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	53.200%		
21) 2-Butanone-d5	7.079	46	54927	62.076	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	124.160%		
24) Chloroform-d	7.652	84	165843	23.144	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.560%		
26) 1,2-Dichloroethane-d4	8.311	65	101712m	24.843	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.360%		
32) Benzene-d6	8.274	84	277955	29.620	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	118.480%		
36) 1,2-Dichloropropane-d6	9.274	67	91646	33.748	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	135.000%#		
41) Toluene-d8	10.323	98	205710	22.383	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.520%		
43) trans-1,3-Dichloroprop...	10.579	79	26144	20.399	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.600%		
47) 2-Hexanone-d5	10.920	63	39226	77.637	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	155.280%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	73615	31.881	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	127.520%#		
66) 1,2-Dichlorobenzene-d4	13.852	152	33187	21.161	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.640%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	3583m	5.947	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041222\
Data File : VW022517.D
Acq On : 12 Apr 2022 19:11
Operator : SY/VA
Sample : N2373-01
Misc : 3.29g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFD2

Quant Time: Apr 12 23:35:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 12 23:30:19 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/13/2022
Supervised By :Mahesh Dadoda 04/14/2022

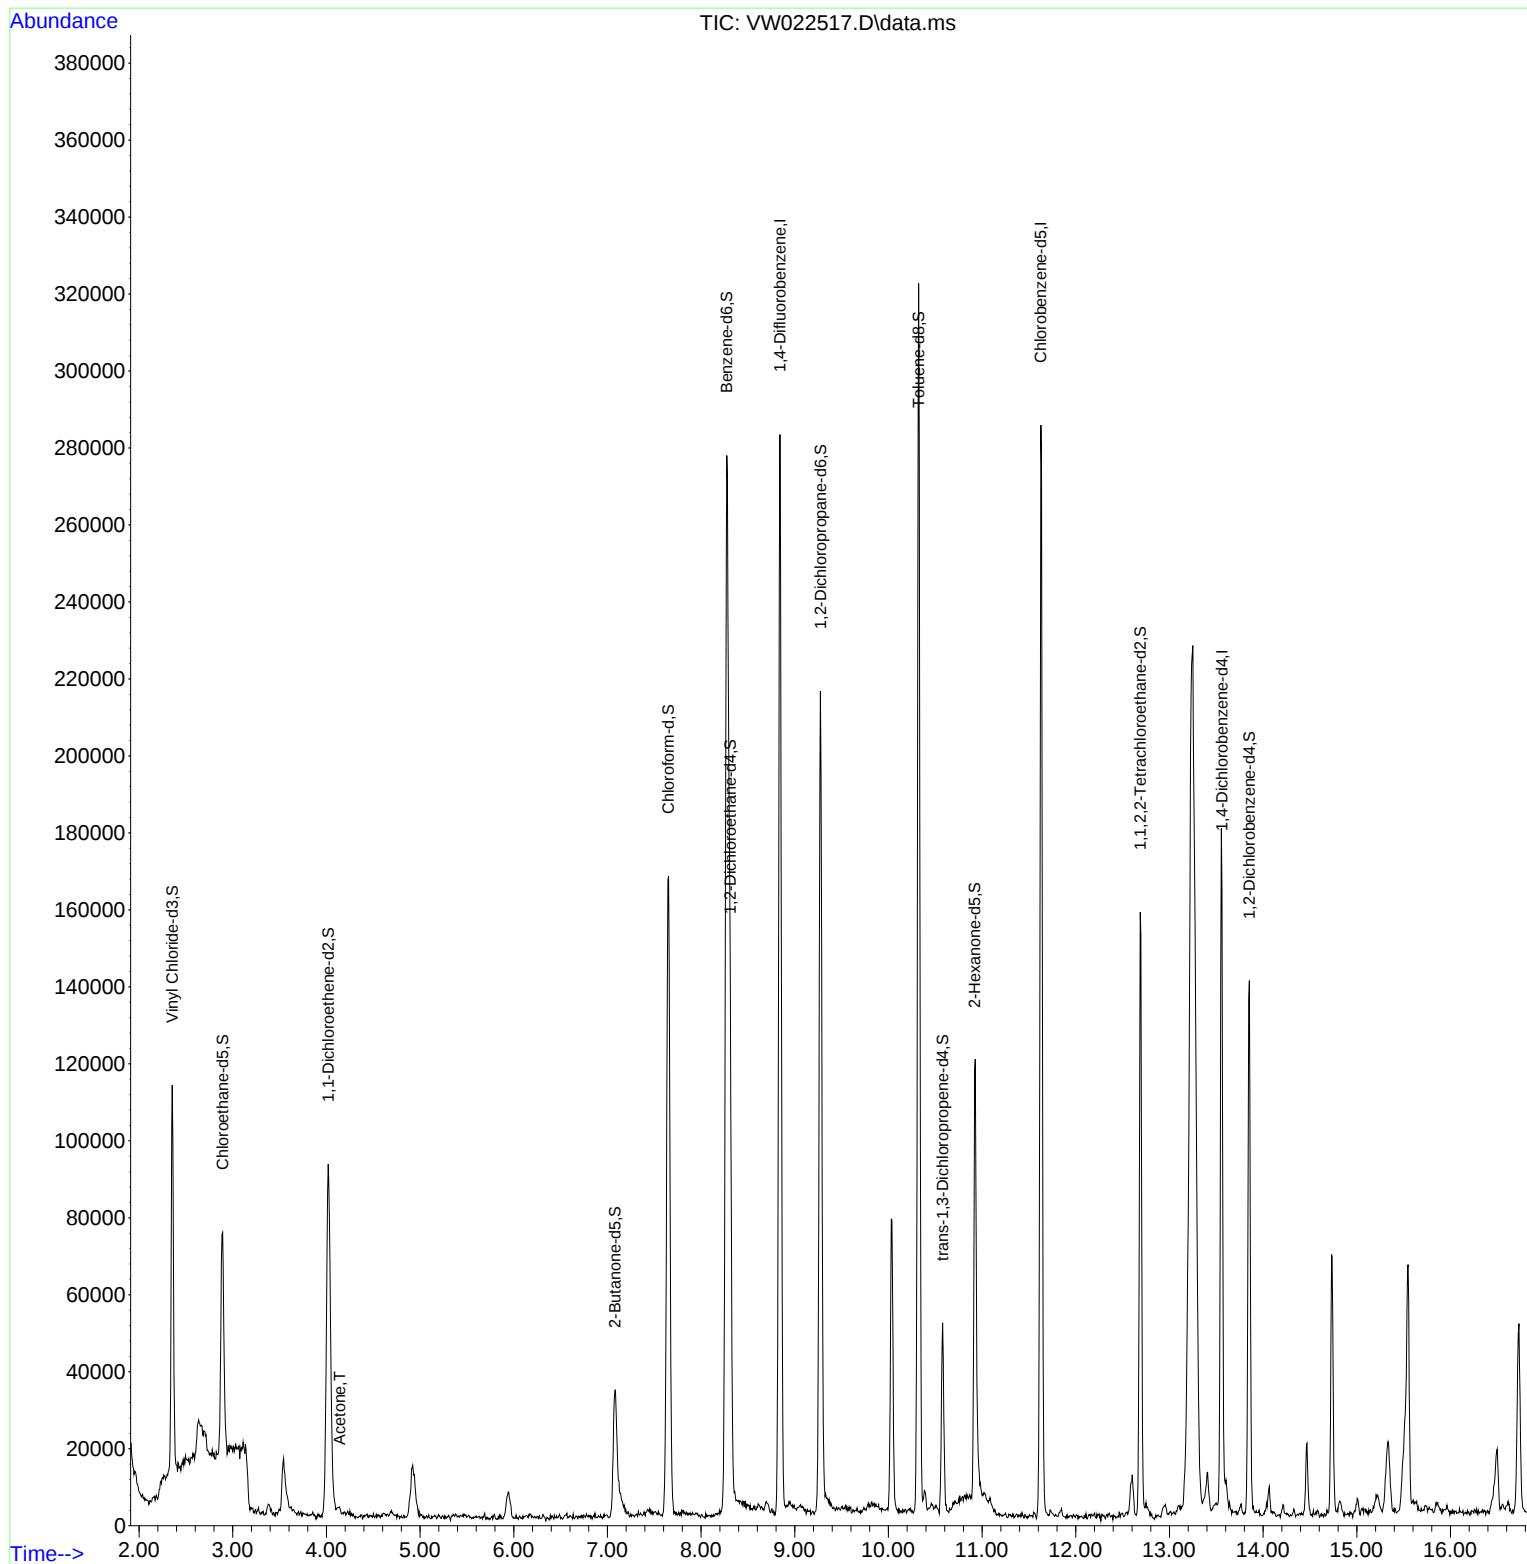

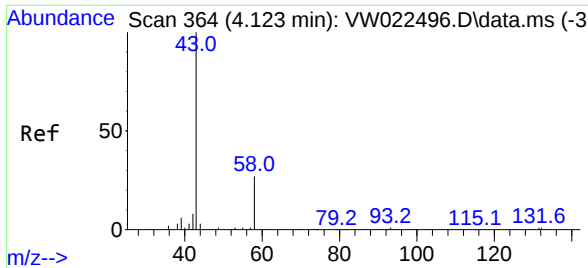

#13
 Acetone
 Concen: 5.947 ug/L m
 RT: 4.141 min Scan# 30
 Delta R.T. 0.018 min
 Lab File: VW022517.D
 Acq: 12 Apr 2022 19:11

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD2

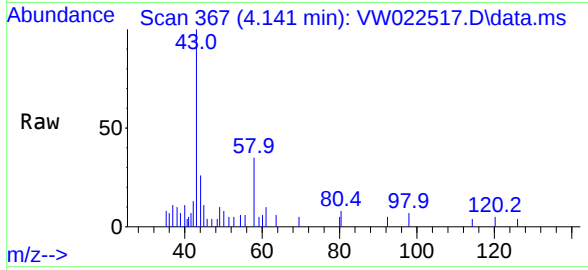

Tgt Ion: 43 Resp: 358
 Ion Ratio Lower Upper
 43 100
 58 6.6 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/13/2022
 Supervised By :Mahesh Dadoda 04/14/2022

