

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041321\
 Data File : VW018642.D
 Acq On : 13 Apr 2021 15:24
 Operator : SY/VA
 Sample : M1968-12
 Misc : 5.08G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleID :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 4/16/2021 12:48:33 PM

Quant Time: Apr 14 01:27:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 14 01:25:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	421482	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	408914	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	203180	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	105837	18.04	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.16%		
7) Chloroethane-d5	2.892	69	94529	18.41	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.64%		
10) 1,1-Dichloroethene-d2	4.019	63	126224m	12.46	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	49.84%		
20) 2-Butanone-d5	7.086	46	66849	51.19	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.38%		
24) Chloroform-d	7.647	84	238555	22.22	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.88%		
26) 1,2-Dichloroethane-d4	8.305	65	149917	23.92	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.68%		
29) Benzene-d6	8.275	84	442125	20.34	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	81.36%		
33) 1,2-Dichloropropane-d6	9.275	67	137007	21.85	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	87.40%		
37) Toluene-d8	10.323	98	409035	19.54	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.16%		
38) trans-1,3-Dichloroprop...	10.579	79	58488	18.09	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	72.36%		
39) 2-Hexanone-d5	10.927	63	52261	42.59	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	85.18%		
48) 1,1,2,2-Tetrachloroeth...	12.689	84	132758	23.67	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.68%		
61) 1,2-Dichlorobenzene-d4	13.853	152	154894	21.44	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.76%		
Target Compounds					Qvalue	
13) Acetone	4.160	43	2440	2.60	ug/L	70
16) Methylene chloride	4.922	84	5889	0.85	ug/L	93
43) 4-Methyl-2-pentanone	10.213	43	3909	1.12	ug/L #	95
44) Toluene	10.390	91	8795	0.33	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041321\
Data File : VW018642.D
Acq On : 13 Apr 2021 15:24
Operator : SY/VA
Sample : M1968-12
Misc : 5.08G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED


MMDadoda
4/16/2021 12:48:33 PM

Quant Time: Apr 14 01:27:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 14 01:25:39 2021
Response via : Initial Calibration



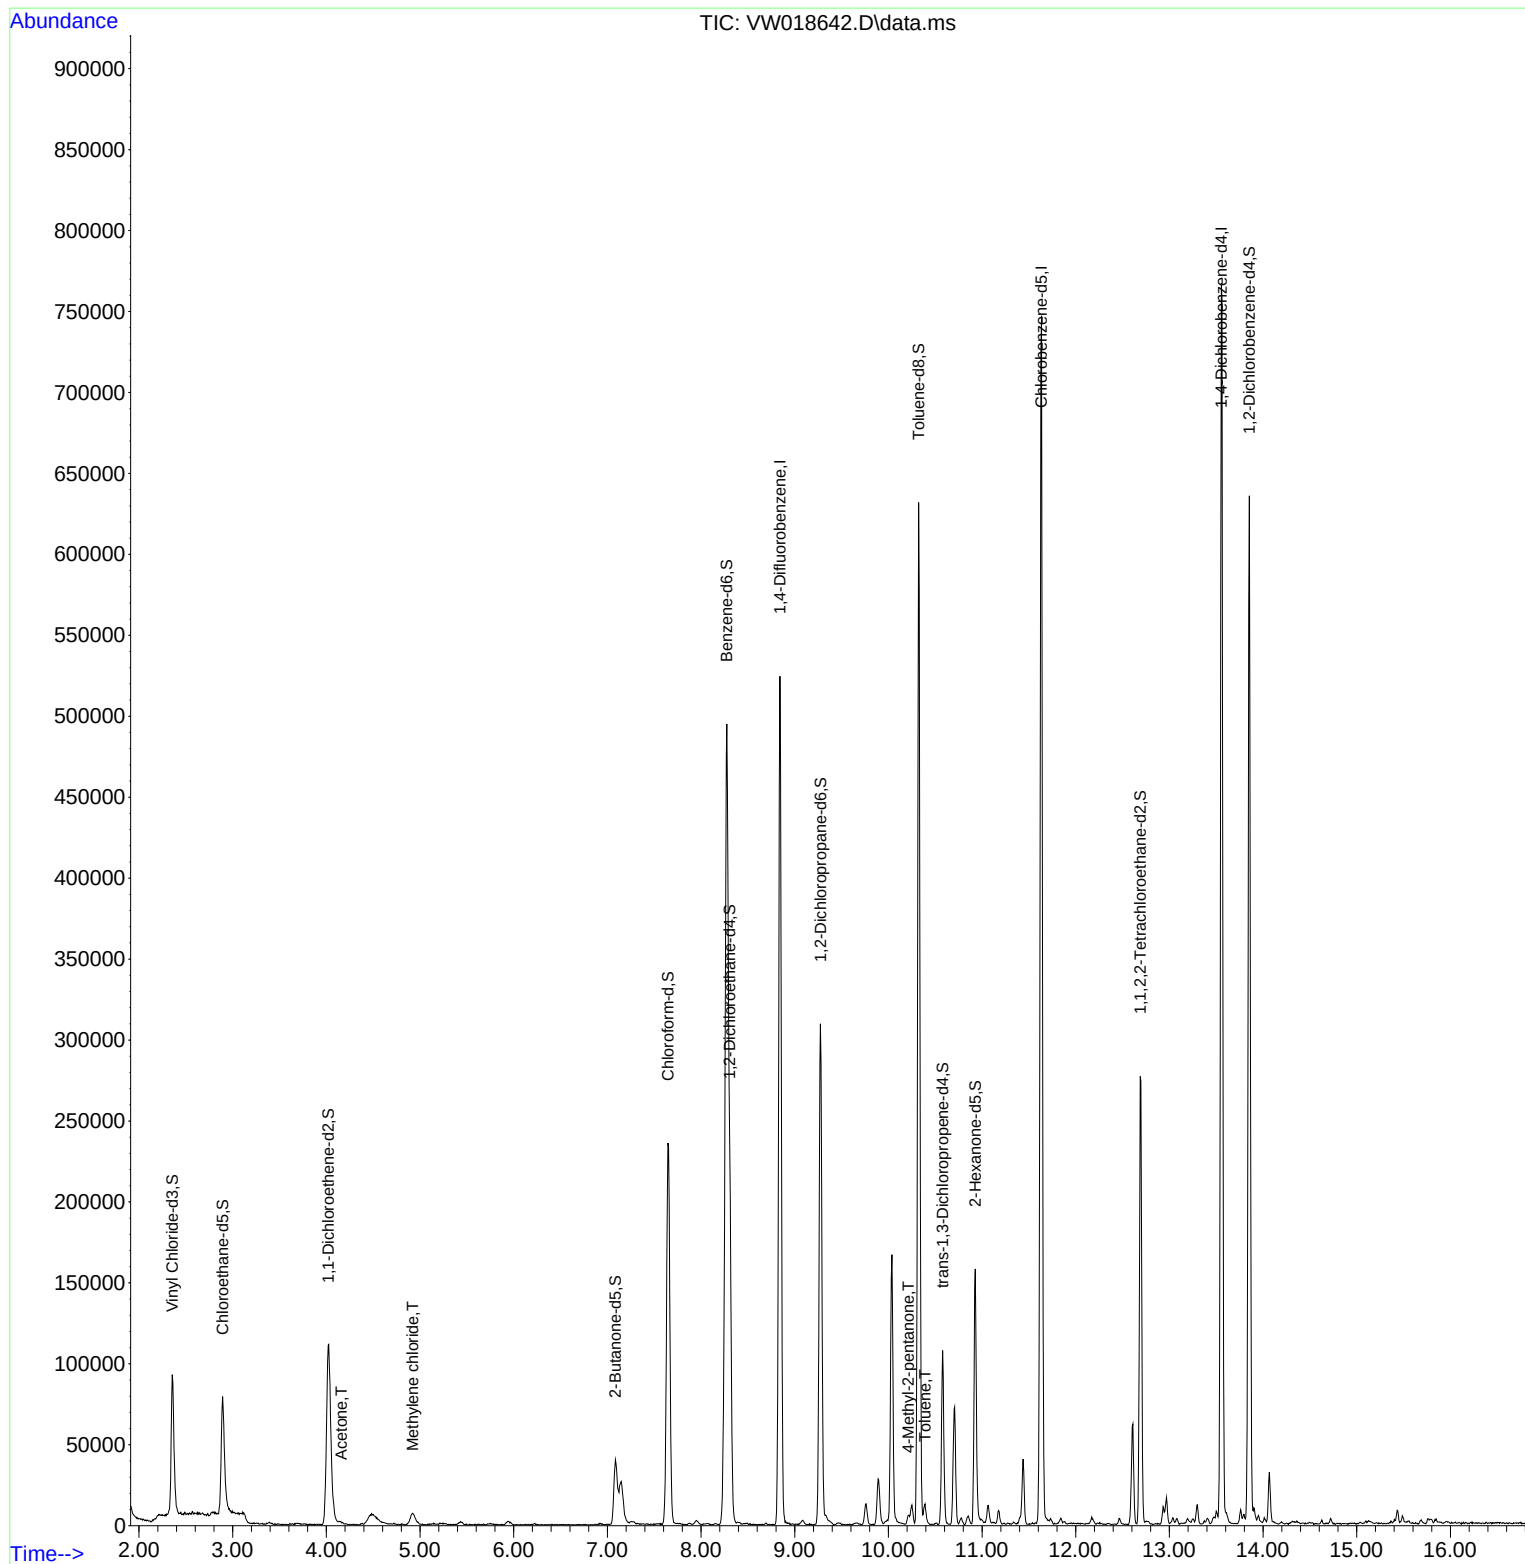


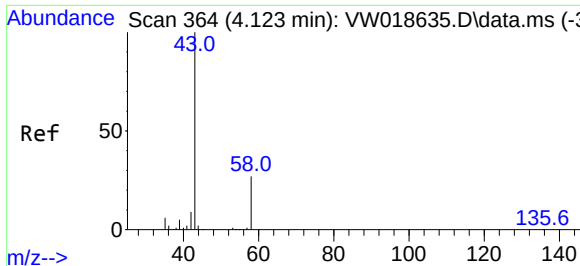


#13
Acetone
Concen: 2.60 ug/L
RT: 4.160 min Scan# 370
Delta R.T. 0.037 min
Lab File: VW018642.D
Acq: 13 Apr 2021 15:24

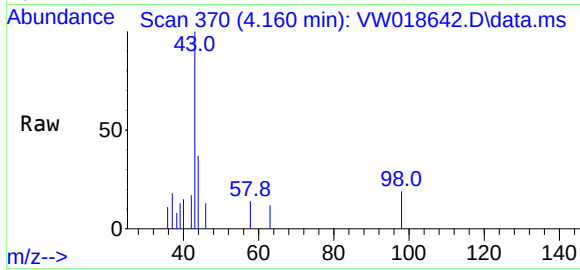



Tgt Ion: 43 Resp: 2440
Ion Ratio Lower Upper
43 100
58 14.6 0.0 62.2

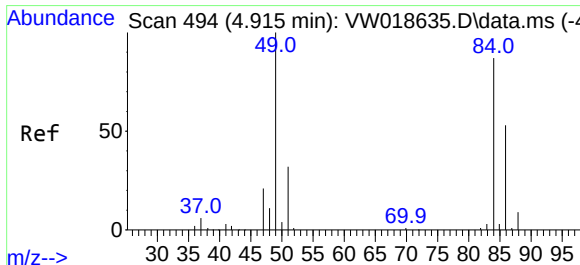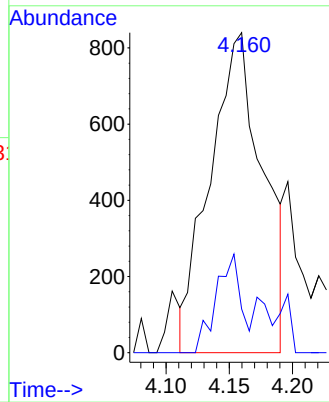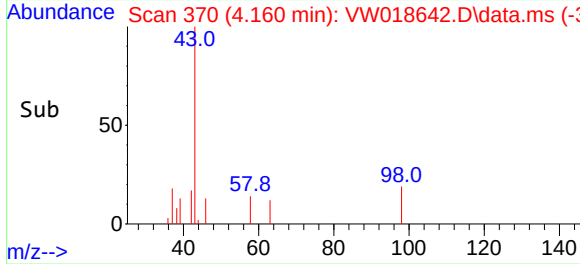

#16
Methylene chloride
Concen: 0.85 ug/L
RT: 4.922 min Scan# 495
Delta R.T. 0.007 min
Lab File: VW018642.D
Acq: 13 Apr 2021 15:24

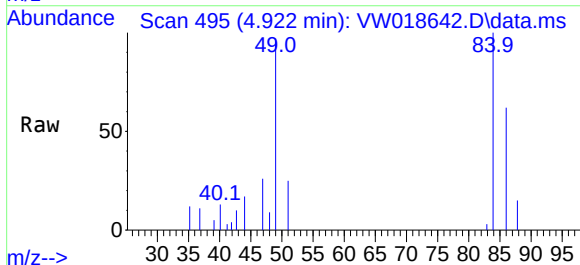


Tgt Ion: 84 Resp: 5889
Ion Ratio Lower Upper
84 100
49 97.4 74.4 138.2
86 62.5 46.1 85.7

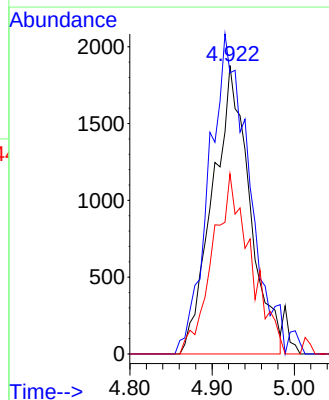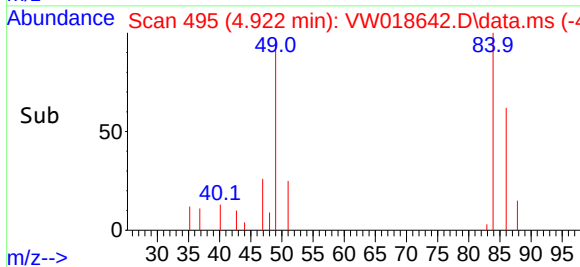

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
4/16/2021 12:48:33 PM

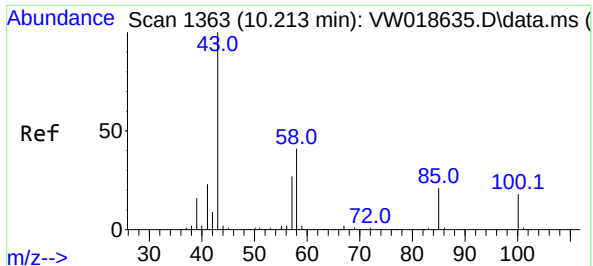





#43
4-Methyl-2-pentanone
Concen: 1.12 ug/L
RT: 10.213 min Scan# 1363
Delta R.T. 0.000 min
Lab File: VW018642.D
Acq: 13 Apr 2021 15:24

Tgt Ion:	43	Resp:	3909
Ion	Ratio	Lower	Upper
43	100		
58	42.9	34.8	52.2
100	12.8	15.9	23.9#

Instrument :
MSVOA_W
ClientSampled :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
4/16/2021 12:48:33 PM

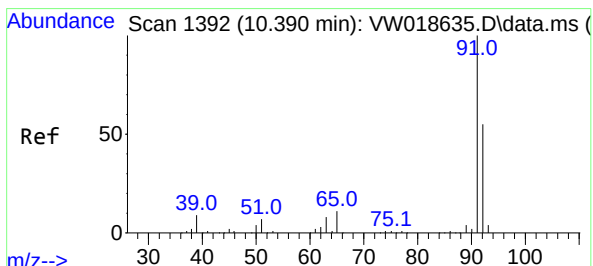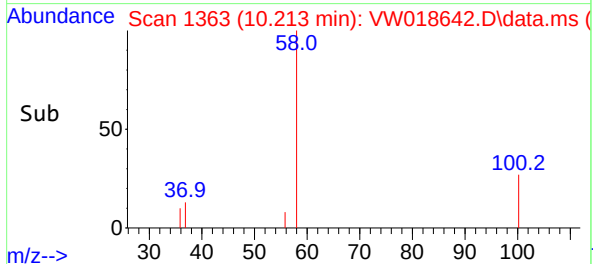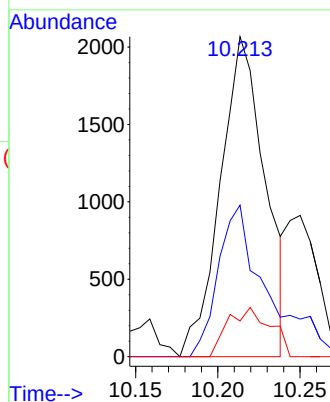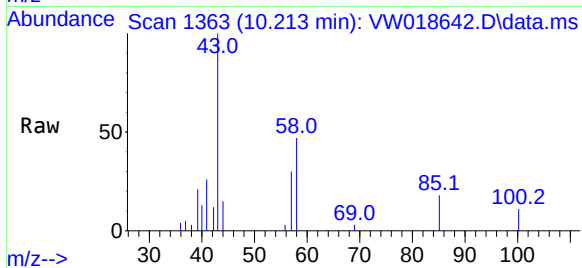

#44
Toluene
Concen: 0.33 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW018642.D
Acq: 13 Apr 2021 15:24

Tgt Ion:	91	Resp:	8795
Ion	Ratio	Lower	Upper
91	100		
92	62.2	42.3	78.5

