


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW041520\
Data File : VW015195.D
Acq On : 15 Apr 2020 10:56
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041520S.M
Title : SW846 8260
Last Update : Wed Apr 15 14:44:16 2020

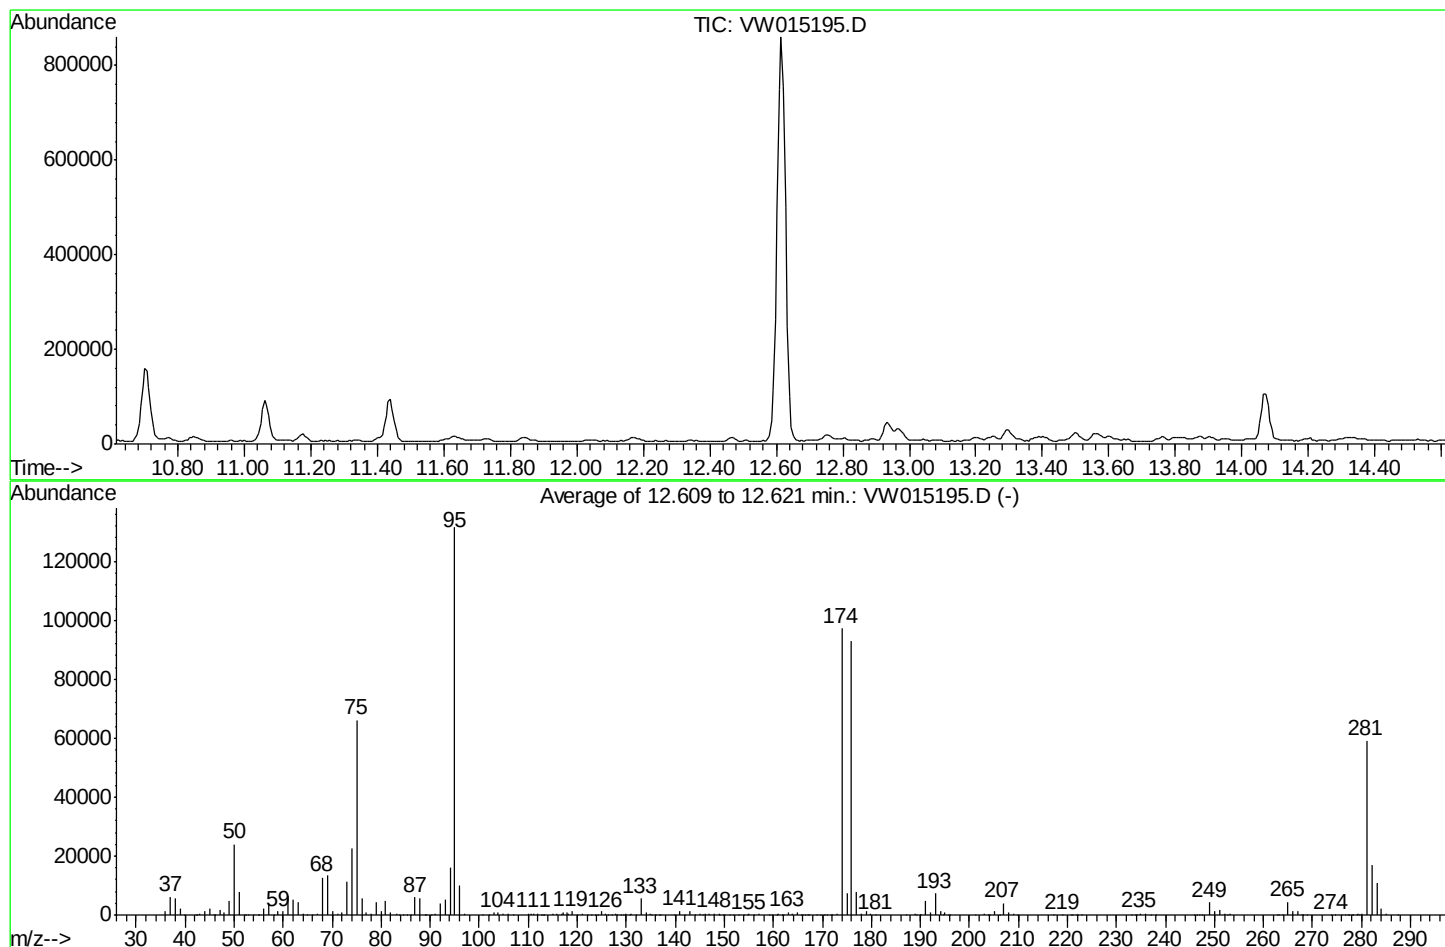

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	24048	PASS
75	95	30	60	50.3	66135	PASS
95	95	100	100	100.0	131501	PASS
96	95	5	9	7.5	9849	PASS
173	174	0.00	2	0.3	279	PASS
174	95	50	100	73.8	97098	PASS
175	174	5	9	7.6	7336	PASS
176	174	95	101	95.6	92842	PASS
177	176	5	9	8.5	7907	PASS