

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041619\
 Data File : VW009995.D
 Acq On : 16 Apr 2019 13:47
 Operator : SY/VA
 Sample : VW0416SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK08

Quant Time: Apr 17 02:10:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 17 02:07:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	633569	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	598593	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	266412	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	163455	27.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.20%
7) Chloroethane-d5	2.89	69	138620	22.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.44%
10) 1,1-Dichloroethene-d2	4.01	63	312883	18.84	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.36%
20) 2-Butanone-d5	7.07	46	137922	42.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.16%
24) Chloroform-d	7.64	84	406611	22.20	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.80%
26) 1,2-Dichloroethane-d4	8.30	65	254781	22.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.68%
29) Benzene-d6	8.27	84	797751	24.25	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.00%
33) 1,2-Dichloropropane-d6	9.27	67	248453	23.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.84%
37) Toluene-d8	10.32	98	715549	23.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.36%
38) trans-1,3-Dichloropropene-	10.58	79	111895	22.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.08%
39) 2-Hexanone-d5	10.93	63	100042	43.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.18%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	204313	20.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	243919	24.36	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.44%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.12	43	5312	1.844	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW041619\
Data File : VW009995.D
Acq On : 16 Apr 2019 13:47
Operator : SY/VA
Sample : VW0416SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK08

Quant Time: Apr 17 02:10:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 17 02:07:51 2019
Response via : Initial Calibration

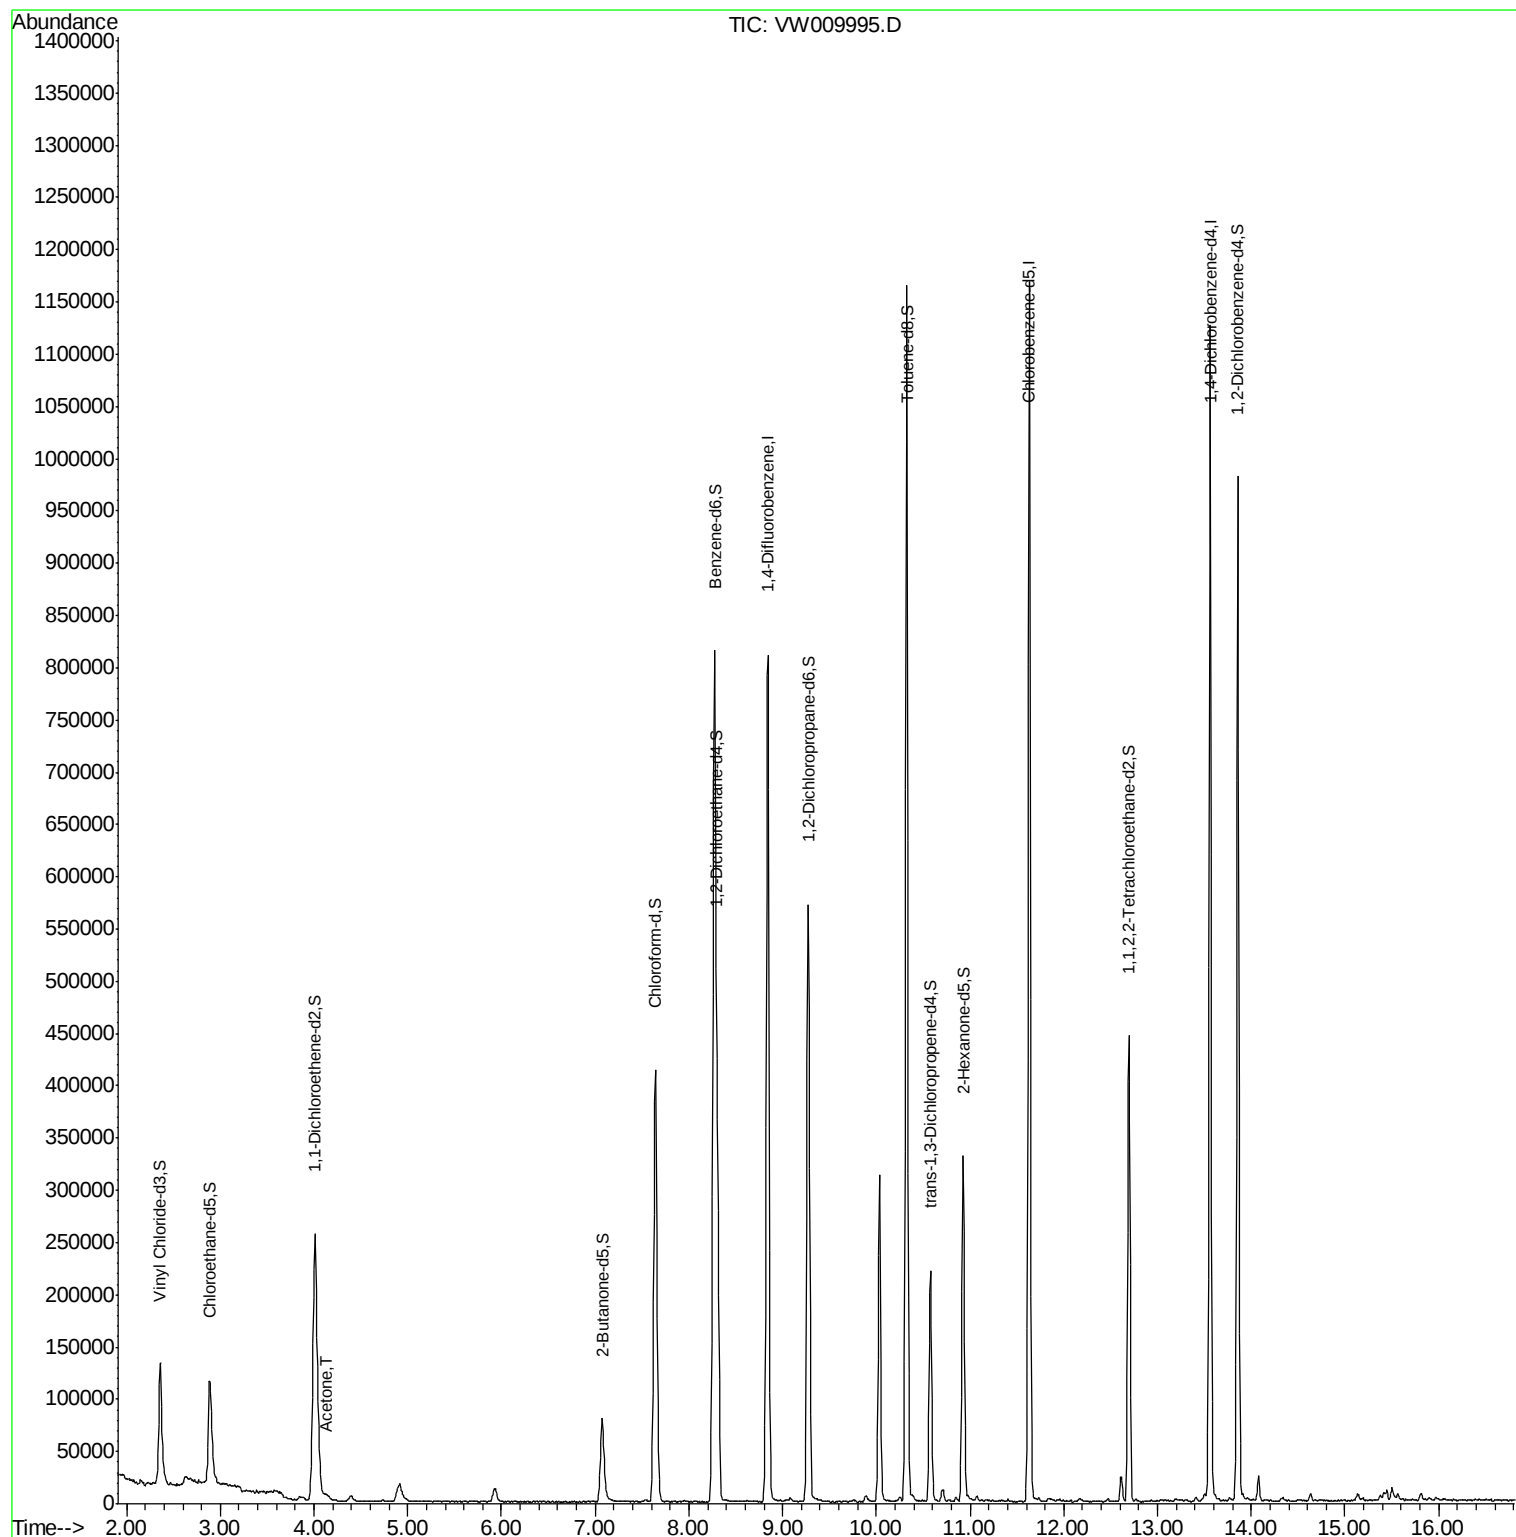

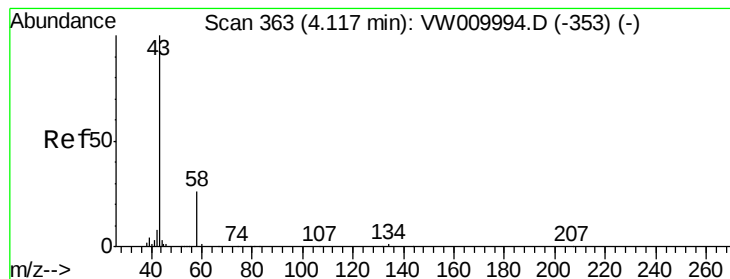

#13

Acetone

Concen: 1.844 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.00 min

Lab File: VW009995.D

Acq: 16 Apr 2019 13:47

Instrument :

MSVOA_W

ClientSampleId :

VBLK08

Tgt Ion: 43 Resp: 5312

Ion Ratio Lower Upper

43 100

58 30.7 0.0 56.2

