

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041619\
 Data File : VW009999.D
 Acq On : 16 Apr 2019 16:31
 Operator : SY/VA
 Sample : K2403-02
 Misc : 7.76G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A5102RE

Quant Time: Apr 17 00:45:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 17 00:43:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	296918	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	300571	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	132462	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	78257	27.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.56%
7) Chloroethane-d5	2.89	69	67561	23.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.08%
10) 1,1-Dichloroethene-d2	4.00	63	154790	19.89	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.56%
20) 2-Butanone-d5	7.08	46	66295	43.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.36%
24) Chloroform-d	7.65	84	202798	23.62	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.48%
26) 1,2-Dichloroethane-d4	8.30	65	128226	24.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.32%
29) Benzene-d6	8.27	84	374536	22.67	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.68%
33) 1,2-Dichloropropane-d6	9.27	67	121170	23.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.12%
37) Toluene-d8	10.32	98	322256	21.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.52%
38) trans-1,3-Dichloropropene-	10.58	79	51416	20.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.44%
39) 2-Hexanone-d5	10.93	63	47363	40.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	107178	21.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.12%
61) 1,2-Dichlorobenzene-d4	13.86	152	118595	23.82	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.28%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.13	43	7543	5.589	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW041619\
Data File : VW009999.D
Acq On : 16 Apr 2019 16:31
Operator : SY/VA
Sample : K2403-02
Misc : 7.76G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A5102RE

Quant Time: Apr 17 00:45:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 17 00:43:03 2019
Response via : Initial Calibration

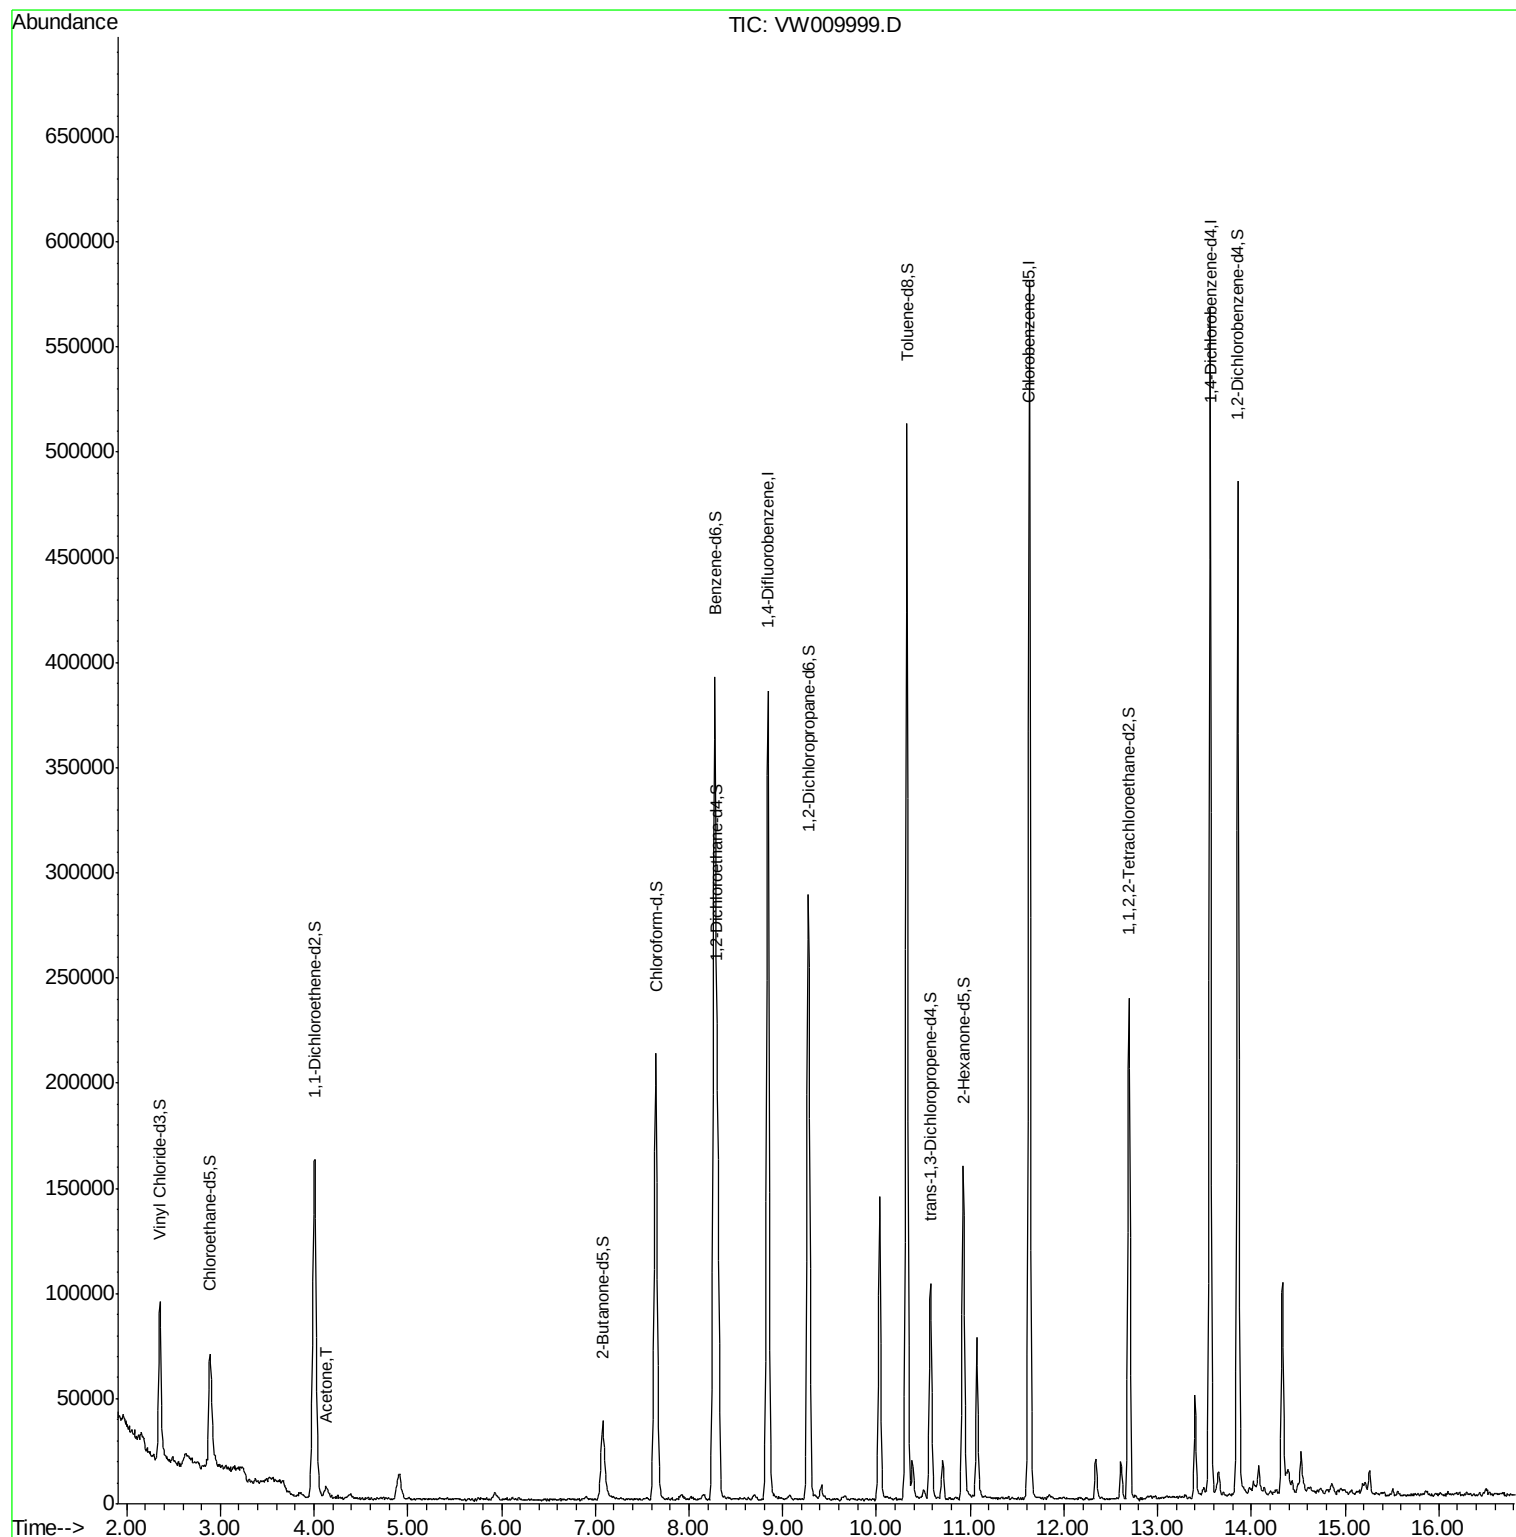

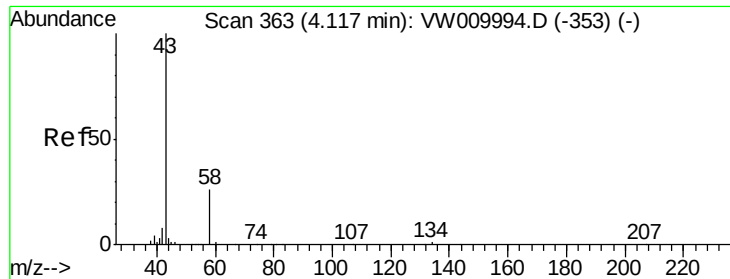

#13

Acetone

Concen: 5.589 ug/L

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW009999.D

Acq: 16 Apr 2019 16:31

Instrument :

MSVOA_W

ClientSampleId :

A5102RE

Tgt Ion: 43 Resp: 7543

Ion Ratio Lower Upper

43 100

58 21.4 0.0 56.2

