



Methylcyclohexane

Response Ratio

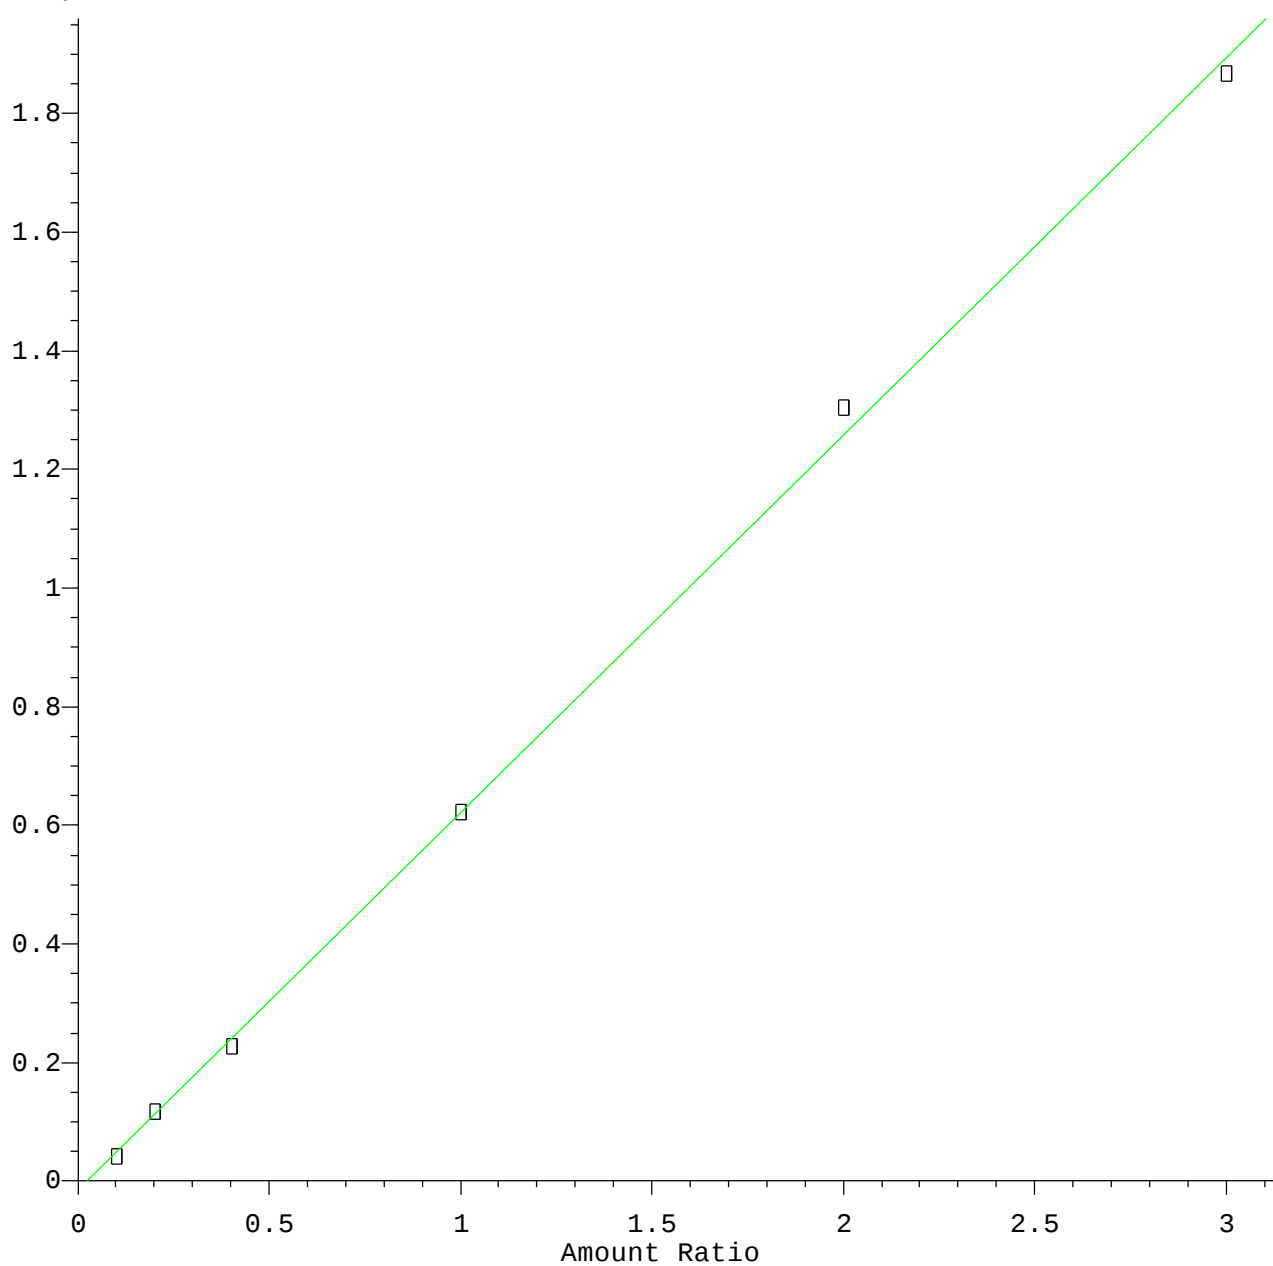


Resp Ratio = $6.37 \times 10^{-1} \times \text{Amt} - 1.52 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041719S.M
Calibration Table Last Updated: Thu Apr 18 11:26:35 2019

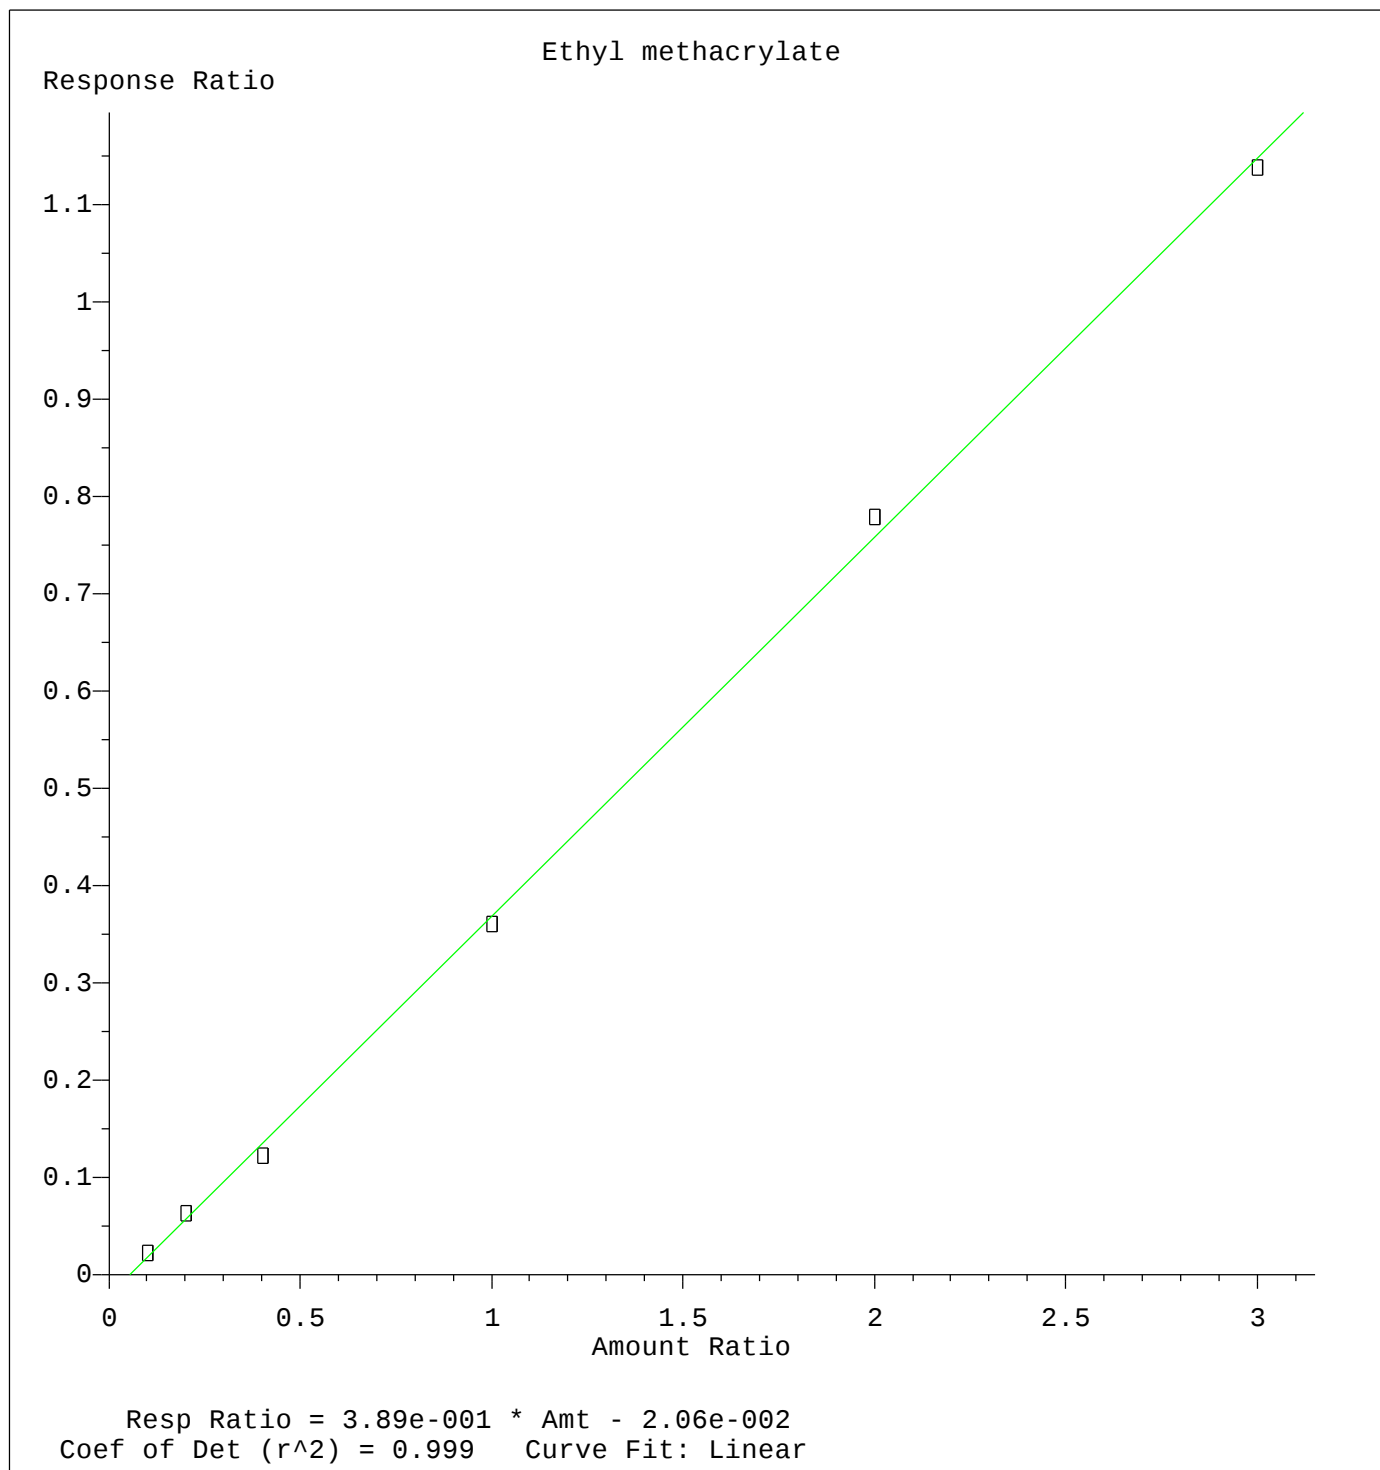

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041719S.M
Calibration Table Last Updated: Thu Apr 18 11:26:35 2019

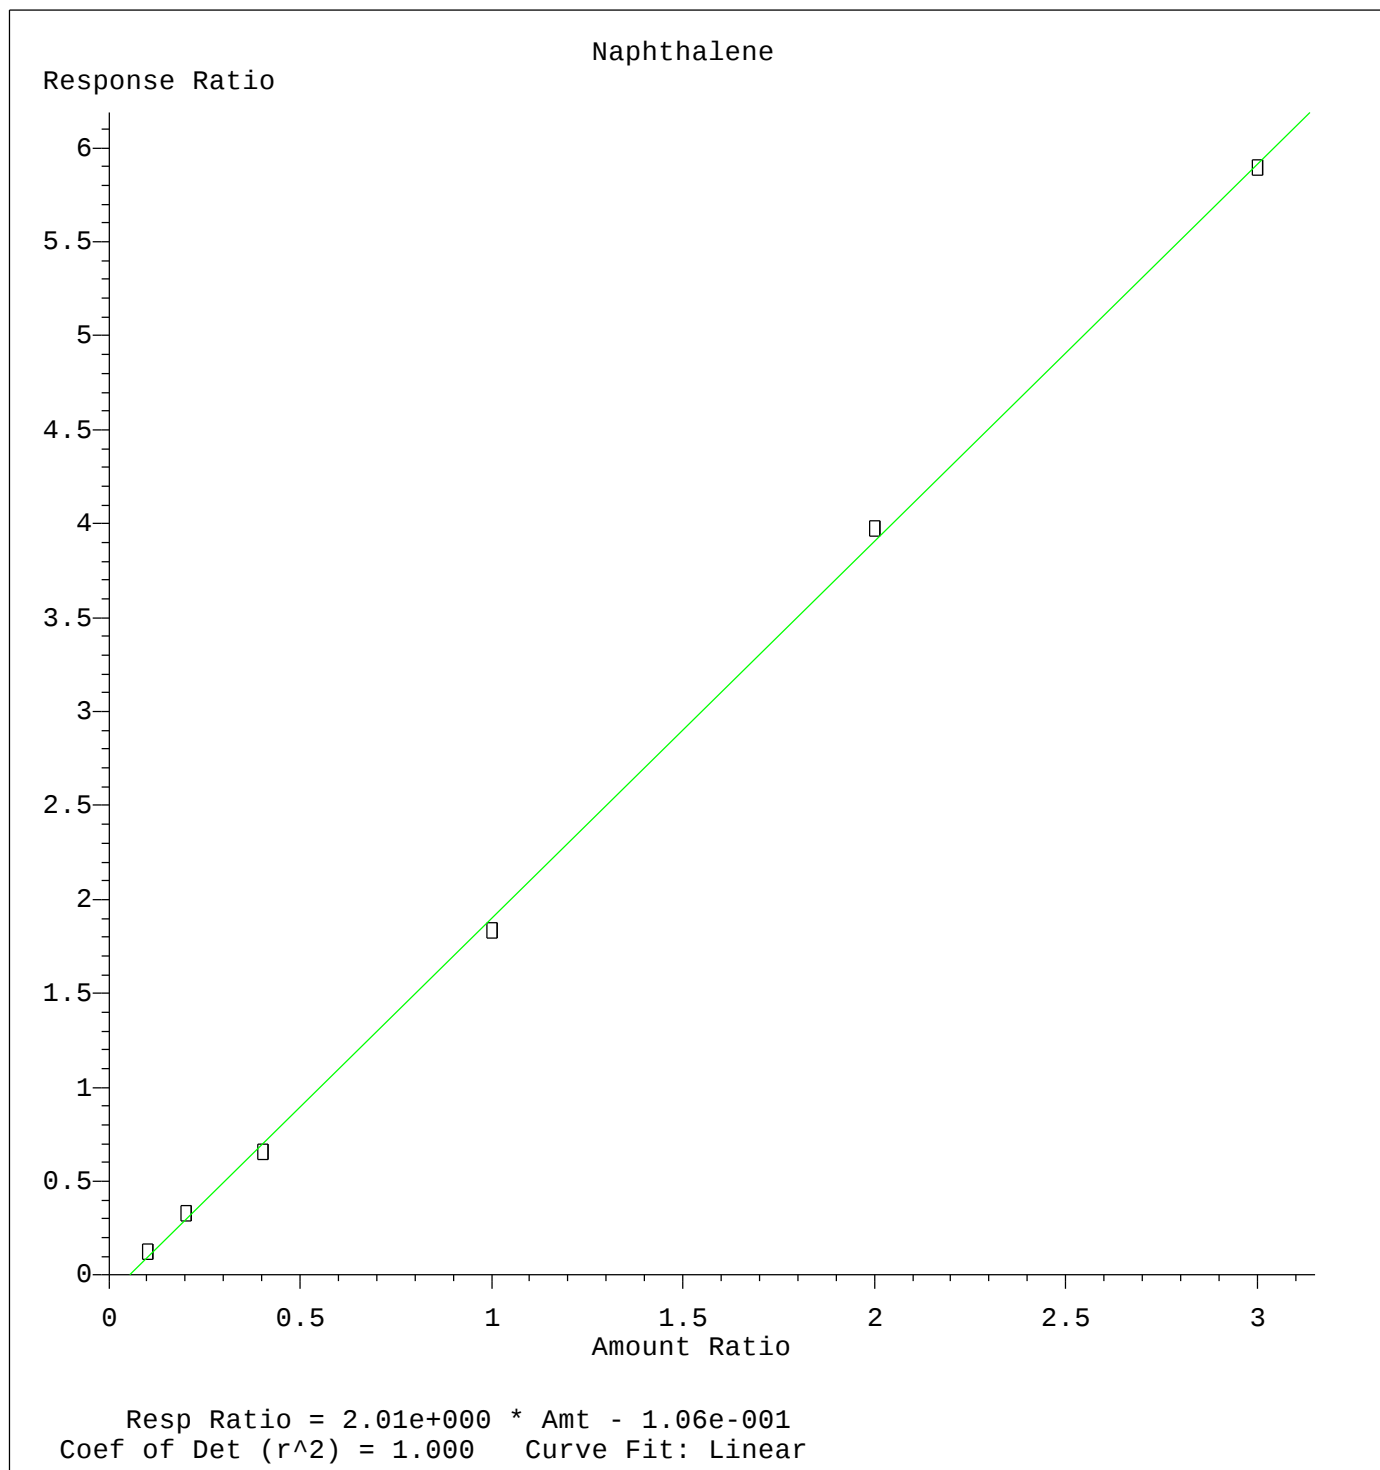


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041719S.M
Calibration Table Last Updated: Thu Apr 18 11:26:35 2019

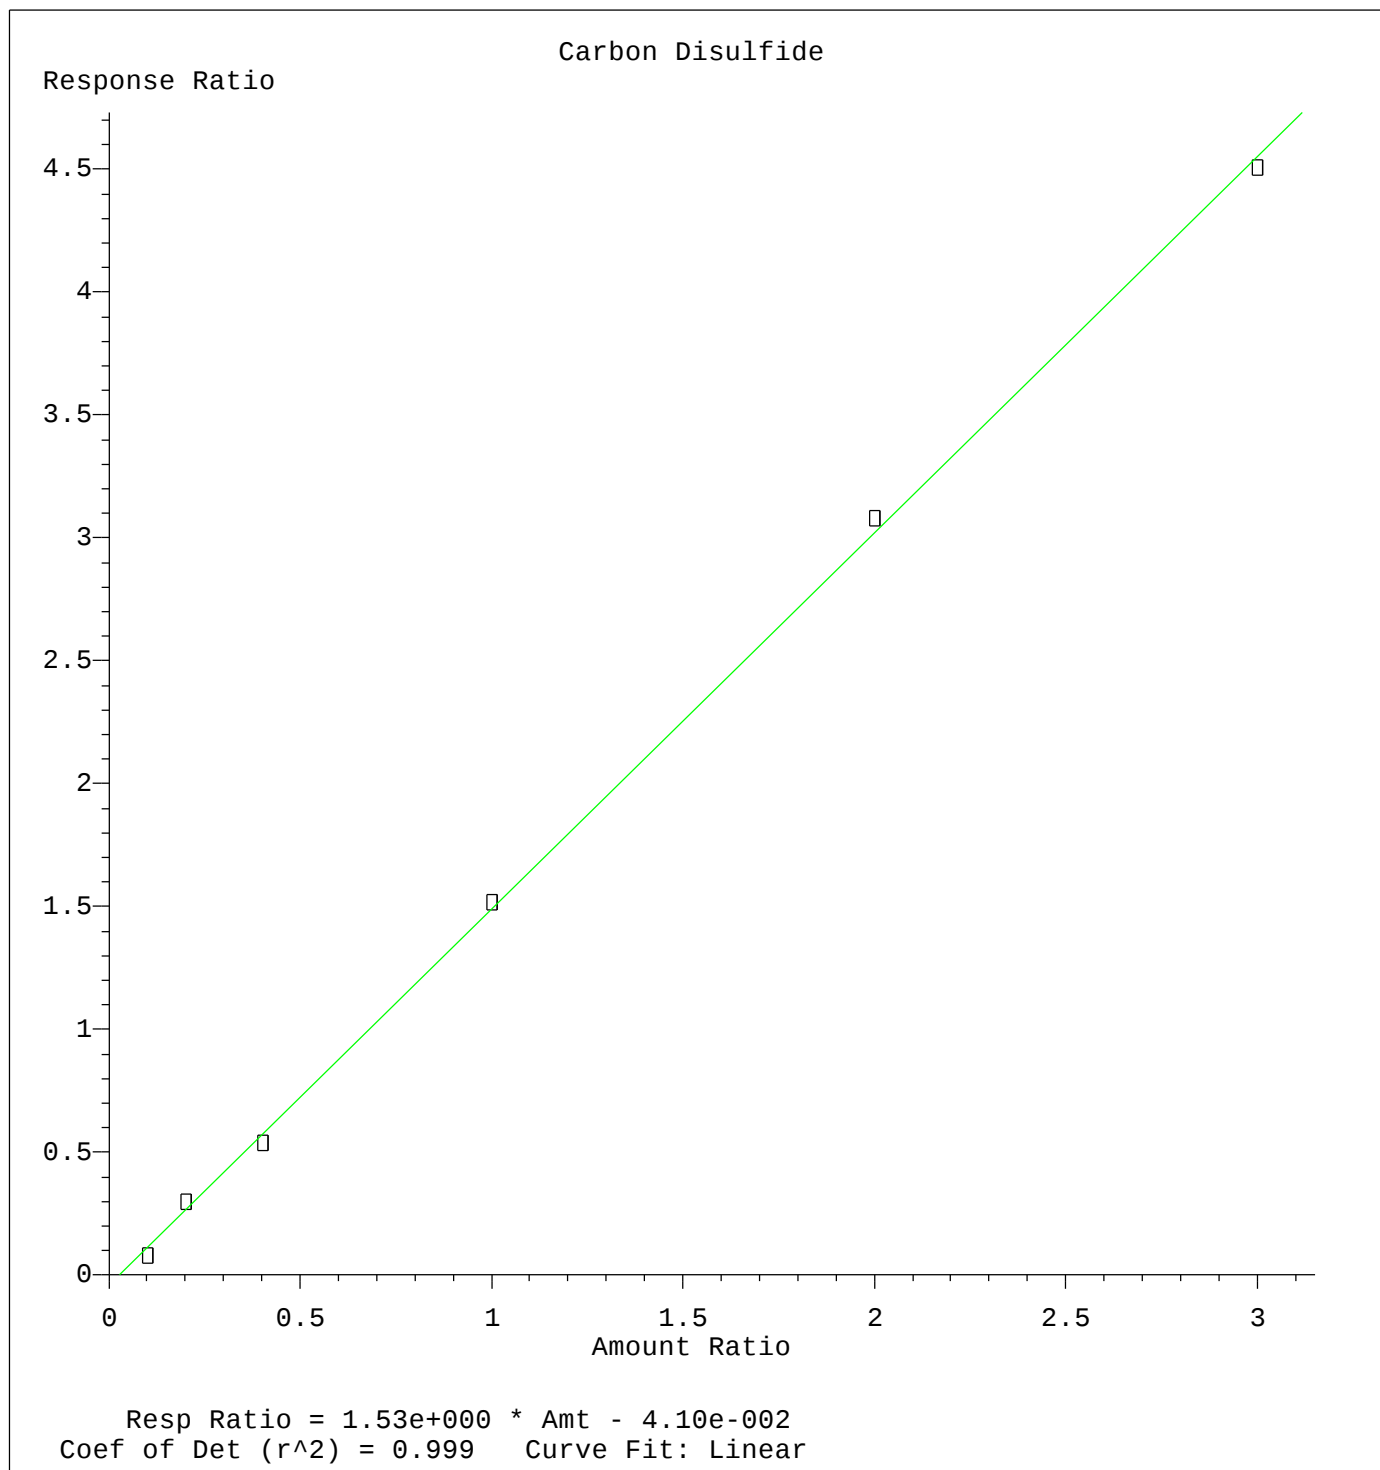

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041719S.M
Calibration Table Last Updated: Thu Apr 18 11:26:35 2019

Methylene Chloride

Response Ratio

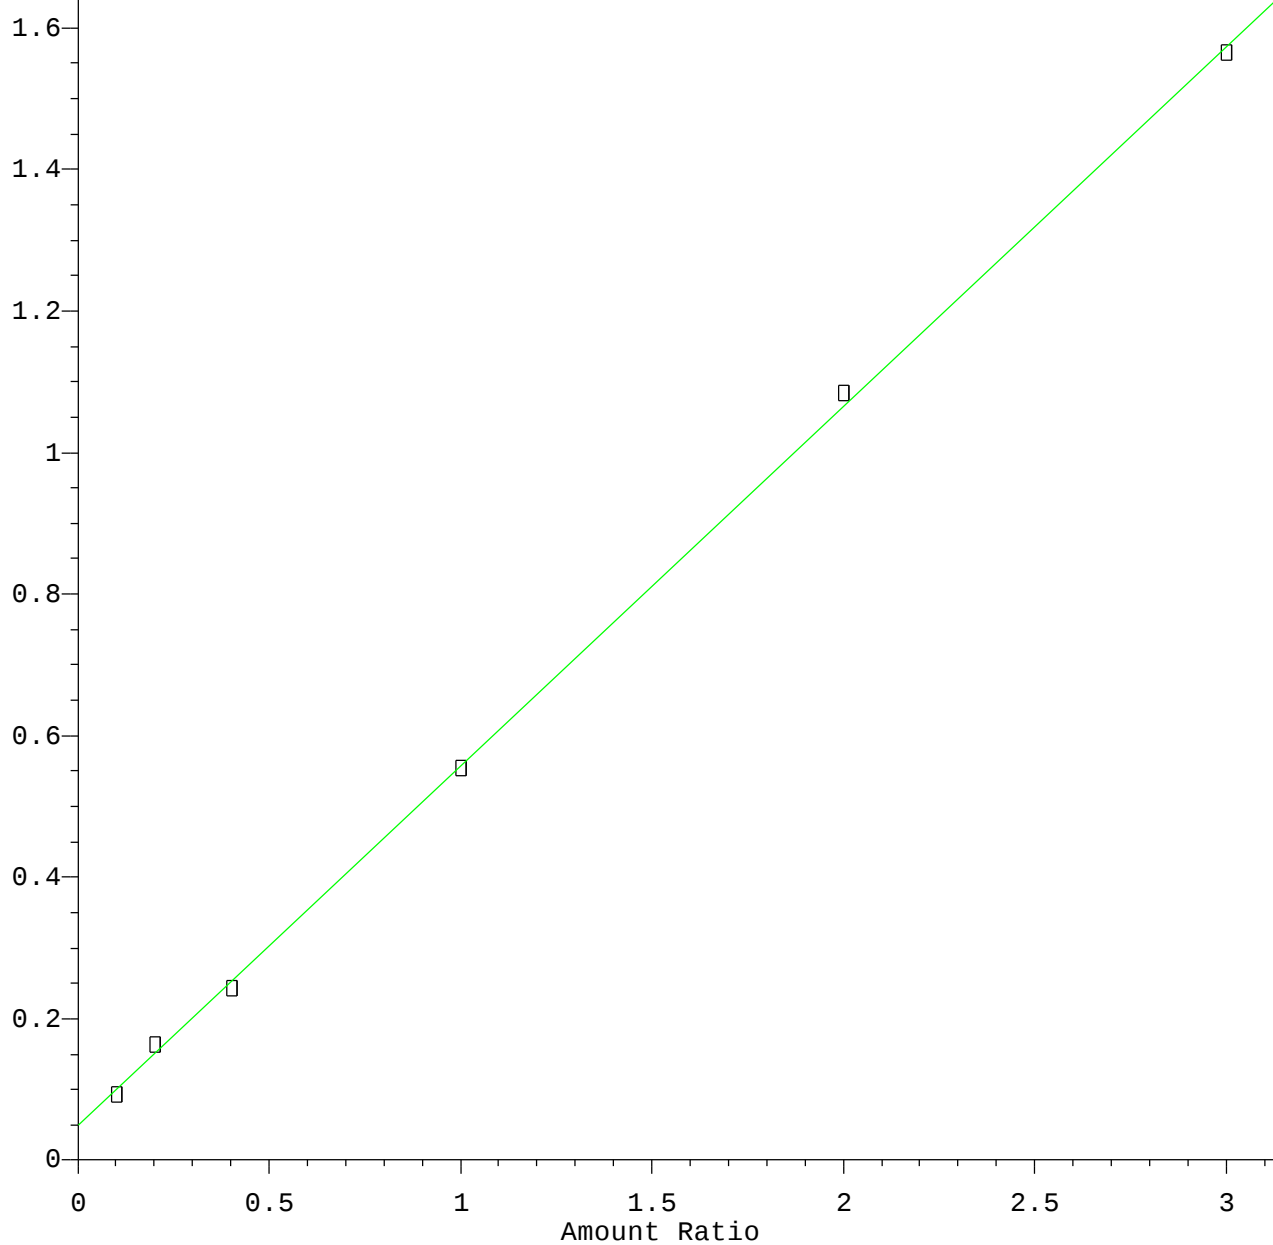

Resp Ratio = 5.09e-001 * Amt + 4.79e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041719S.M
Calibration Table Last Updated: Thu Apr 18 11:26:35 2019