


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW041819\
Data File : VW010037.D
Acq On : 18 Apr 2019 09:42
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W041719S.M
Title : SW846 8260
Last Update : Thu Apr 18 11:26:35 2019

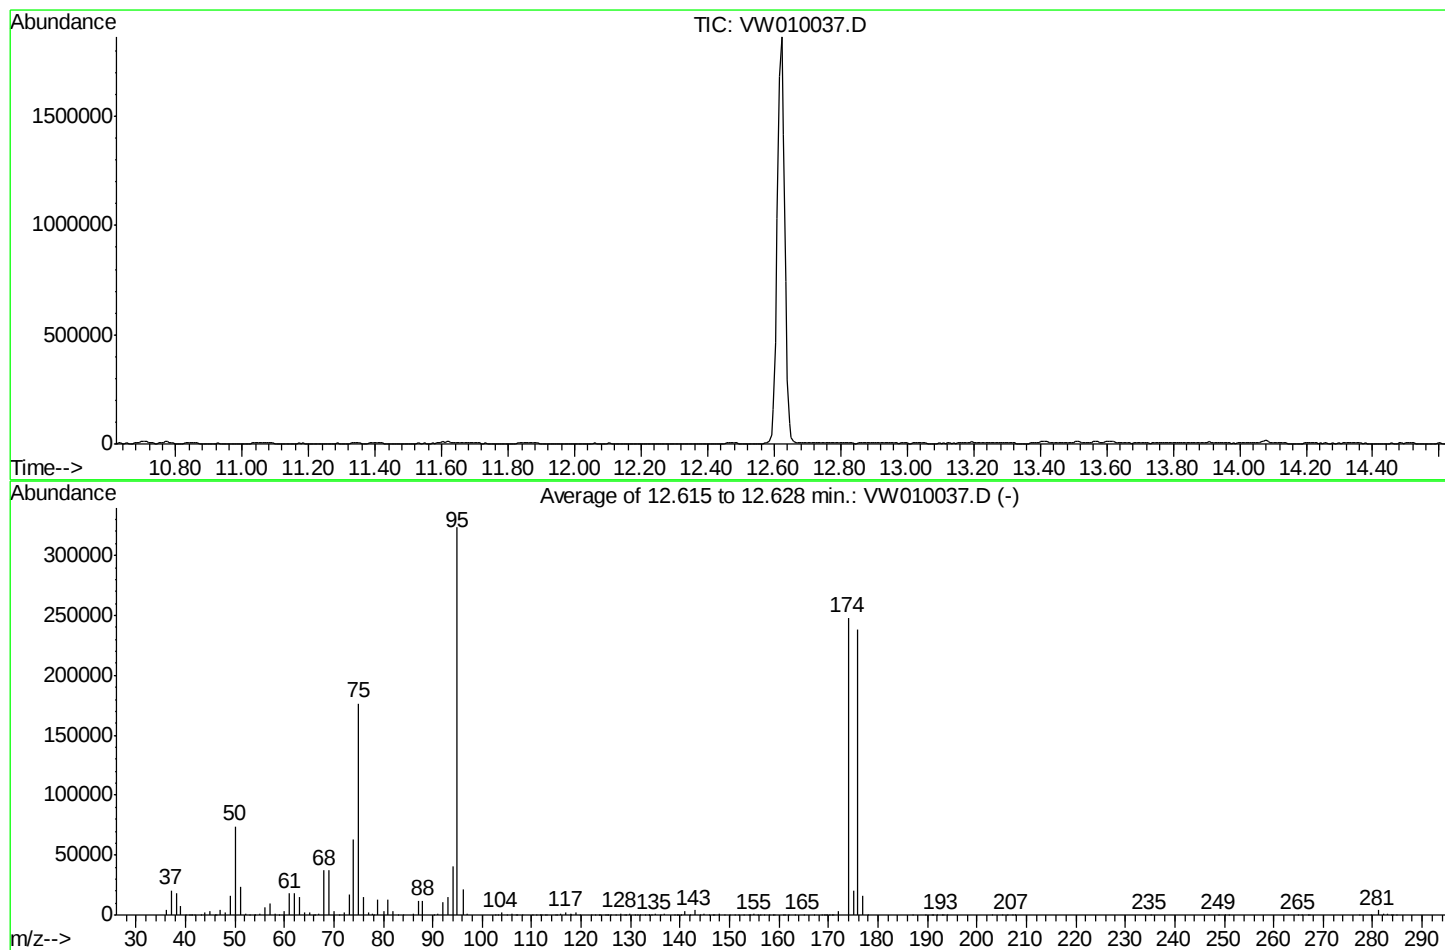

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	73762	PASS
75	95	30	60	54.6	176789	PASS
95	95	100	100	100.0	323520	PASS
96	95	5	9	6.7	21520	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.7	248128	PASS
175	174	5	9	8.2	20418	PASS
176	174	95	101	95.8	237781	PASS
177	176	5	9	6.8	16137	PASS