

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041823\
 Data File : VW025576.D
 Acq On : 18 Apr 2023 16:05
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK442

Quant Time: Apr 19 04:12:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 19 04:10:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	674604	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	614655	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	283932	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	207666	18.917	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.680%
7) Chloroethane-d5	2.899	69	160395	20.522	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.080%
11) 1,1-Dichloroethene-d2	4.027	63	340444	15.335	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.360%
21) 2-Butanone-d5	7.081	46	133137	54.364	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.720%
24) Chloroform-d	7.648	84	435185	22.975	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.920%
26) 1,2-Dichloroethane-d4	8.307	65	240559	24.412	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.640%
32) Benzene-d6	8.276	84	885892	22.259	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.040%
36) 1,2-Dichloropropane-d6	9.276	67	288274	23.230	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.920%
41) Toluene-d8	10.324	98	773081	22.237	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.960%
43) trans-1,3-Dichloroprop...	10.574	79	106410	22.871	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.480%
47) 2-Hexanone-d5	10.922	63	89662	52.860	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	212912	25.420	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.680%
66) 1,2-Dichlorobenzene-d4	13.854	152	238296	24.430	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.720%
Target Compounds					Qvalue	
13) Acetone	4.124	43	6345	3.061	ug/L	86
48) 2-Hexanone	10.922	43	12470	2.822	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041823\
Data File : VW025576.D
Acq On : 18 Apr 2023 16:05
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK442

Quant Time: Apr 19 04:12:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 19 04:10:43 2023
Response via : Initial Calibration




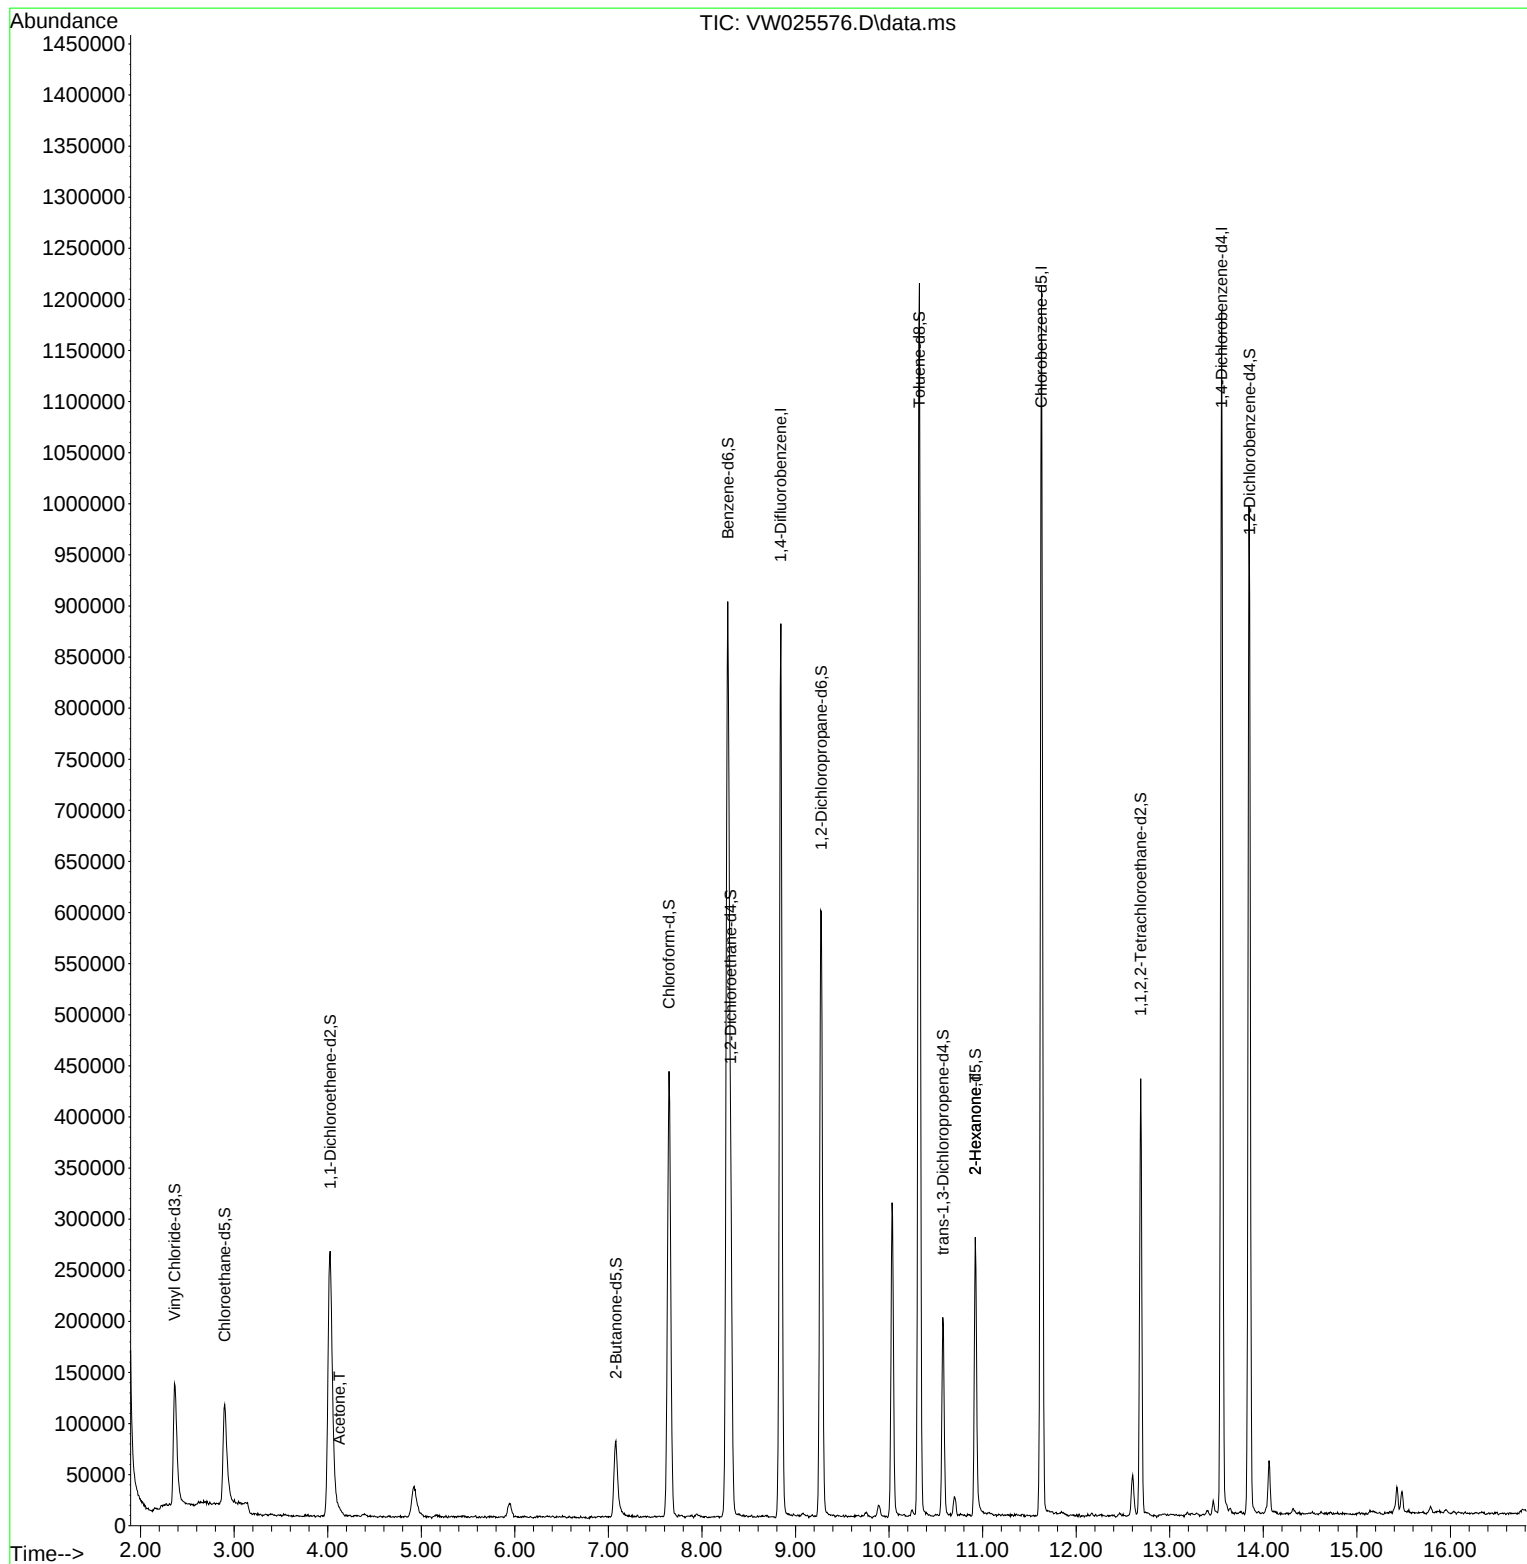


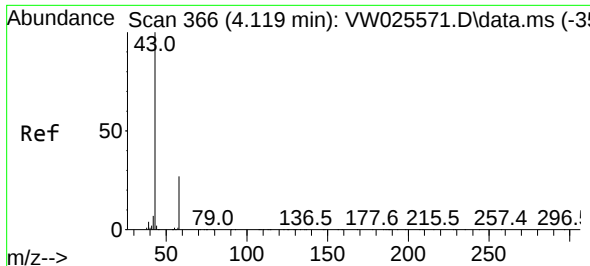

#13
Acetone
Concen: 3.061 ug/L
RT: 4.124 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW025576.D
Acq: 18 Apr 2023 16:05

Instrument :
MSVOA_W
ClientSampleId :
VIBLK442

Tgt Ion: 43 Resp: 6345
Ion Ratio Lower Upper
43 100
58 21.2 0.0 57.4

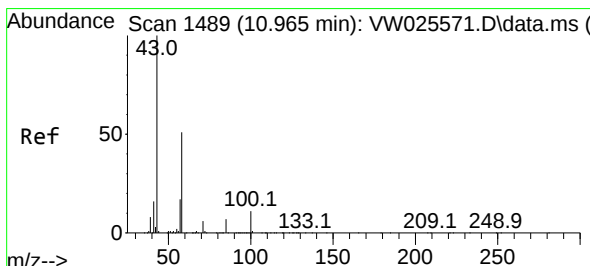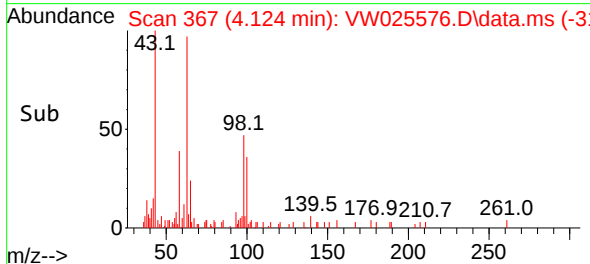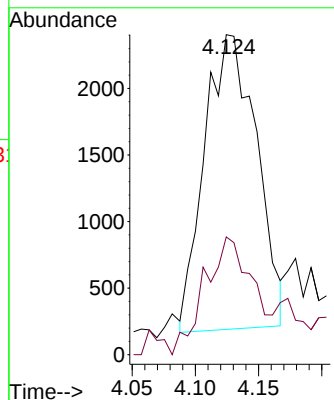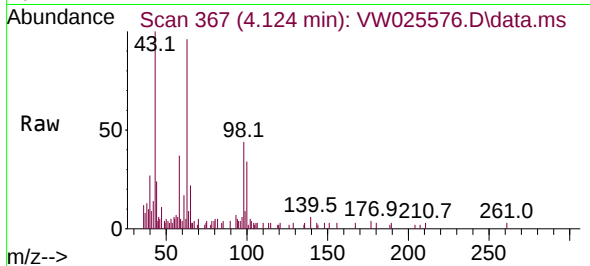

#48
2-Hexanone
Concen: 2.822 ug/L
RT: 10.922 min Scan# 1482
Delta R.T. -0.043 min
Lab File: VW025576.D
Acq: 18 Apr 2023 16:05

Tgt Ion: 43 Resp: 12470
Ion Ratio Lower Upper
43 100
58 25.9 38.6 57.8#
57 30.5 13.9 20.9#
100 1.6 8.2 12.2#

