

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041922\
 Data File : VW022573.D
 Acq On : 19 Apr 2022 10:33
 Operator : SY/VA
 Sample : VW0419SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK482

Quant Time: Apr 20 01:26:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 20 01:25:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	356355	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	336292	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	177308	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	165996	21.071	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.280%		
7) Chloroethane-d5	2.885	69	100723	20.401	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.600%		
11) 1,1-Dichloroethene-d2	4.013	63	190265	18.621	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.480%		
21) 2-Butanone-d5	7.080	46	60797	44.204	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.400%		
24) Chloroform-d	7.647	84	257315	23.102	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.400%		
26) 1,2-Dichloroethane-d4	8.305	65	144617	22.724	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.880%		
32) Benzene-d6	8.275	84	514299	25.031	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	100.120%		
36) 1,2-Dichloropropane-d6	9.268	67	143204	24.085	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.320%		
41) Toluene-d8	10.323	98	496969	24.697	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.800%		
43) trans-1,3-Dichloroprop...	10.579	79	60852	21.686	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.760%		
47) 2-Hexanone-d5	10.921	63	50379	45.541	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.080%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	118022	23.345	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.360%		
66) 1,2-Dichlorobenzene-d4	13.853	152	155598	24.776	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.120%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	5931	0.683	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041922\
Data File : VW022573.D
Acq On : 19 Apr 2022 10:33
Operator : SY/VA
Sample : VW0419SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK482

Quant Time: Apr 20 01:26:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 20 01:25:38 2022
Response via : Initial Calibration

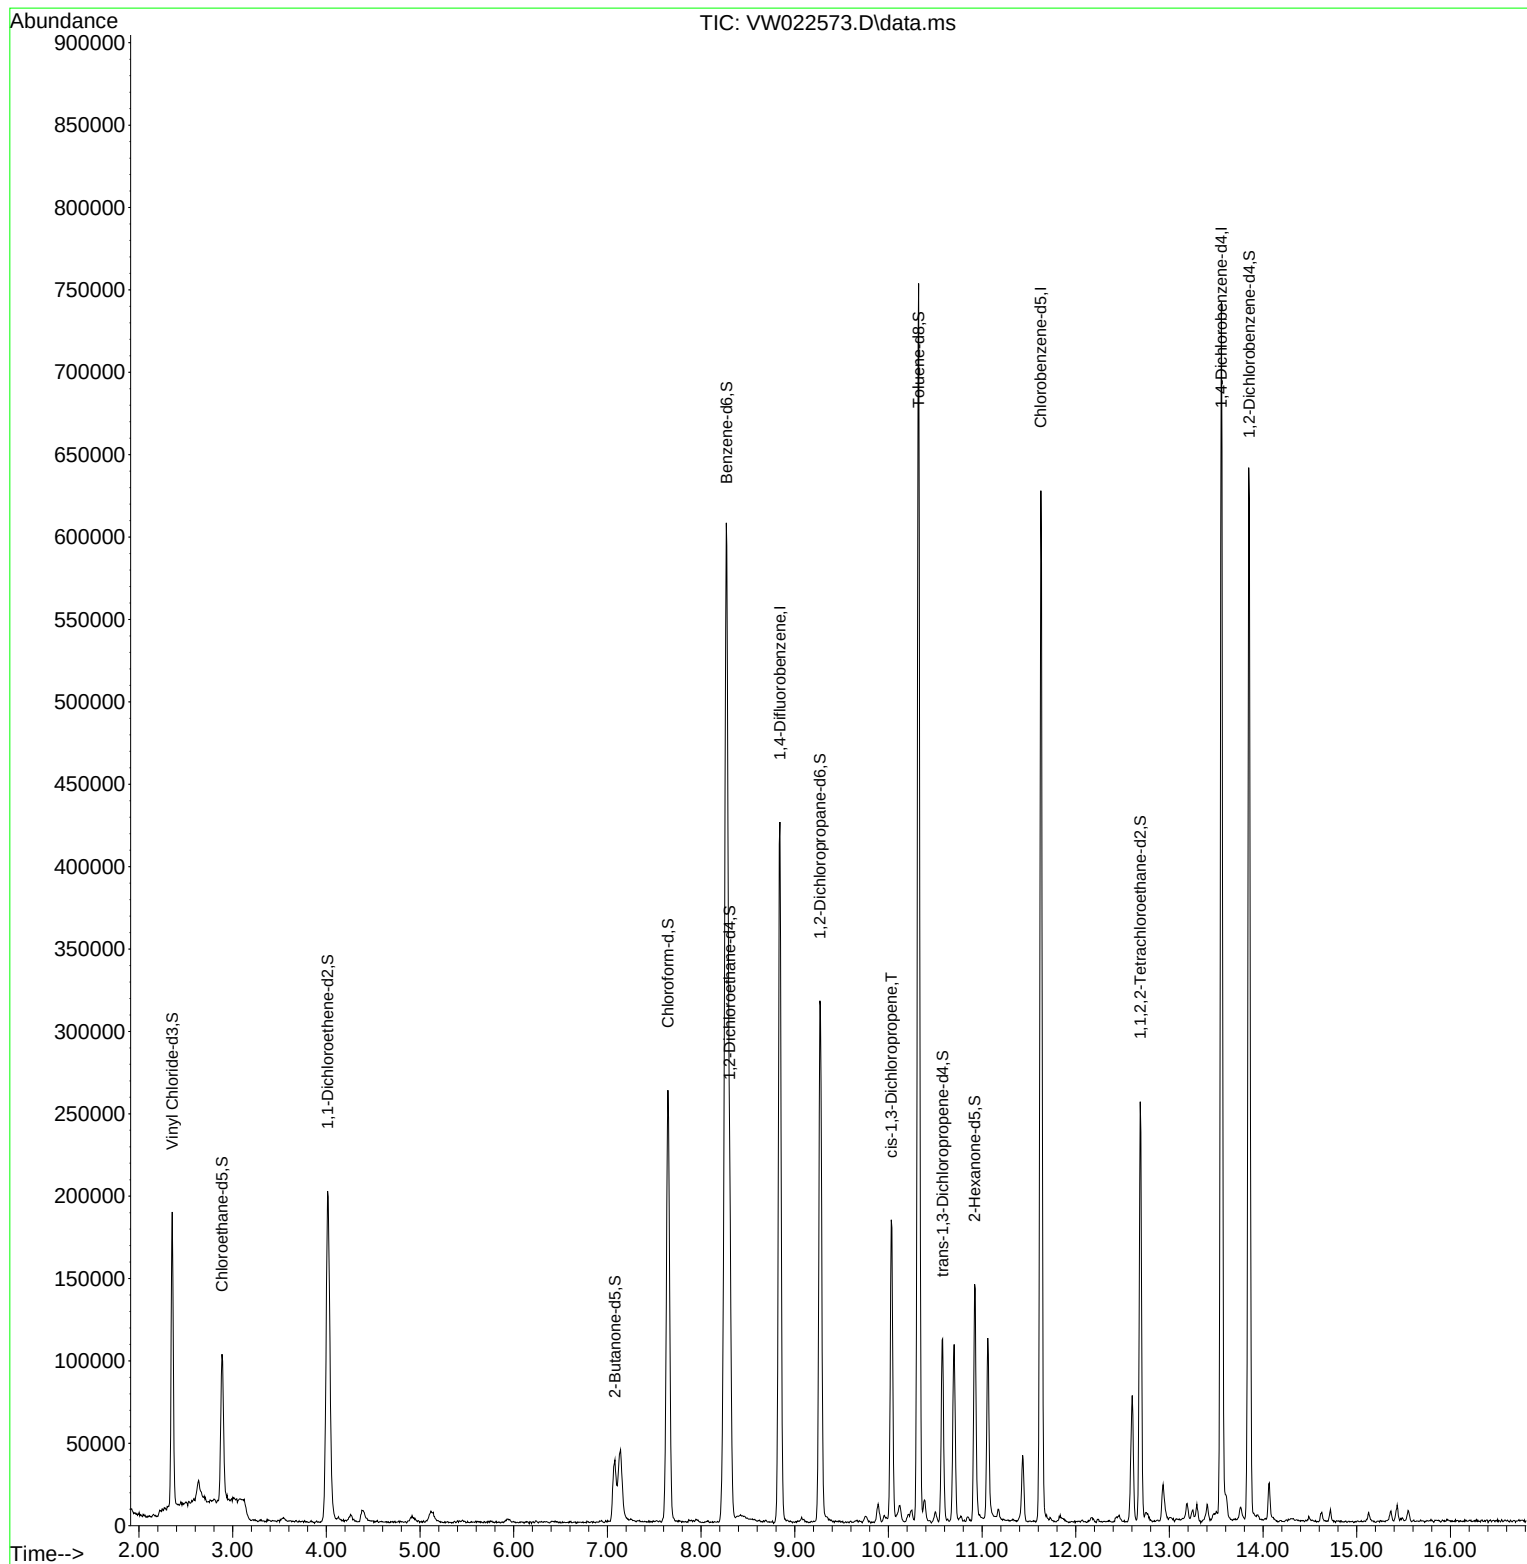

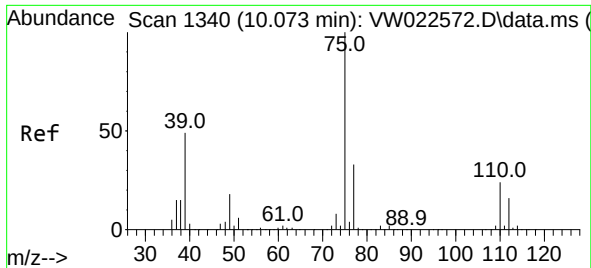

#39

cis-1,3-Dichloropropene

Concen: 0.683 ug/L

RT: 10.030 min Scan# 11

Delta R.T. -0.042 min

Lab File: VW022573.D

Acq: 19 Apr 2022 10:33

Instrument :

MSVOA_W

ClientSampleId :

VBLK482

Tgt Ion: 75 Resp: 5931

Ion Ratio Lower Upper

75 100

77 45.9 22.6 42.0#

