

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041922\
 Data File : VW022574.D
 Acq On : 19 Apr 2022 11:21
 Operator : SY/VA
 Sample : N2373-06
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Apr 20 01:26:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 20 01:25:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	315276	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	309118	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159656	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	154009	22.097	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.400%
7) Chloroethane-d5	2.891	69	97344	22.285	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.160%
11) 1,1-Dichloroethene-d2	4.019	63	168781	18.670	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.680%
21) 2-Butanone-d5	7.080	46	53458	43.932	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.860%
24) Chloroform-d	7.653	84	231972	23.540	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.160%
26) 1,2-Dichloroethane-d4	8.305	65	130637	23.202	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	8.274	84	476683	25.240	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.960%
36) 1,2-Dichloropropane-d6	9.274	67	132678	24.276	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.120%
41) Toluene-d8	10.323	98	452183	24.447	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.800%
43) trans-1,3-Dichloroprop...	10.579	79	52468	20.342	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.360%
47) 2-Hexanone-d5	10.920	63	42389	41.687	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.380%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	105210	22.640	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	142158	25.138	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.560%
Target Compounds					Qvalue	
13) Acetone	4.129	43	3712	4.480	ug/L	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041922\
Data File : VW022574.D
Acq On : 19 Apr 2022 11:21
Operator : SY/VA
Sample : N2373-06
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Apr 20 01:26:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 20 01:25:38 2022
Response via : Initial Calibration

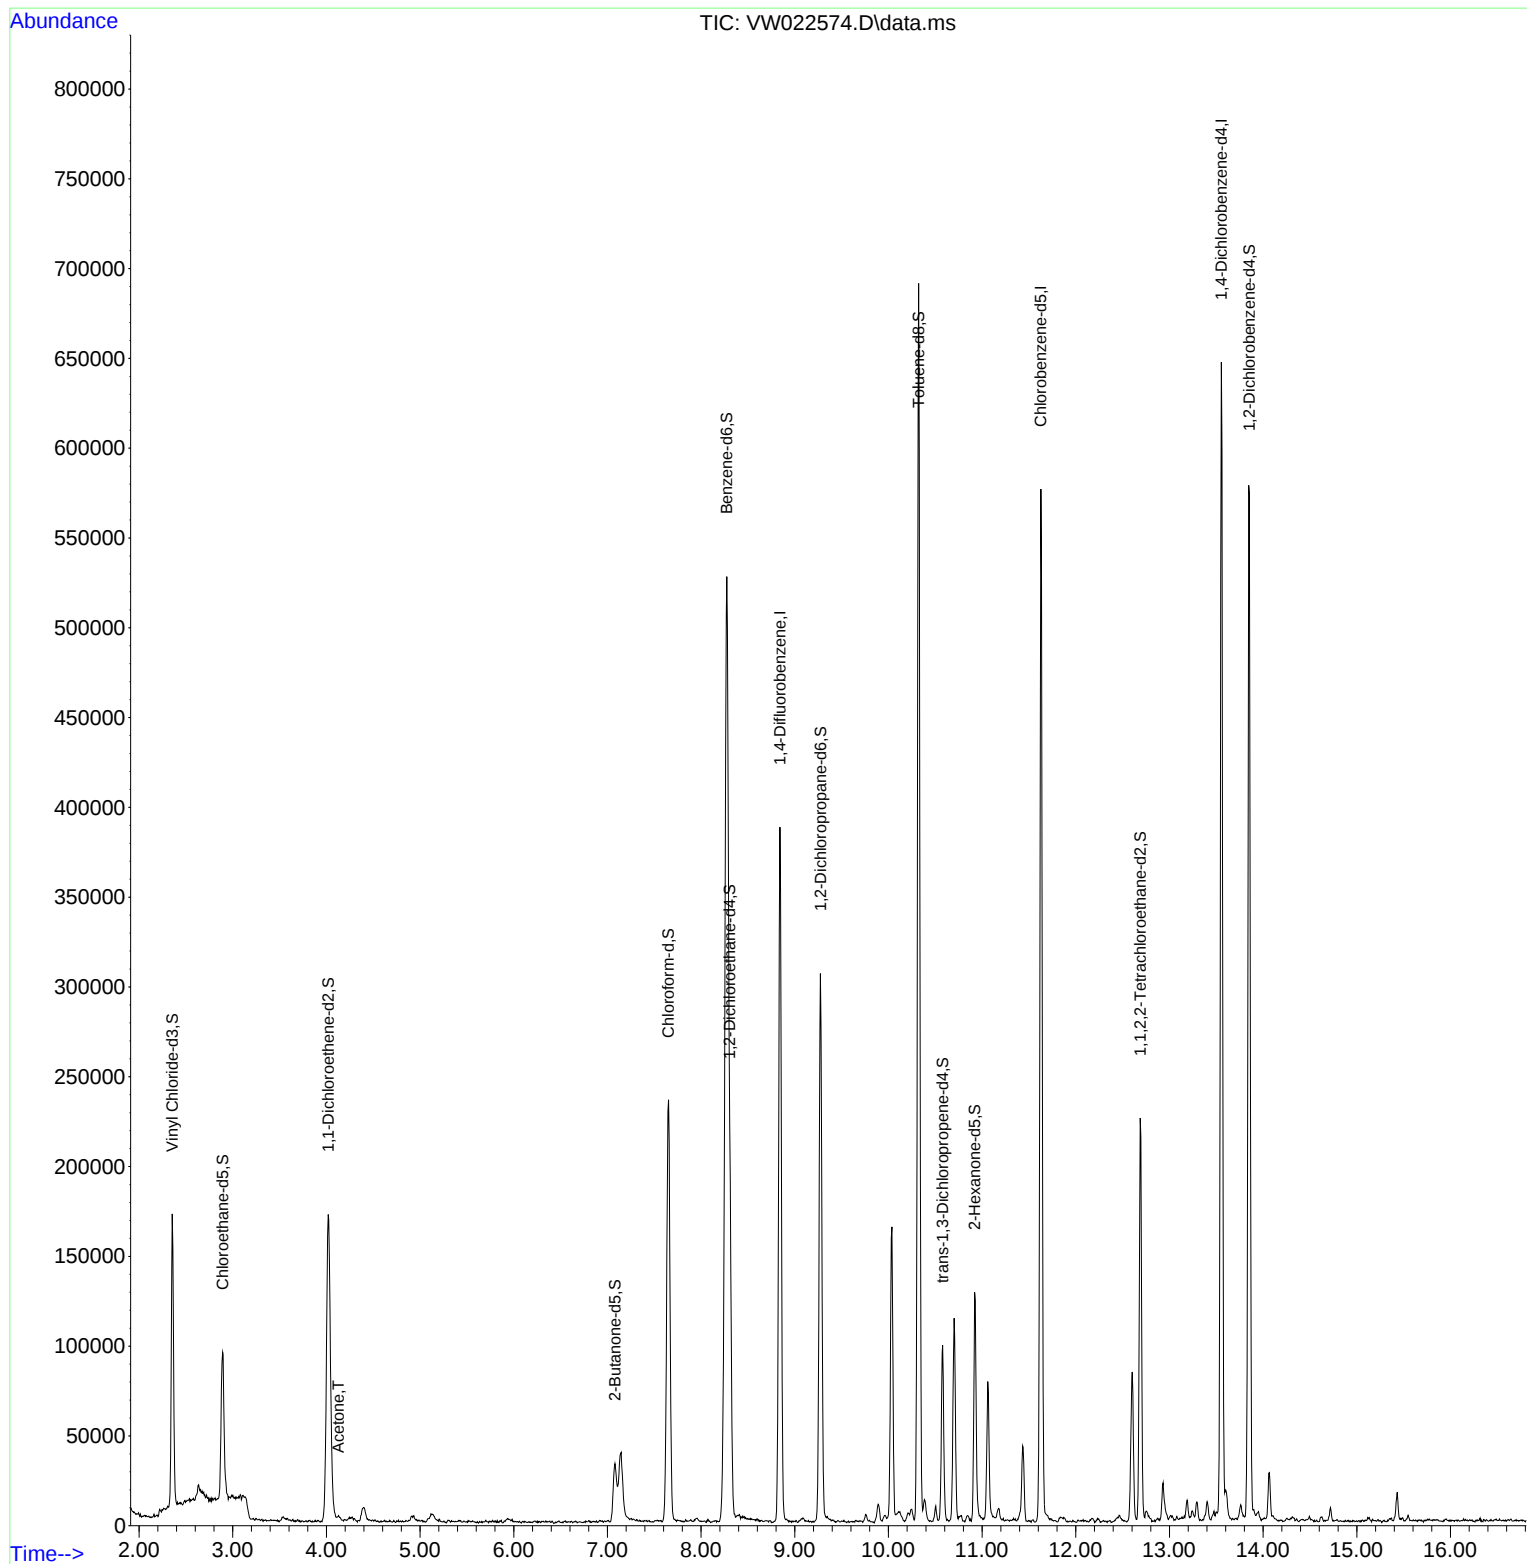

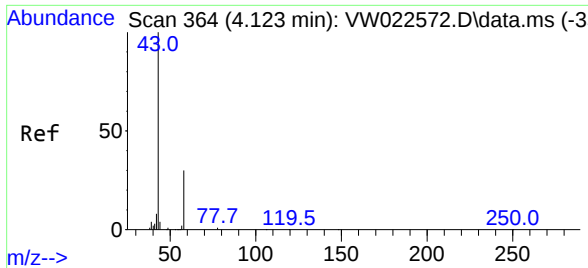

#13
 Acetone
 Concen: 4.480 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022574.D
 Acq: 19 Apr 2022 11:21

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Tgt Ion: 43 Resp: 3712
 Ion Ratio Lower Upper
 43 100
 58 5.7 0.0 57.0

