

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041922\
 Data File : VW022576.D
 Acq On : 19 Apr 2022 13:04
 Operator : SY/VA
 Sample : N2469-01
 Misc : 5.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFF8

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/20/2022
 Supervised By : Mahesh Dadoda 04/22/2022

Quant Time: Apr 20 01:26:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 20 01:25:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	317336	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	256679	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	89708	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	87081	12.413	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	49.640%		
7) Chloroethane-d5	2.892	69	60769	13.822	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	55.280%		
11) 1,1-Dichloroethene-d2	4.019	63	99293m	10.912	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	43.640%#		
21) 2-Butanone-d5	7.080	46	56358	46.015	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.020%		
24) Chloroform-d	7.647	84	188898	19.044	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	76.160%		
26) 1,2-Dichloroethane-d4	8.305	65	112576m	19.864	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	79.440%		
32) Benzene-d6	8.275	84	321027	20.471	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	81.880%		
36) 1,2-Dichloropropane-d6	9.275	67	103295	22.761	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.040%		
41) Toluene-d8	10.323	98	260499	16.961	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	67.840%		
43) trans-1,3-Dichloroprop...	10.579	79	38056	17.768	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.080%		
47) 2-Hexanone-d5	10.921	63	43137	51.089	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.180%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	89043	23.075	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	92.320%		
66) 1,2-Dichlorobenzene-d4	13.847	152	61148	19.244	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	76.960%		
Target Compounds					Qvalue	
13) Acetone	4.117	43	7165	8.592	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041922\
Data File : VW022576.D
Acq On : 19 Apr 2022 13:04
Operator : SY/VA
Sample : N2469-01
Misc : 5.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFF8

Quant Time: Apr 20 01:26:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 20 01:25:38 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/20/2022
Supervised By :Mahesh Dadoda 04/22/2022

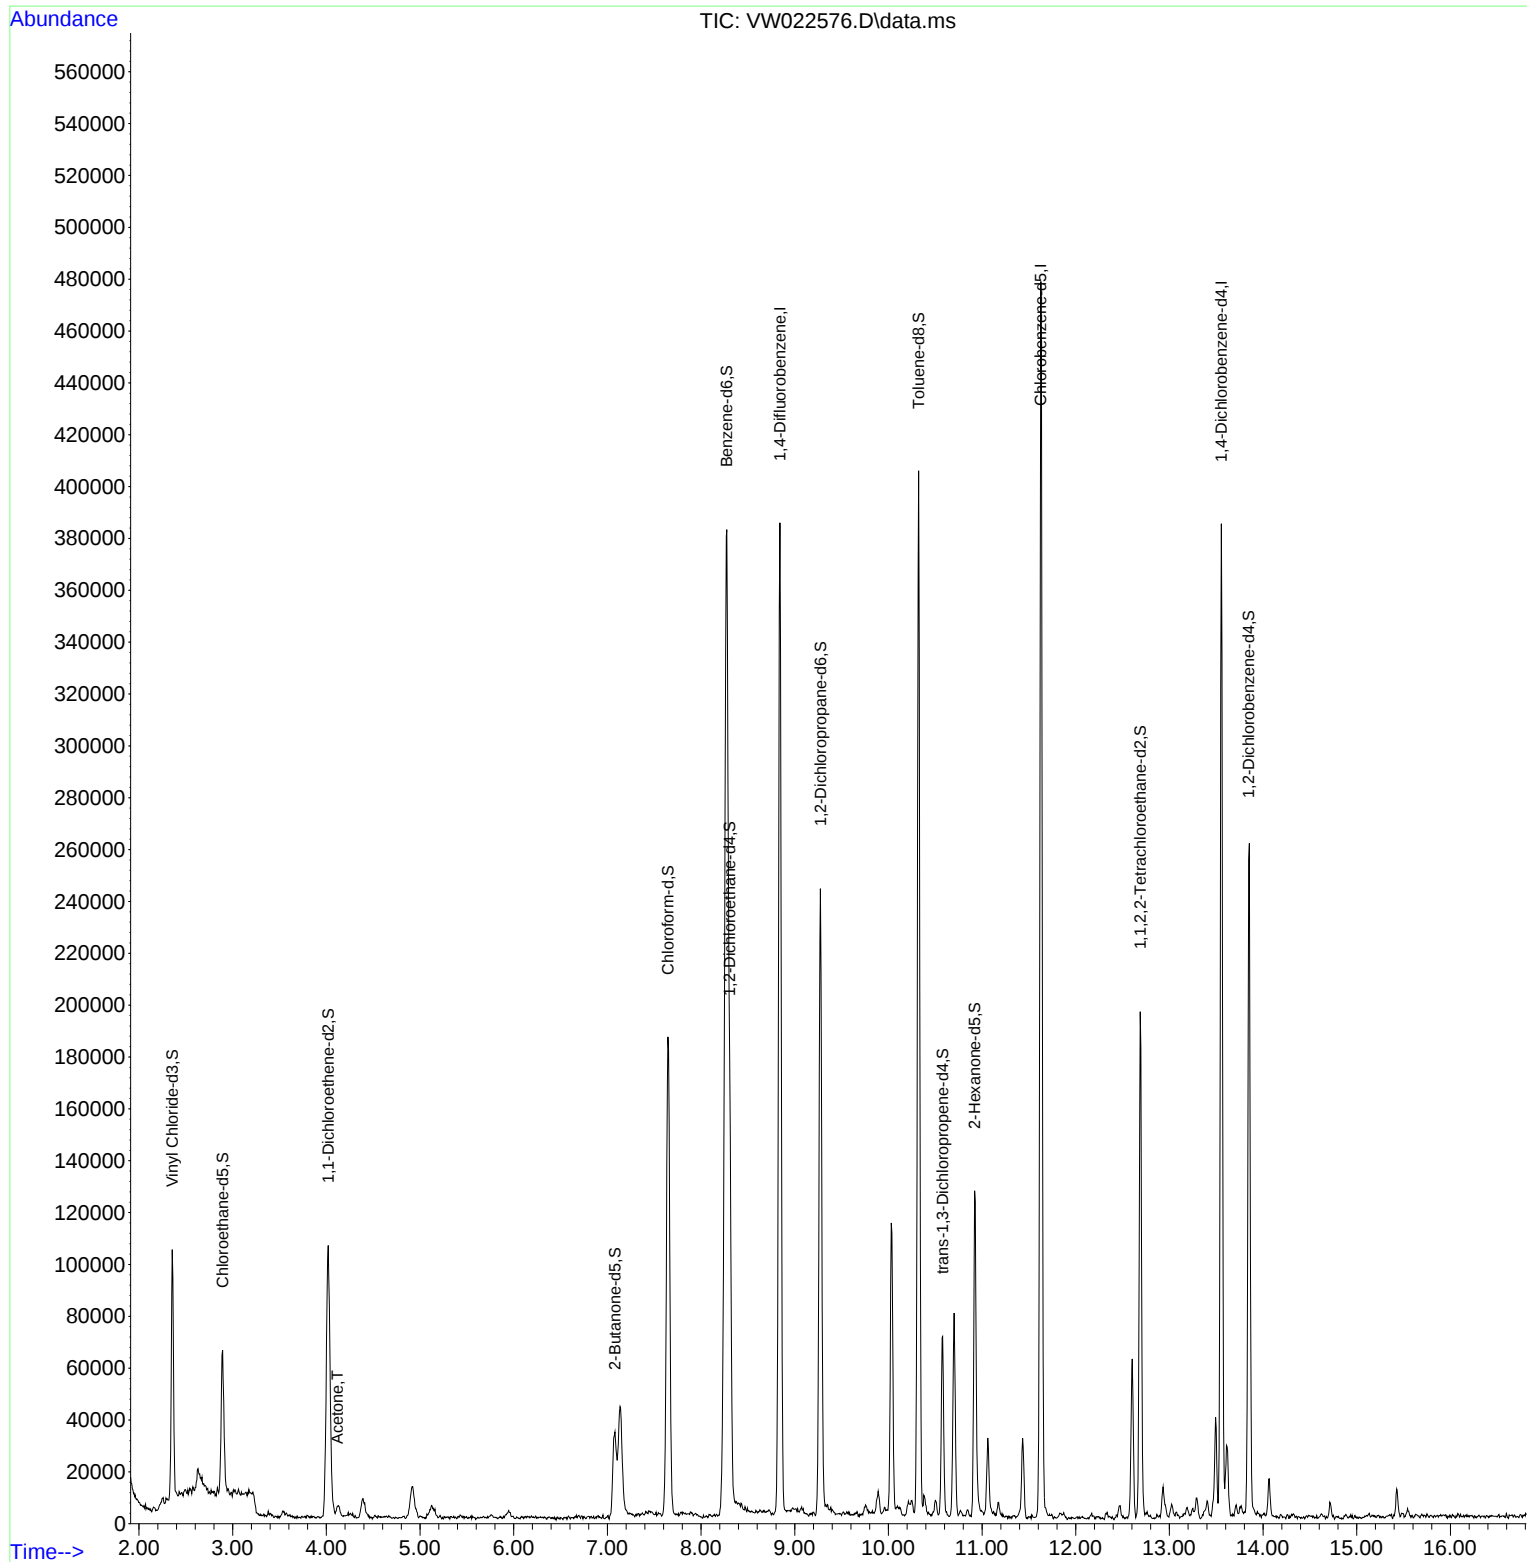

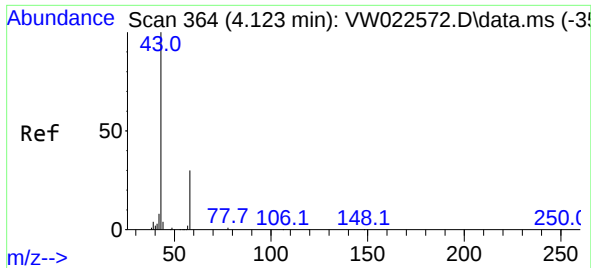

#13
 Acetone
 Concen: 8.592 ug/L
 RT: 4.117 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022576.D
 Acq: 19 Apr 2022 13:04

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFF8

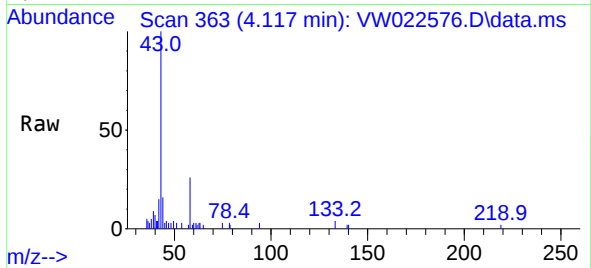

Tgt Ion: 43 Resp: 716
 Ion Ratio Lower Upper
 43 100
 58 27.6 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/20/2022
 Supervised By :Mahesh Dadoda 04/22/2022

