

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042021\
Data File : VW018686.D
Acq On : 20 Apr 2021 13:12
Operator : SY/VA
Sample : M2065-07
Misc : 5.45G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG560

Manual Integrations
APPROVED

MMDadoda
4/21/2021 4:51:29 PM

Quant Time: Apr 21 01:27:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 21 01:26:40 2021
Response via : Initial Calibration

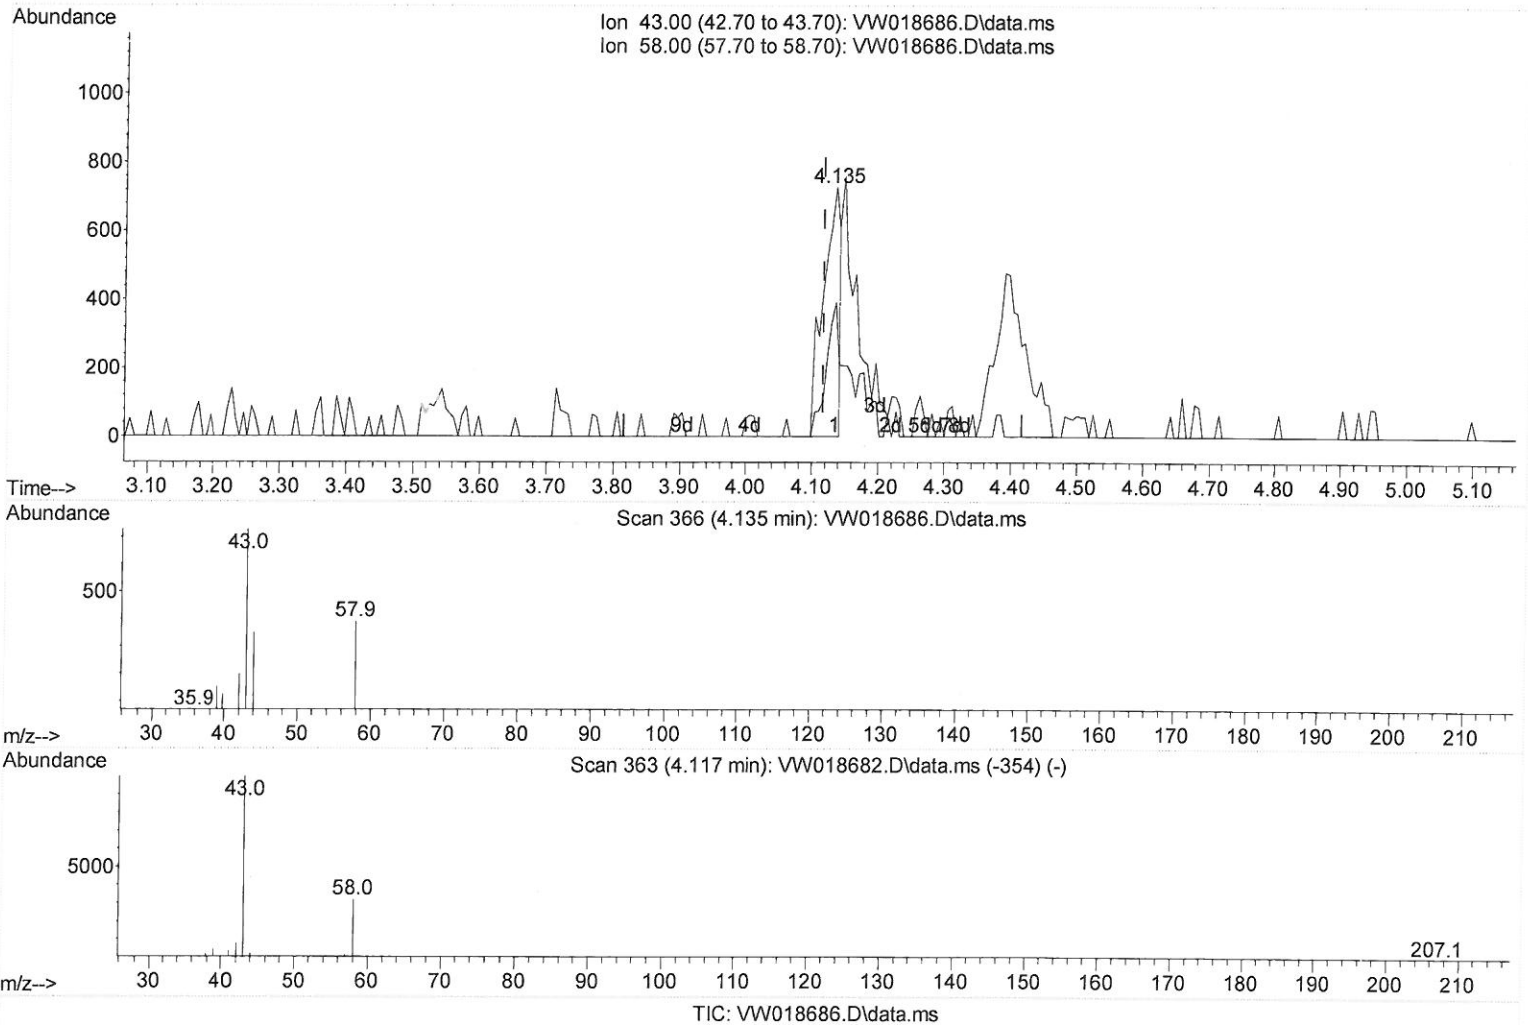

(13) Acetone (T)

4.135min (+ 0.018) 9.98 ug/L

response 1303

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	45.66
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042021\
 Data File : VW018686.D
 Acq On : 20 Apr 2021 13:12
 Operator : SY/VA
 Sample : M2065-07
 Misc : 5.45G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG560

Manual Integrations
 APPROVED

MMDadoda
 4/21/2021 4:51:29 PM

Quant Time: Apr 21 01:27:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 21 01:26:40 2021
 Response via : Initial Calibration

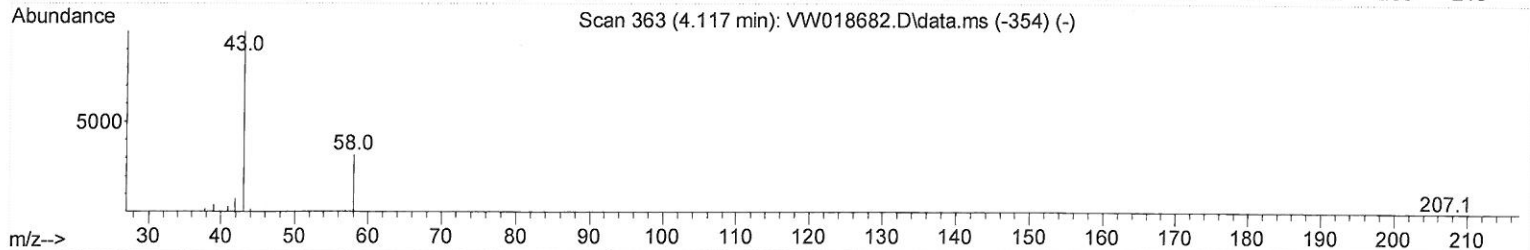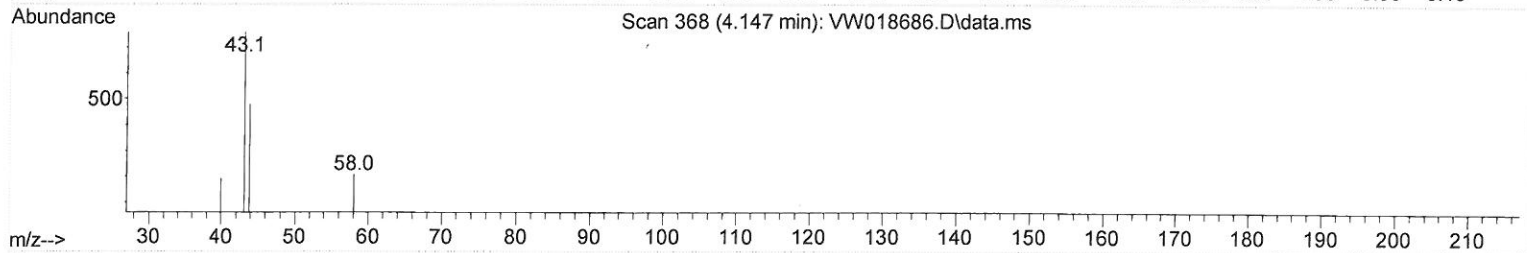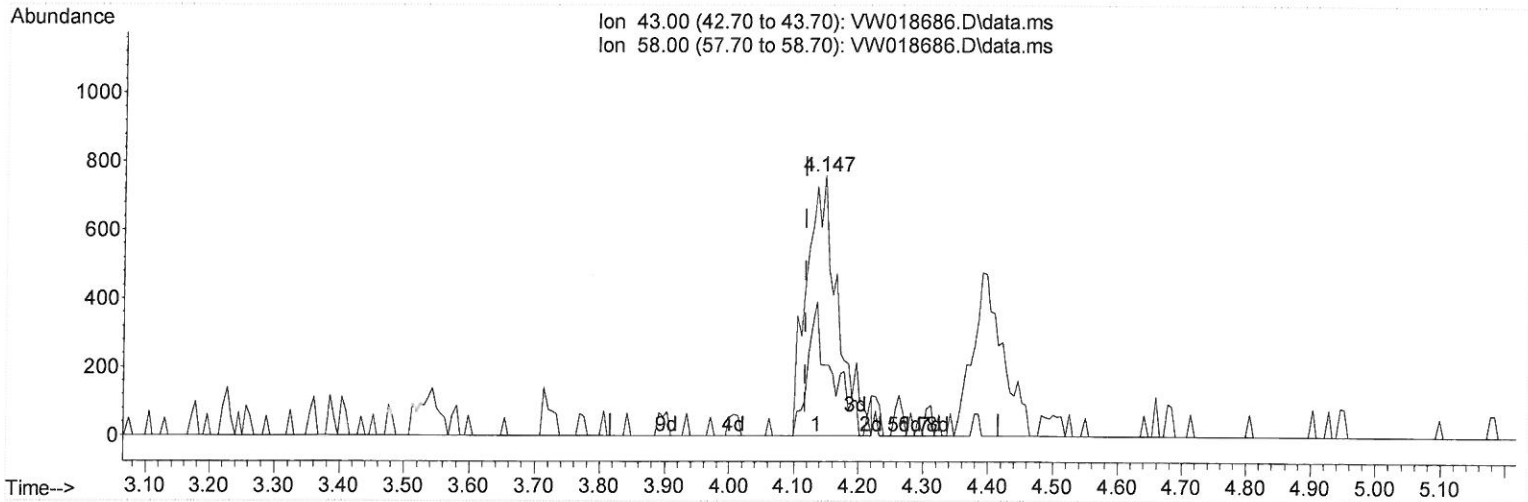

TIC: VW018686.D\data.ms

(13) Acetone (T)

4.147min (+ 0.030) 19.72 ug/L m

04/22/21 Sy

response 2576

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	23.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042021\
 Data File : VW018686.D
 Acq On : 20 Apr 2021 13:12
 Operator : SY/VA
 Sample : M2065-07
 Misc : 5.45G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG560

Manual Integrations
 APPROVED

MMDadoda
 4/21/2021 4:51:29 PM

Quant Time: Apr 21 01:27:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 21 01:26:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	52018	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	47721	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	20017	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	12658	16.01	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.04%
7) Chloroethane-d5	2.891	69	13102	18.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.80%
11) 1,1-Dichloroethene-d2	4.025	63	15883	11.57	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.28%
21) 2-Butanone-d5	7.092	46	9058	50.34	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.68%
24) Chloroform-d	7.652	84	30722	21.52	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.08%
26) 1,2-Dichloroethane-d4	8.311	65	19113	23.81	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.24%
32) Benzene-d6	8.280	84	49351	17.63	ug/L	0.01
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.52%
36) 1,2-Dichloropropane-d6	9.280	67	18718	22.19	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.76%
41) Toluene-d8	10.329	98	38244	14.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	59.76%
43) trans-1,3-Dichloroprop...	10.585	79	6450	17.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.84%
47) 2-Hexanone-d5	10.926	63	7041	48.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.00%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	18289	25.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.84%
66) 1,2-Dichlorobenzene-d4	13.852	152	16351	23.25	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.00%
Target Compounds						
13) Acetone	4.147	43	2576m	19.72	ug/L	Qvalue
16) Methylene chloride	4.921	84	4715	5.53	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042021\
Data File : VW018686.D
Acq On : 20 Apr 2021 13:12
Operator : SY/VA
Sample : M2065-07
Misc : 5.45G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG560

Manual Integrations
APPROVED

MMDadoda
4/21/2021 4:51:29 PM

Quant Time: Apr 21 01:27:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 21 01:26:40 2021
Response via : Initial Calibration

