

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042021\
 Data File : VW018686.D
 Acq On : 20 Apr 2021 13:12
 Operator : SY/VA
 Sample : M2065-07
 Misc : 5.45G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG560

Manual Integrations
 APPROVED

MMDadoda
 4/21/2021 4:51:29 PM

Quant Time: Apr 21 01:27:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 21 01:26:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	52018	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	47721	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	20017	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	12658	16.01	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.04%		
7) Chloroethane-d5	2.891	69	13102	18.70	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.80%		
11) 1,1-Dichloroethene-d2	4.025	63	15883	11.57	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.28%		
21) 2-Butanone-d5	7.092	46	9058	50.34	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.68%		
24) Chloroform-d	7.652	84	30722	21.52	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.08%		
26) 1,2-Dichloroethane-d4	8.311	65	19113	23.81	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.24%		
32) Benzene-d6	8.280	84	49351	17.63	ug/L	0.01
Spiked Amount 25.000	Range 20 - 135		Recovery =	70.52%		
36) 1,2-Dichloropropane-d6	9.280	67	18718	22.19	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.76%		
41) Toluene-d8	10.329	98	38244	14.94	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	59.76%		
43) trans-1,3-Dichloroprop...	10.585	79	6450	17.96	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.84%		
47) 2-Hexanone-d5	10.926	63	7041	48.00	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.00%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	18289	25.96	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.84%		
66) 1,2-Dichlorobenzene-d4	13.852	152	16351	23.25	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	93.00%		
Target Compounds						Qvalue
13) Acetone	4.147	43	2576m	19.72	ug/L	
16) Methylene chloride	4.921	84	4715	5.53	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042021\
Data File : VW018686.D
Acq On : 20 Apr 2021 13:12
Operator : SY/VA
Sample : M2065-07
Misc : 5.45G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG560

Manual Integrations
APPROVED

MMDadoda
4/21/2021 4:51:29 PM


Quant Time: Apr 21 01:27:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 21 01:26:40 2021
Response via : Initial Calibration

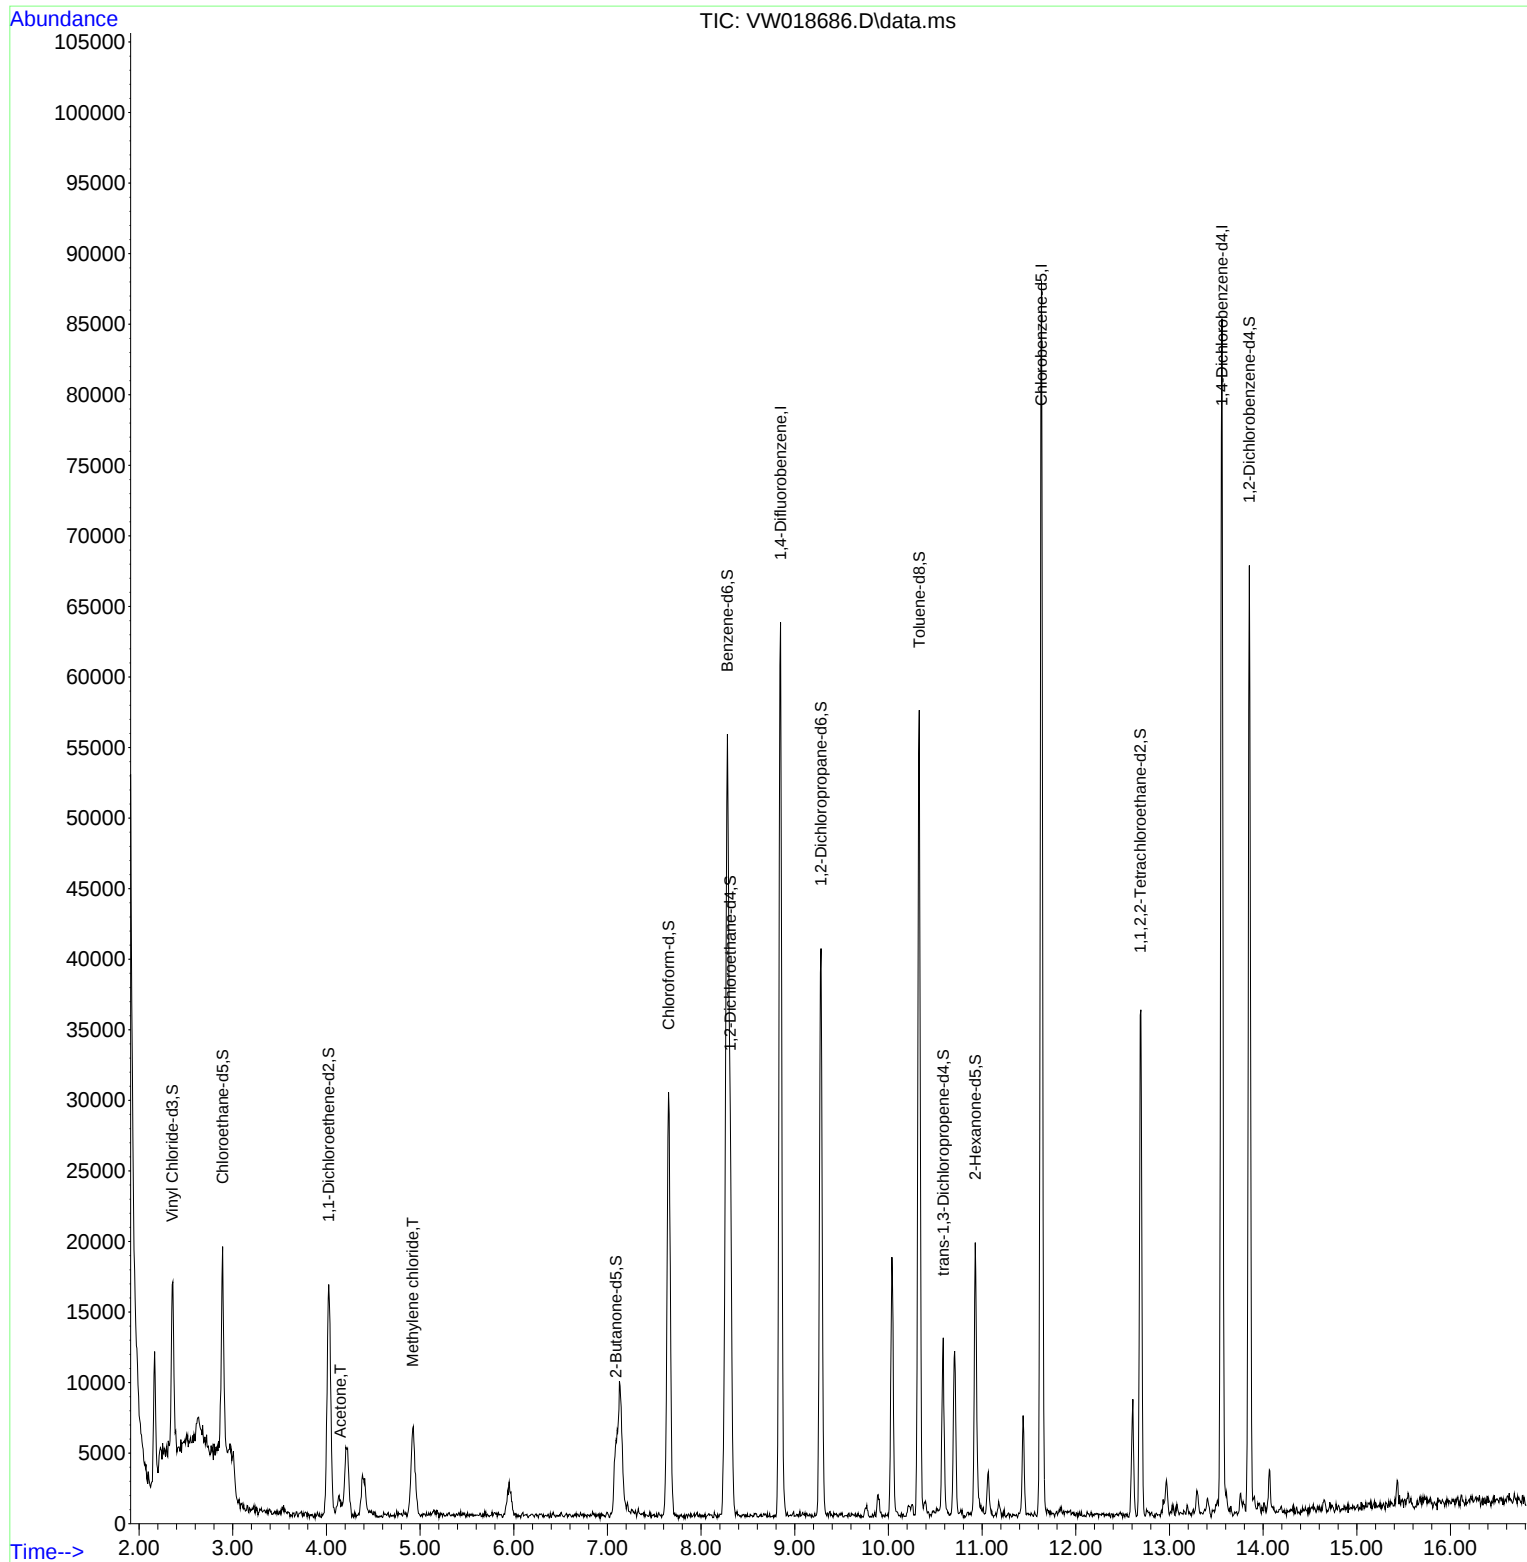

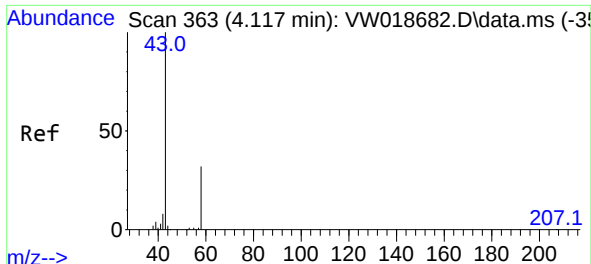

#13
Acetone
Concen: 19.72 ug/L m
RT: 4.147 min Scan# 368
Delta R.T. 0.030 min
Lab File: VW018686.D
Acq: 20 Apr 2021 13:12




Instrument :
MSVOA_W
ClientSampled :
BG560

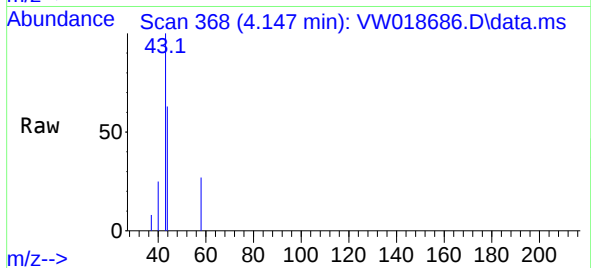


Tgt Ion: 43 Resp: 2576
Ion Ratio Lower Upper
43 100
58 23.1 0.0 53.8

Manual Integrations
APPROVED

MMDadoda
4/21/2021 4:51:29 PM

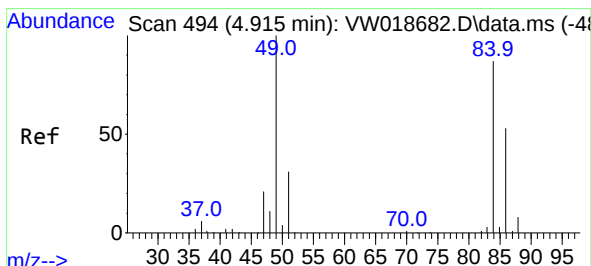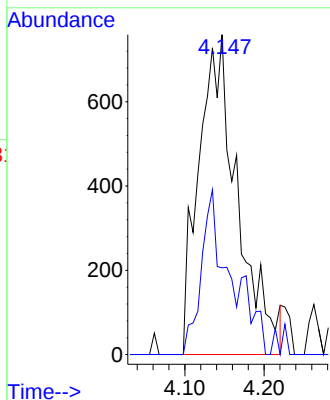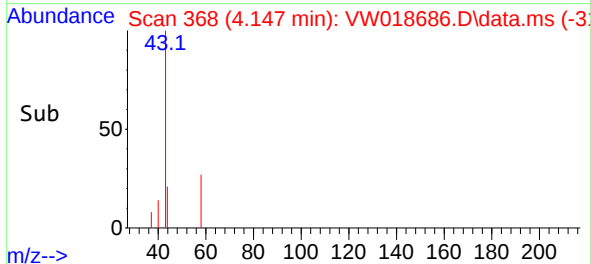

#16
Methylene chloride
Concen: 5.53 ug/L
RT: 4.921 min Scan# 495
Delta R.T. 0.006 min
Lab File: VW018686.D
Acq: 20 Apr 2021 13:12

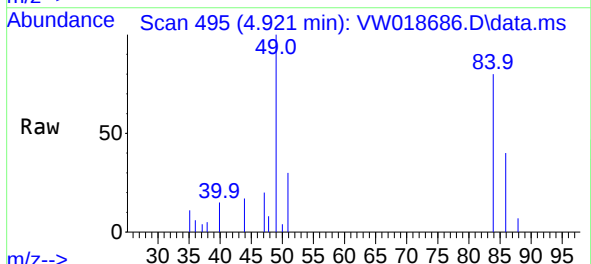

Tgt Ion: 84 Resp: 4715
Ion Ratio Lower Upper
84 100
86 49.6 45.3 84.1
49 125.4 86.6 160.8

