

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042120\
 Data File : VW015296.D
 Acq On : 22 Apr 2020 06:31
 Operator : SY/VA
 Sample : L2123-12
 Misc : 6.13G/5ML/MSVOA W/SOIL
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 TR-05-042020

Quant Time: Apr 22 07:58:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W042020S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 21 06:39:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	202915	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	282742	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	242808	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	92682	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	80377	48.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.88%	
35) Dibromofluoromethane	7.88	113	81867	52.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.54%	
50) Toluene-d8	10.32	98	337090	51.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.32%	
62) 4-Bromofluorobenzene	12.62	95	101567	40.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	80.80%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW042120\
Data File : VW015296.D
Acq On : 22 Apr 2020 06:31
Operator : SY/VA
Sample : L2123-12
Misc : 6.13G/5ML/MSVOA W/SOIL
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
TR-05-042020

Quant Time: Apr 22 07:58:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W042020S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 21 06:39:58 2020
Response via : Initial Calibration

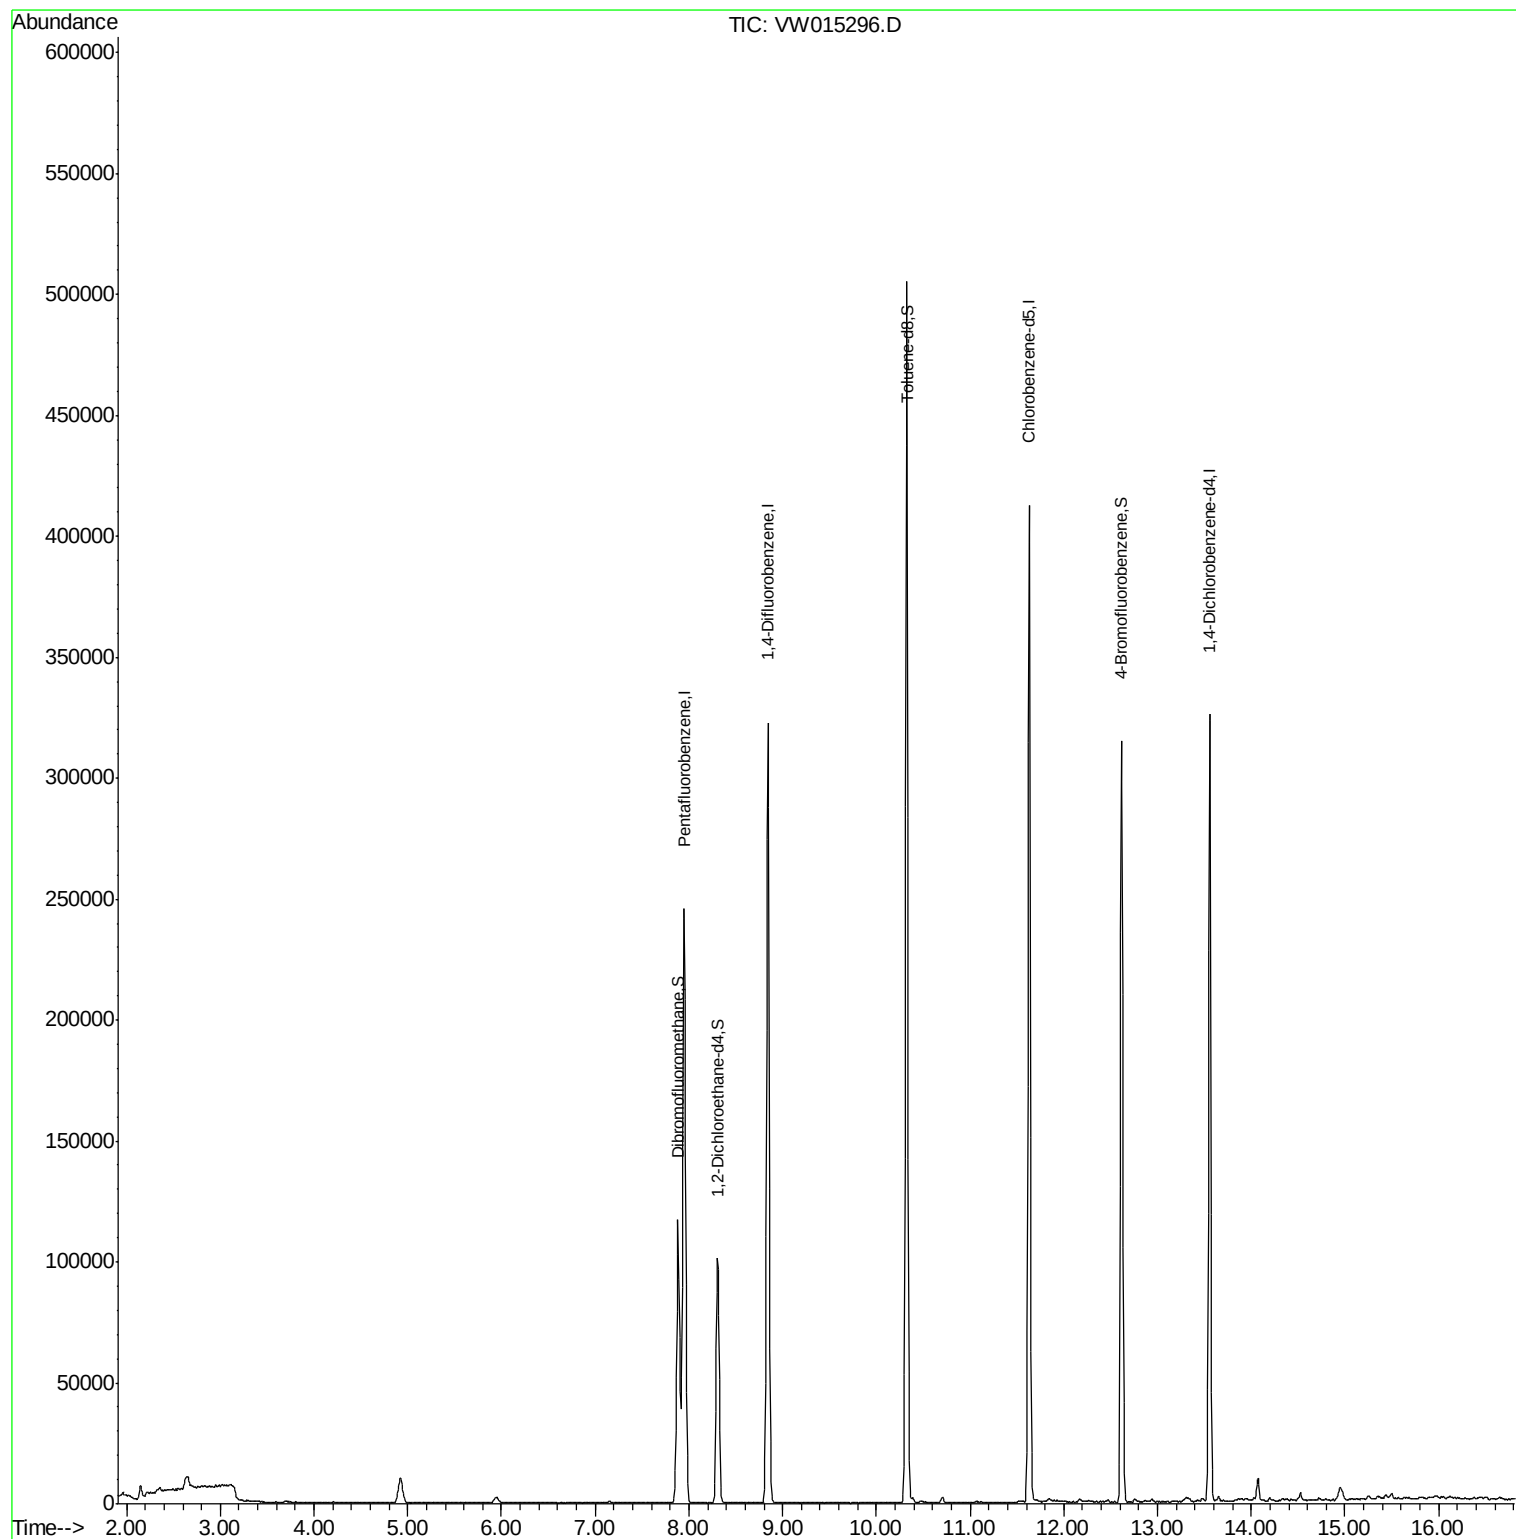

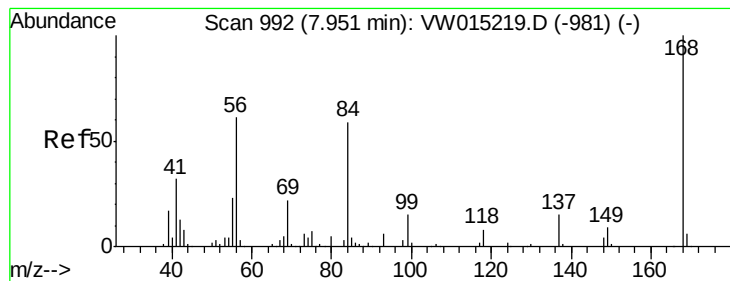

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31

Instrument :

MSVOA_W

ClientSampleId :


TR-05-042020

Tot Ion:168 Resp: 202915

Ion Ratio Lower Upper




168 100

99 50.2 48.5 72.7

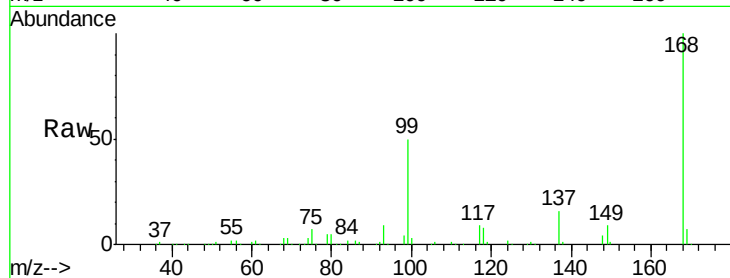

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

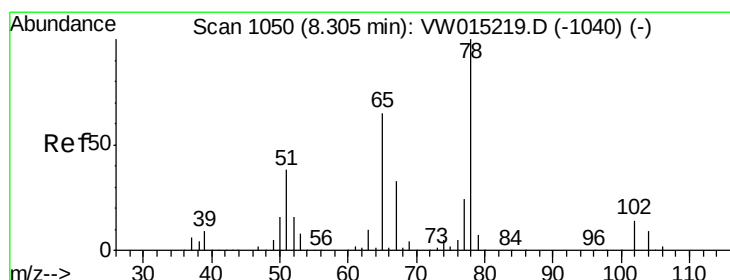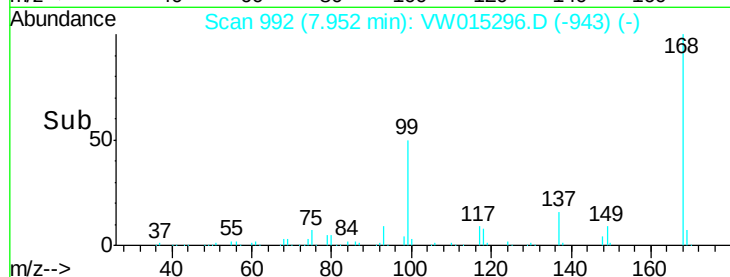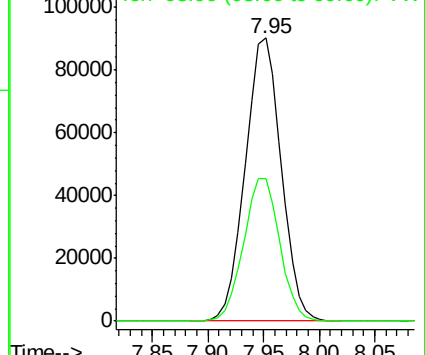

#33

1,2-Dichloroethane-d4

Concen: 48.439 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW015296.D


Acq: 22 Apr 2020 06:31

Tgt Ion: 65 Resp: 80377

Ion Ratio Lower Upper



65 100


67 50.9 0.0 107.0

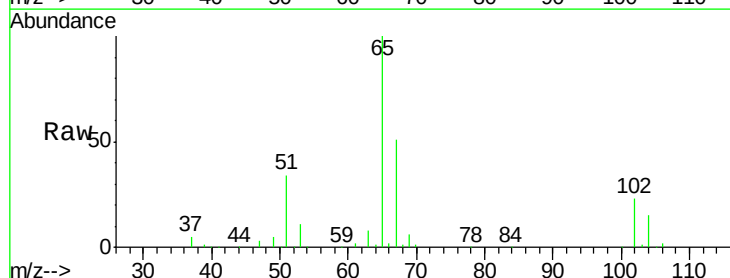

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

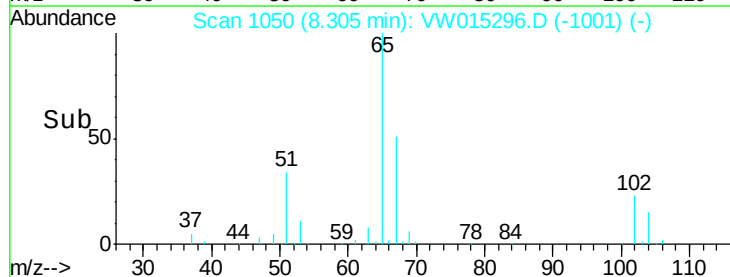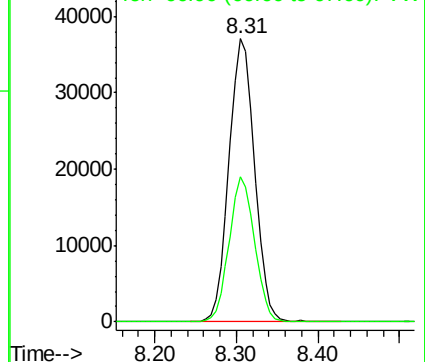

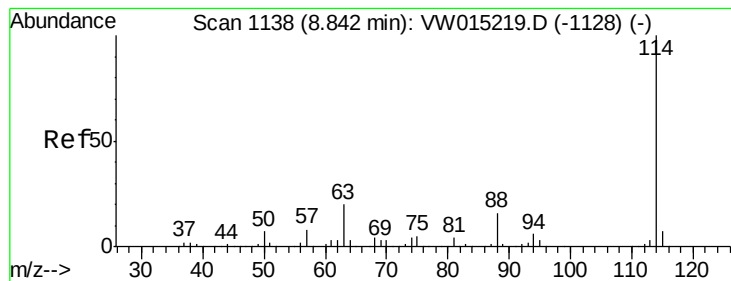

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. 0.00 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31

Instrument :

MSVOA_W

ClientSampleId :

TR-05-042020


Tot Ion:114 Resp: 282742

Ion Ratio Lower Upper

114 100

63 17.9 0.0 39.8




88 15.2 0.0 30.2

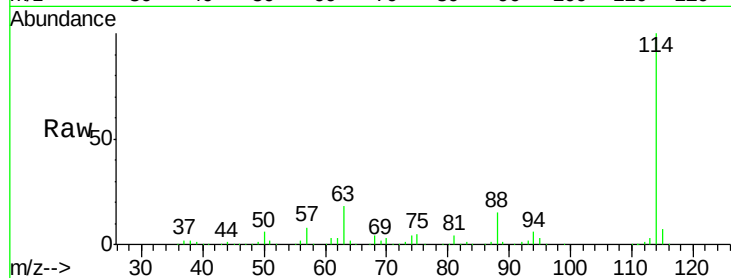

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

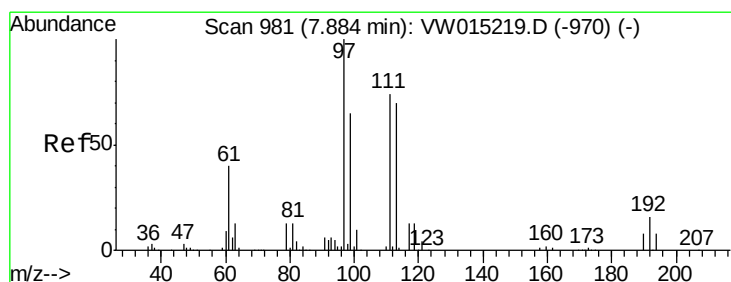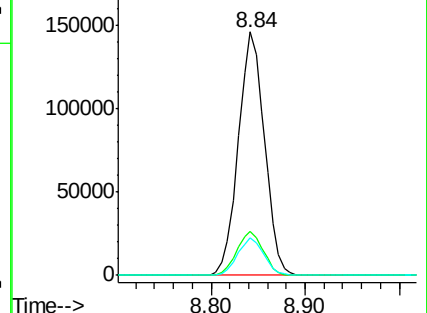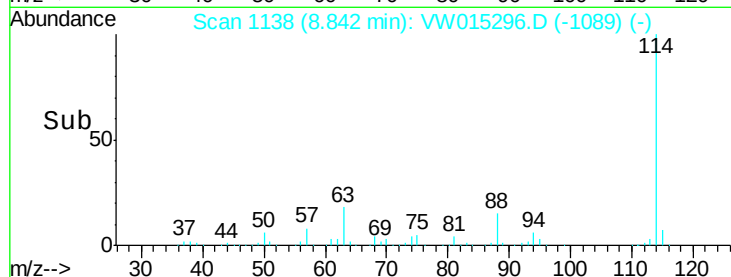

#35

Dibromofluoromethane

Concen: 52.272 ug/l

RT: 7.88 min Scan# 981

Delta R.T. 0.00 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31


Tgt Ion:113 Resp: 81867

Ion Ratio Lower Upper

113 100

111 102.7 83.0 124.4



192 23.3 15.1 22.7#

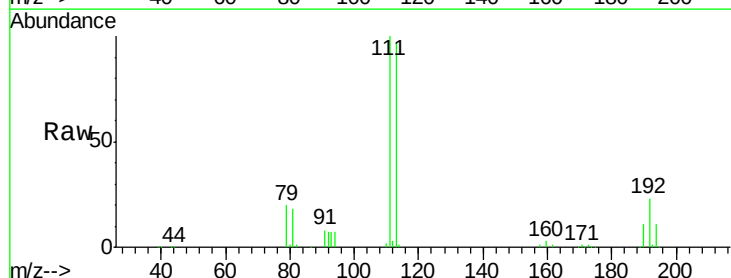


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

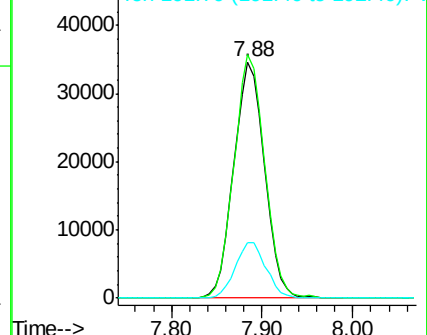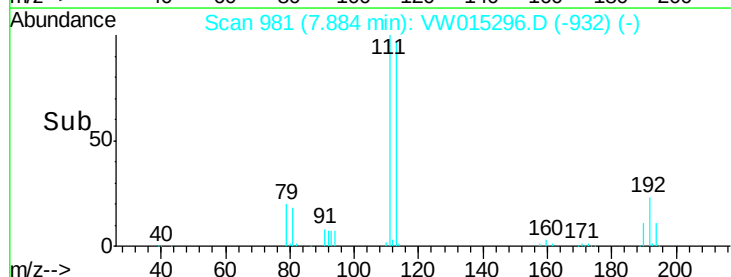

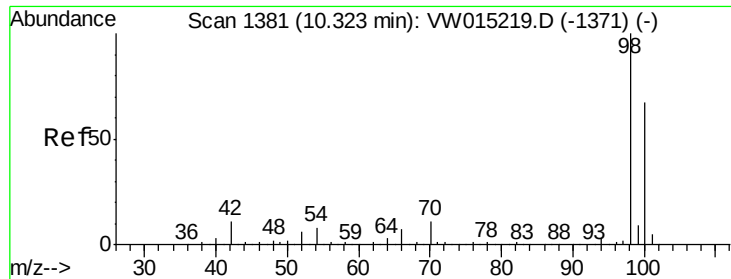

#50

Toluene-d8

Concen: 51.164 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31

Instrument :

MSVOA_W

ClientSampleId :


TR-05-042020

Tot Ion: 98 Resp: 337090

Ion Ratio Lower Upper

98 100

100 65.8 52.9 79.3

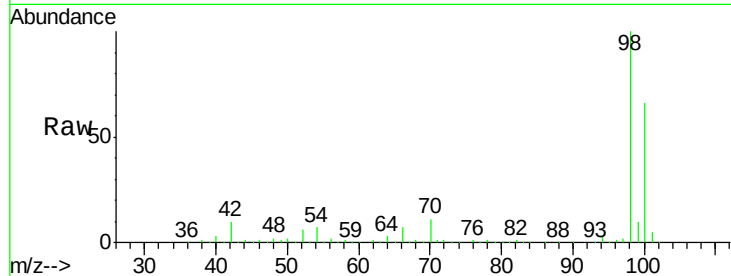

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

200000

150000

100000

50000



0

10.32

10.30

10.40

Time-->

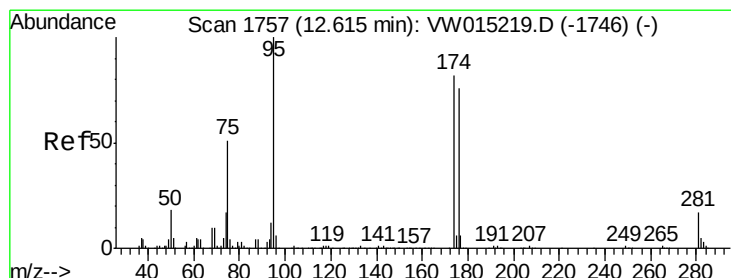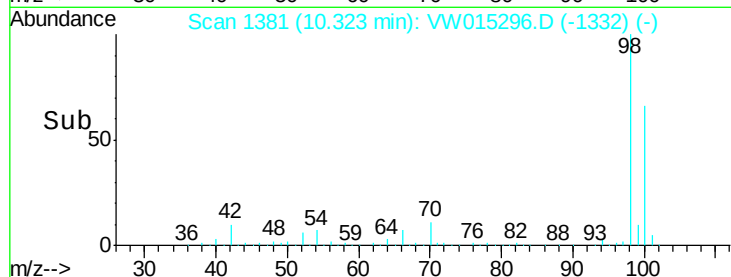

#62

4-Bromofluorobenzene

Concen: 40.404 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31


Tgt Ion: 95 Resp: 101567

Ion Ratio Lower Upper

95 100

174 92.0 0.0 144.4

176 88.1 0.0 140.6

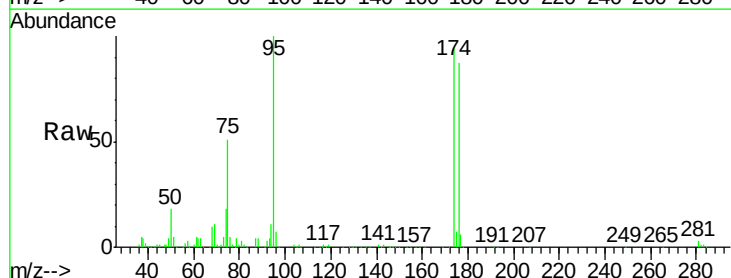

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

80000

60000

40000

20000


0


12.62

12.60

12.70

Time-->

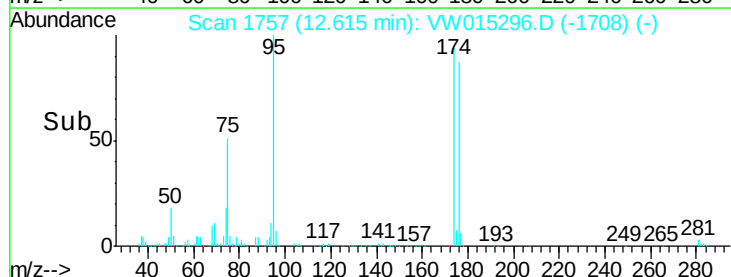

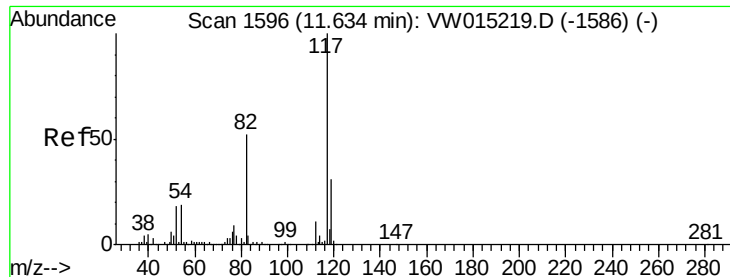

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1595

Delta R.T. -0.01 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31

Instrument :

MSVOA_W

ClientSampleId :

TR-05-042020


Tot Ion:117 Resp: 242808

Ion Ratio Lower Upper

117 100

82 52.3 44.1 66.1




119 30.9 24.9 37.3

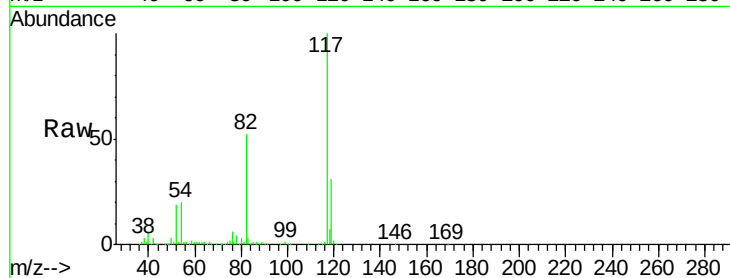

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

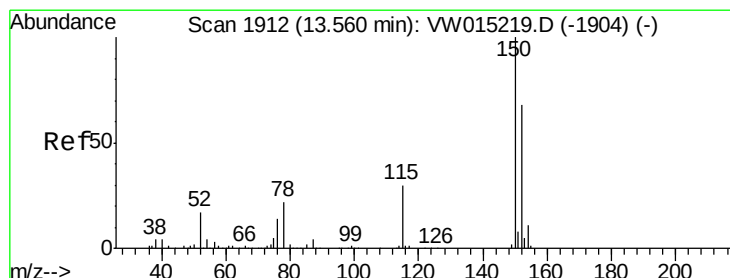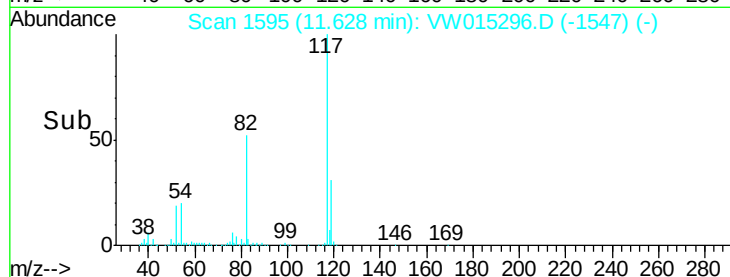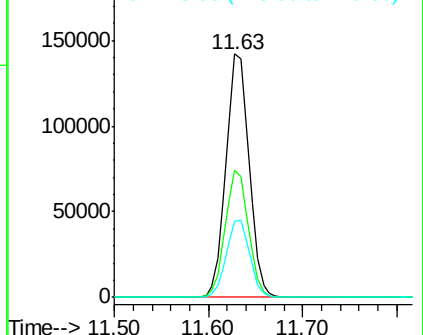

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW015296.D

Acq: 22 Apr 2020 06:31


Tgt Ion:152 Resp: 92682

Ion Ratio Lower Upper

152 100

115 55.2 31.3 93.9

150 155.9 0.0 343.4

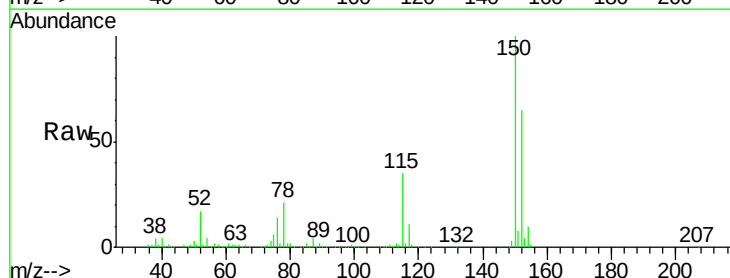

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

