


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW042120\
 Data File : VW015249.D
 Acq On : 21 Apr 2020 09:07
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W042020S.M
 Title : SW846 8260
 Last Update : Tue Apr 21 06:39:58 2020

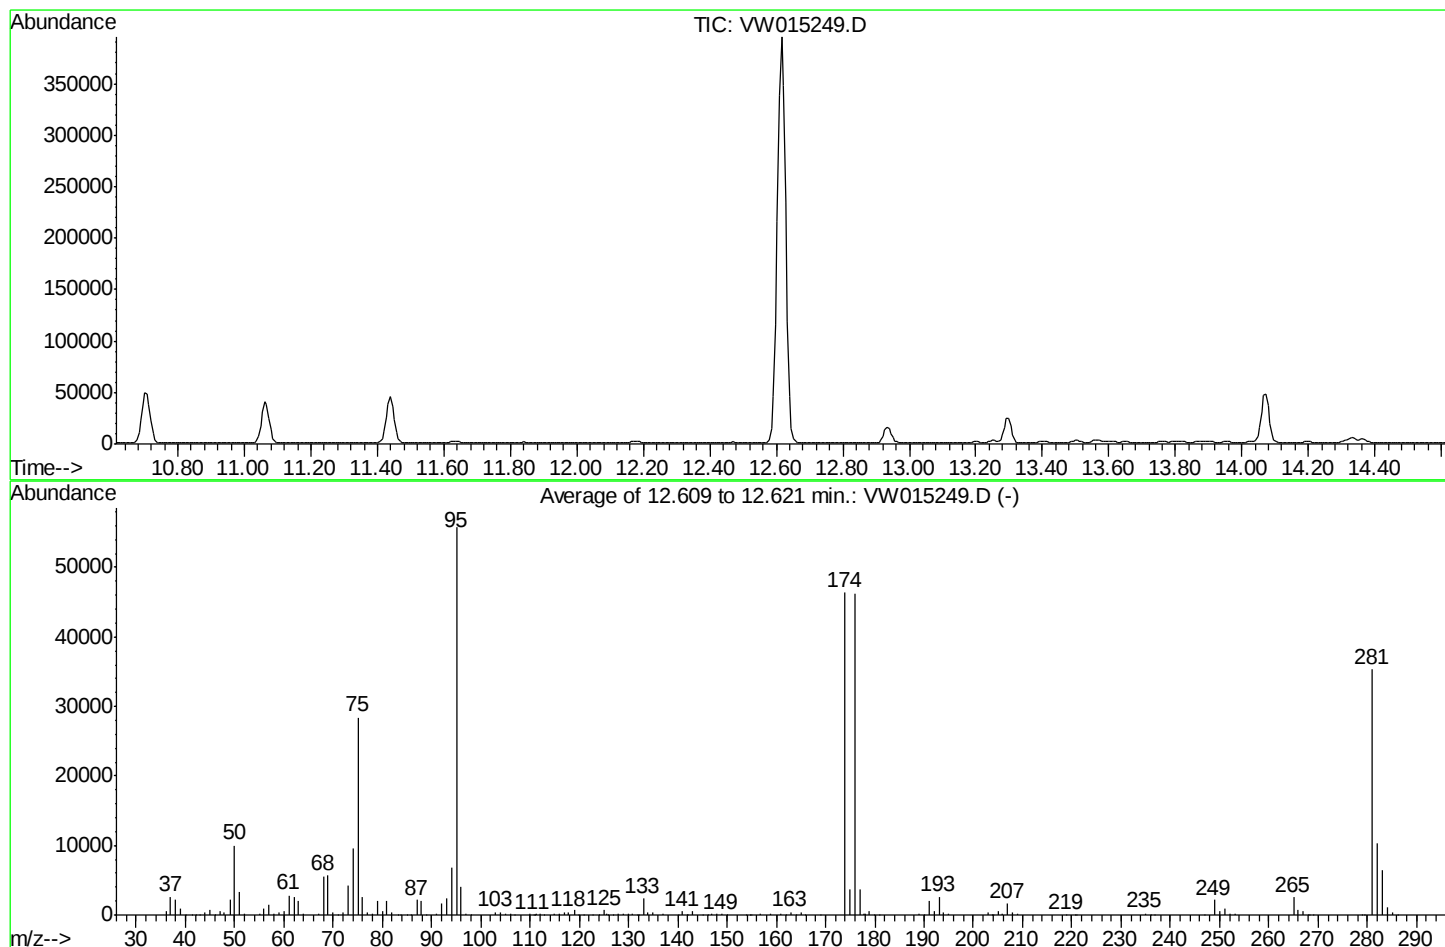

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10035	PASS
75	95	30	60	50.9	28392	PASS
95	95	100	100	100.0	55762	PASS
96	95	5	9	7.3	4088	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.1	46346	PASS
175	174	5	9	8.1	3734	PASS
176	174	95	101	99.7	46210	PASS
177	176	5	9	8.1	3740	PASS