

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042121\
Data File : VW018715.D
Acq On : 21 Apr 2021 16:21
Operator : SY/VA
Sample : M2065-13
Misc : 3.23G/10ML/MSVOA_W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG566

Manual Integrations
APPROVED

MMDadoda
4/27/2021 3:17:08 PM

Quant Time: Apr 22 01:23:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 22 01:20:40 2021
Response via : Initial Calibration

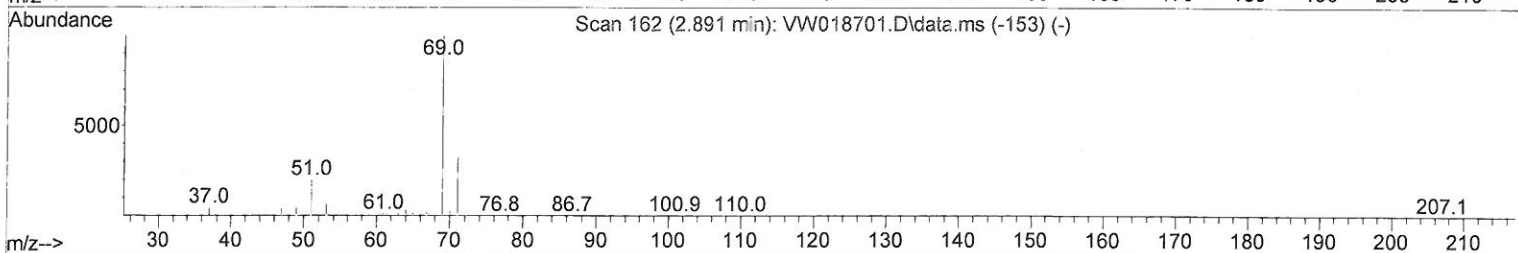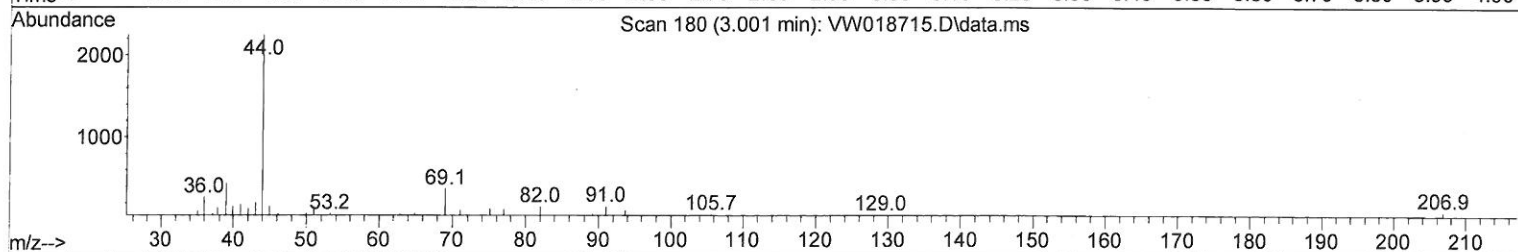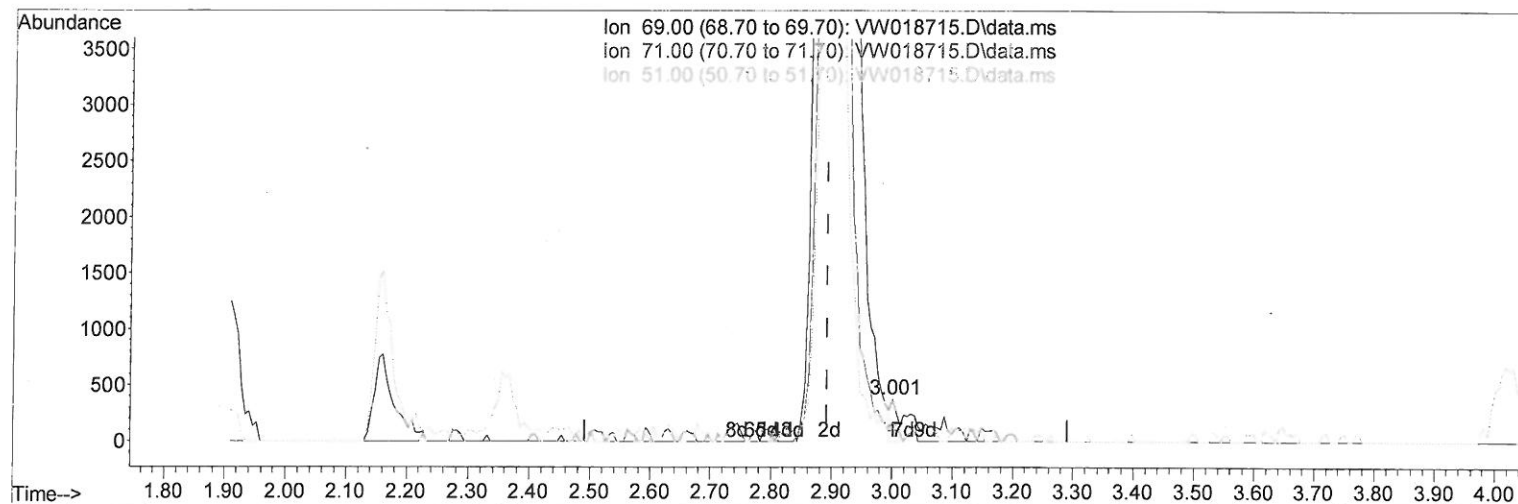

TIC: VW018715.D\data.ms

(7) Chloroethane-d5 (S)

3.001min (+ 0.110) 0.03 ug/L

response 282

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	38.65
51.00	28.40	25.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042121\
 Data File : VW018715.D
 Acq On : 21 Apr 2021 16:21
 Operator : SY/VA
 Sample : M2065-13
 Misc : 3.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG566

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 3:17:08 PM

Quant Time: Apr 22 01:23:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 22 01:20:40 2021
 Response via : Initial Calibration

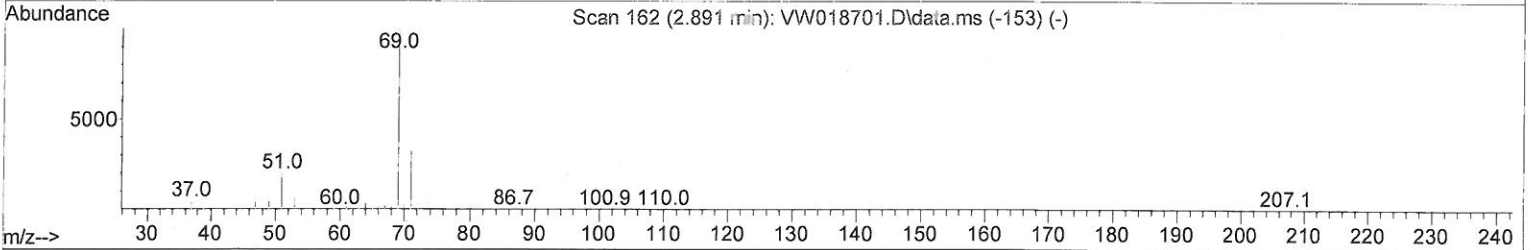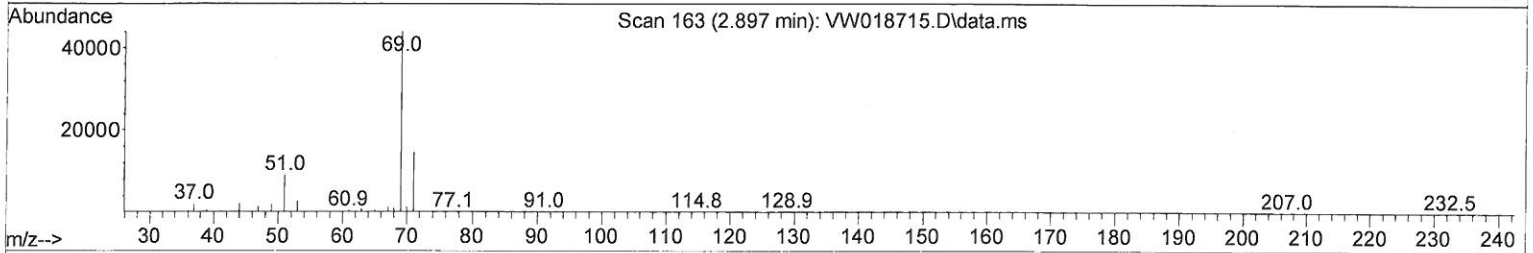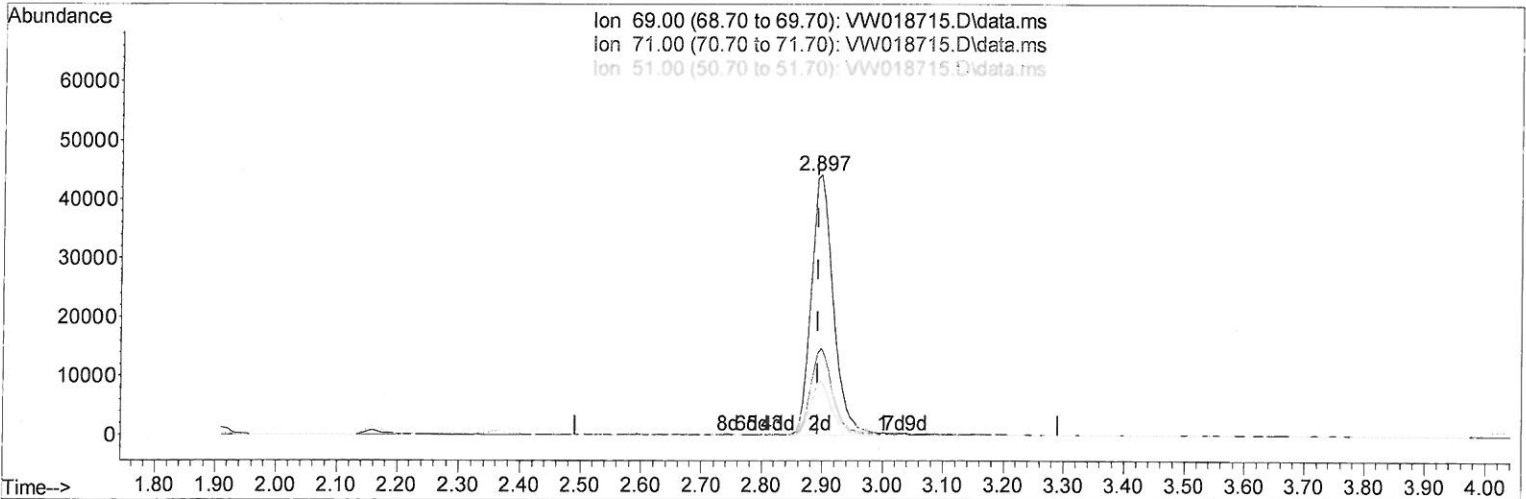

TIC: VW018715.D\data.ms

(7) Chloroethane-d5 (S)

2.897min (+ 0.006) 12.92 ug/L m

response 112340

Ion	Exp%	Act%
-----	------	------

69.00	100.00	100.00
-------	--------	--------

71.00	32.10	0.10#
-------	-------	-------

51.00	28.40	0.06#
-------	-------	-------

0.00	0.00	0.00
------	------	------

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042121\
 Data File : VW018715.D
 Acq On : 21 Apr 2021 16:21
 Operator : SY/VA
 Sample : M2065-13
 Misc : 3.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG566

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 3:17:08 PM

Quant Time: Apr 22 01:23:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 22 01:20:40 2021
 Response via : Initial Calibration

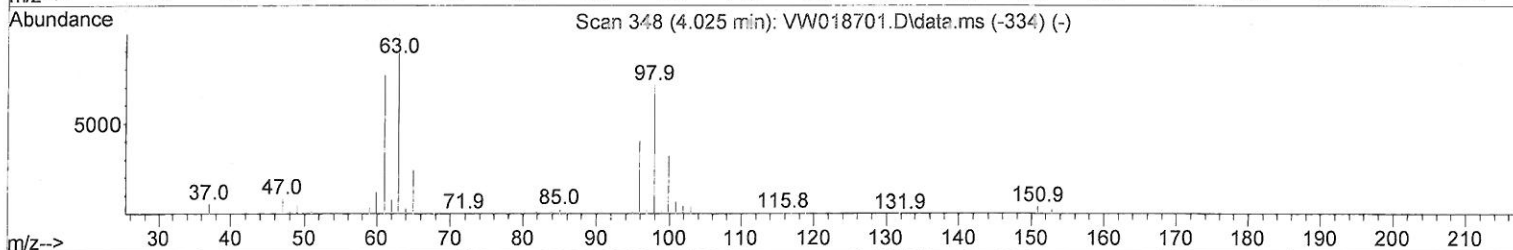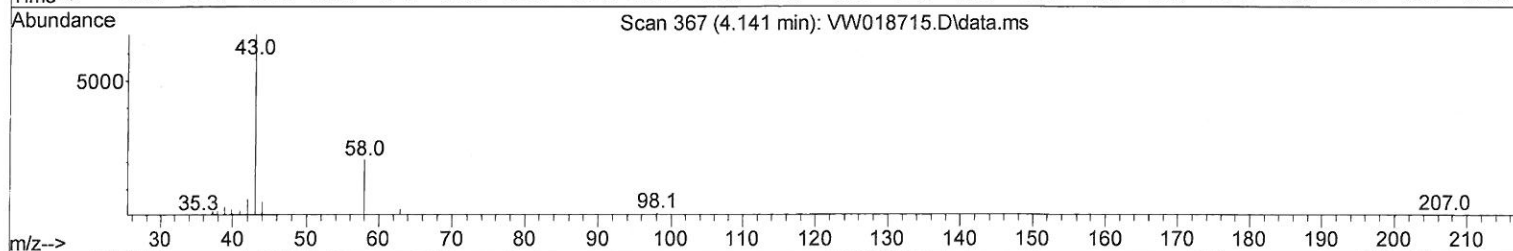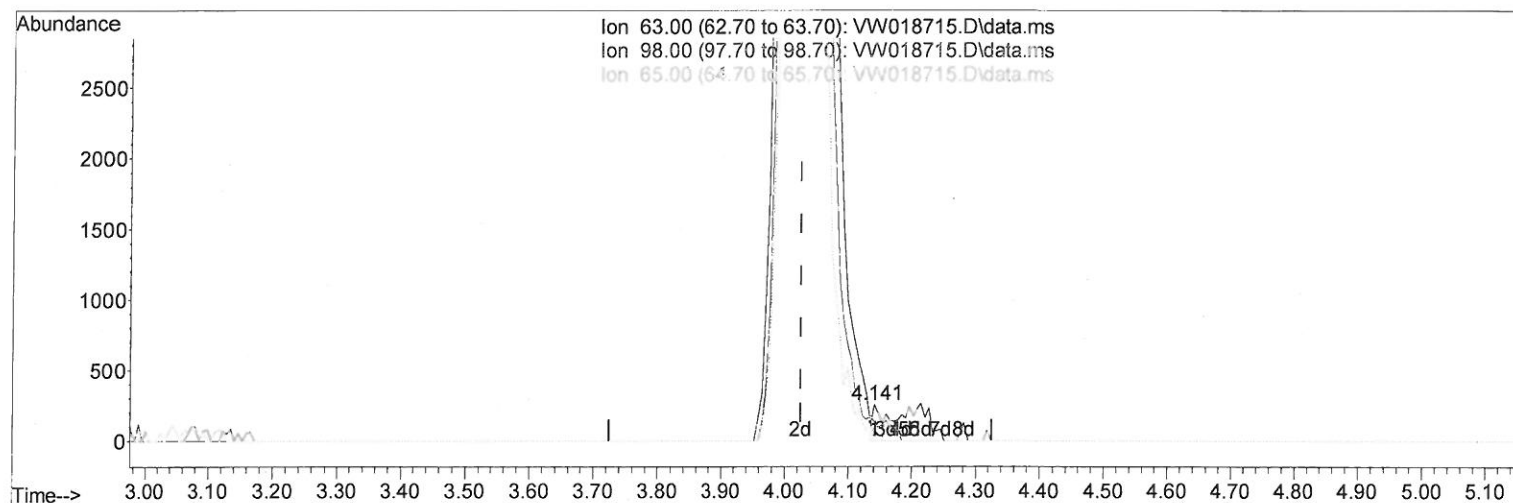

TIC: VW018715.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.141min (+ 0.116) 0.01 ug/L

response 210

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.20	69.05
65.00	23.70	28.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042121\
 Data File : VW018715.D
 Acq On : 21 Apr 2021 16:21
 Operator : SY/VA
 Sample : M2065-13
 Misc : 3.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG566

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 3:17:08 PM

Quant Time: Apr 22 01:23:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 22 01:20:40 2021
 Response via : Initial Calibration

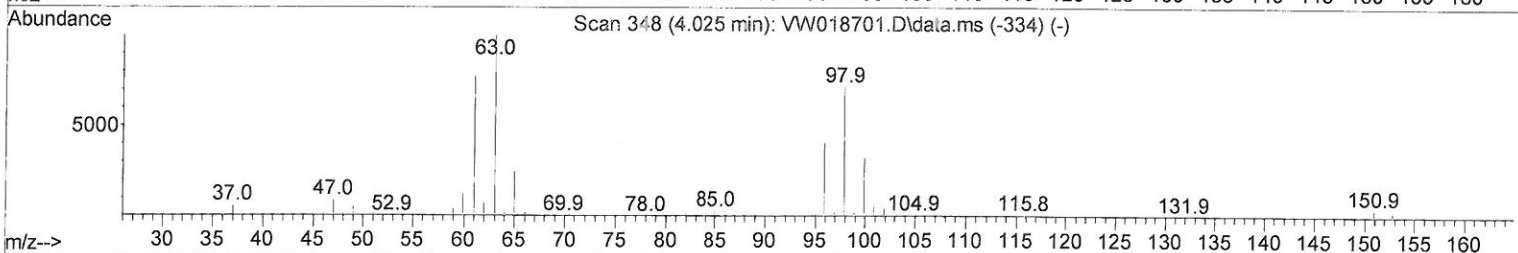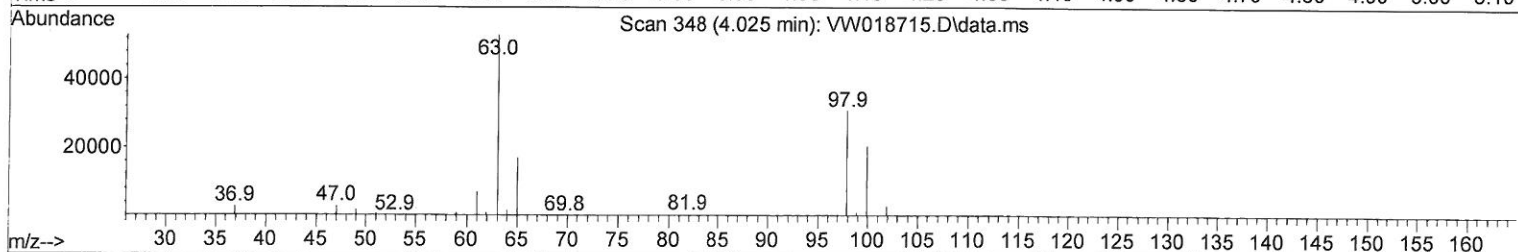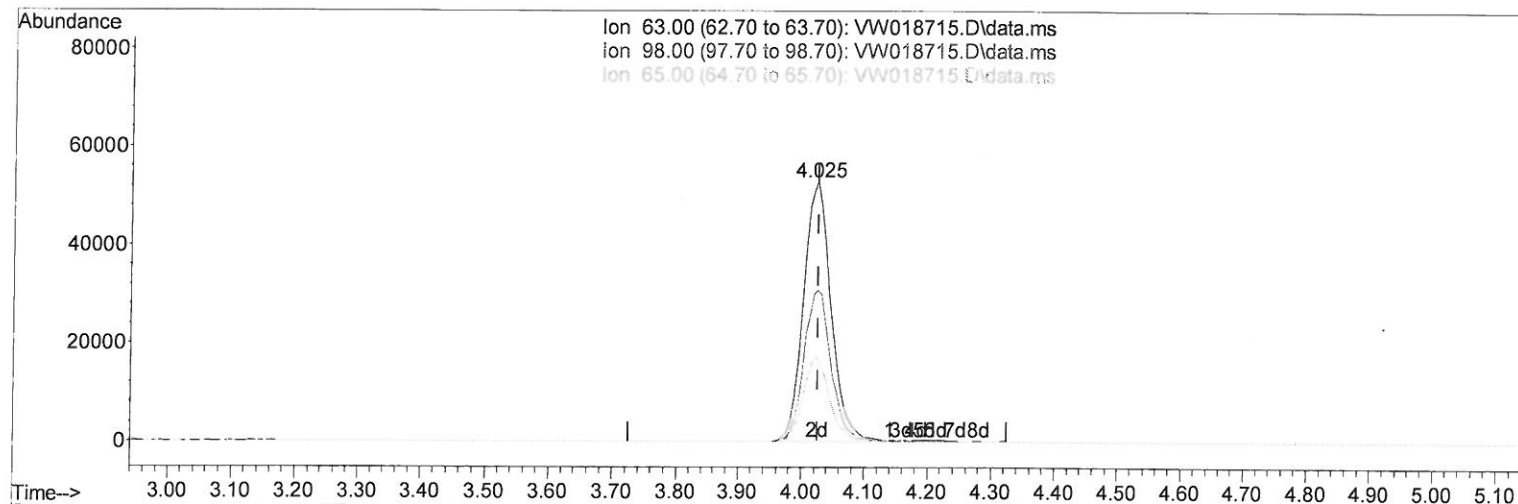

TIC: VW018715.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.025min (-0.000) 9.44 ug/L m

response 160749

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.20	0.09#
65.00	23.70	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042121\
 Data File : VW018715.D
 Acq On : 21 Apr 2021 16:21
 Operator : SY/VA
 Sample : M2065-13
 Misc : 3.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG566

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 3:17:08 PM

Quant Time: Apr 22 01:23:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 22 01:20:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	645545	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	513512	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	195861	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	120138	12.25	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	49.00%		
7) Chloroethane-d5	2.897	69	112340m	12.92	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	51.68%		
11) 1,1-Dichloroethene-d2	4.025	63	160749m	9.44	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	37.76%#		
21) 2-Butanone-d5	7.086	46	72919	32.65	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	65.30%		
24) Chloroform-d	7.653	84	329861	18.62	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	74.48%		
26) 1,2-Dichloroethane-d4	8.311	65	170032	17.07	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	68.28%#		
32) Benzene-d6	8.281	84	568508	18.87	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	75.48%		
36) 1,2-Dichloropropane-d6	9.274	67	191480	21.09	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	84.36%		
41) Toluene-d8	10.323	98	470345	17.07	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	68.28%		
43) trans-1,3-Dichloroprop...	10.579	79	59168	15.31	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	61.24%		
47) 2-Hexanone-d5	10.927	63	61057	38.68	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	77.36%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	136607	18.02	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	72.08%		
66) 1,2-Dichlorobenzene-d4	13.853	152	148534	21.59	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	86.36%		
Target Compounds						
13) Acetone	4.141	43	20456	12.62	ug/L	92
14) Carbon disulfide	4.391	76	19847	0.79	ug/L	95
16) Methylene chloride	4.922	84	38966	3.68	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042121\
Data File : VW018715.D
Acq On : 21 Apr 2021 16:21
Operator : SY/VA
Sample : M2065-13
Misc : 3.23G/10ML/MSVOA_W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG566

Manual Integrations
APPROVED

MMDadoda
4/27/2021 3:17:08 PM

Quant Time: Apr 22 01:23:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 22 01:20:40 2021
Response via : Initial Calibration

