




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025627.D
 Acq On : 21 Apr 2023 12:27
 Operator : SY/MD
 Sample : 02418-08RE
 Misc : 3.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:04:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

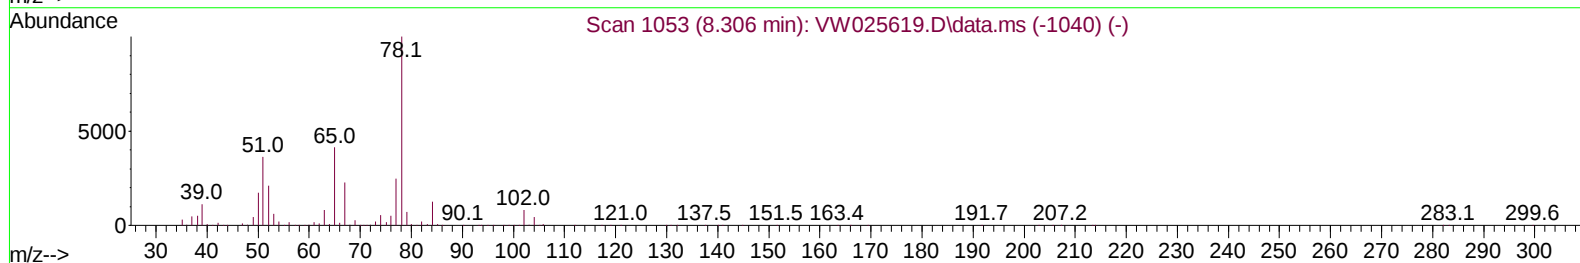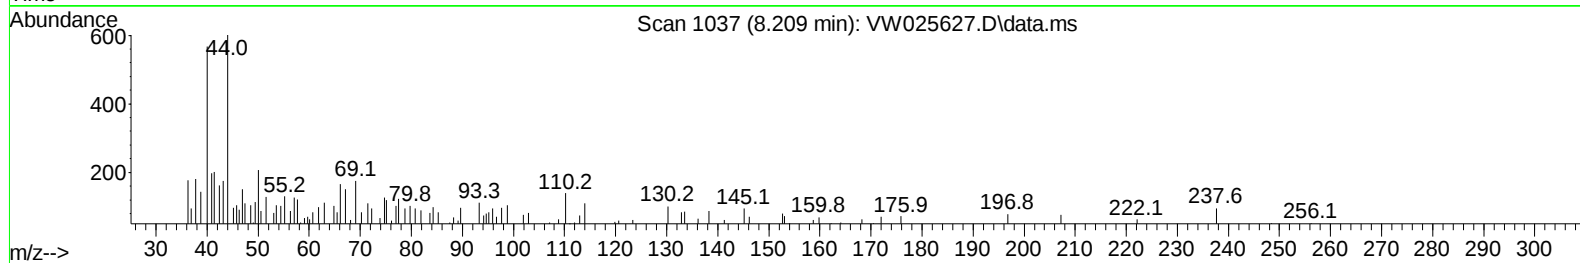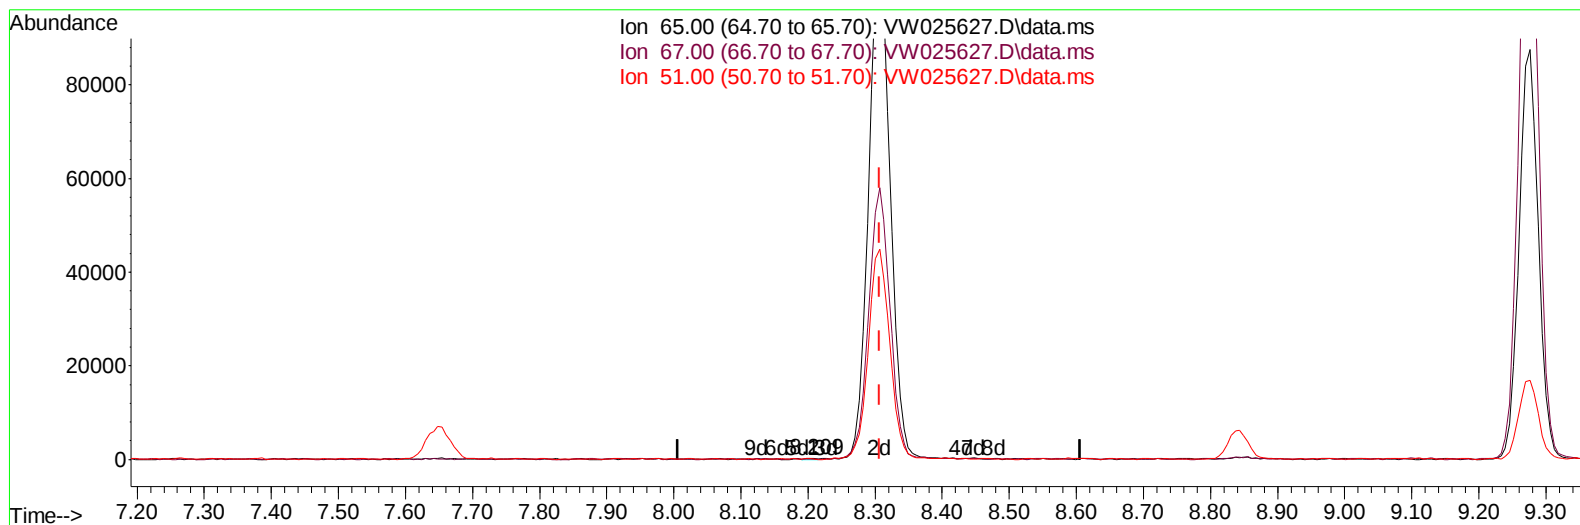

TIC: VW025627.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.209min (-0.097) 0.03 ug/L

response 222

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.50	55.86
51.00	124.00	99.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025627.D
 Acq On : 21 Apr 2023 12:27
 Operator : SY/MD
 Sample : 02418-08RE
 Misc : 3.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:04:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

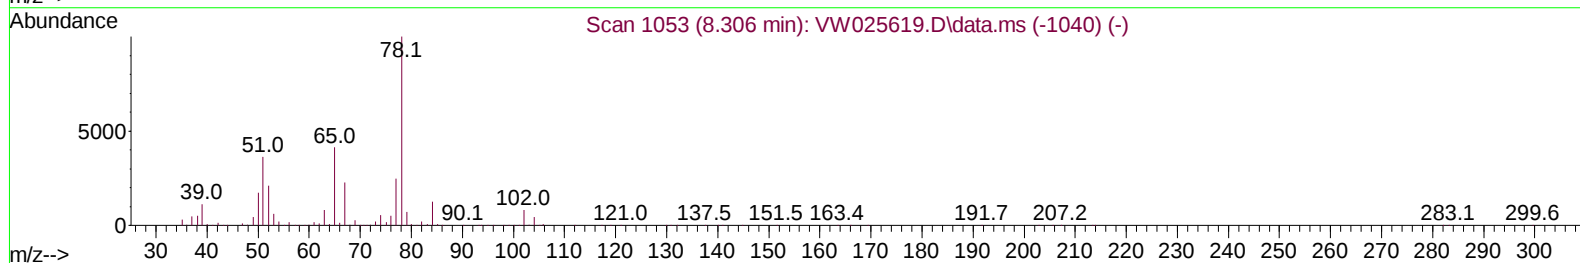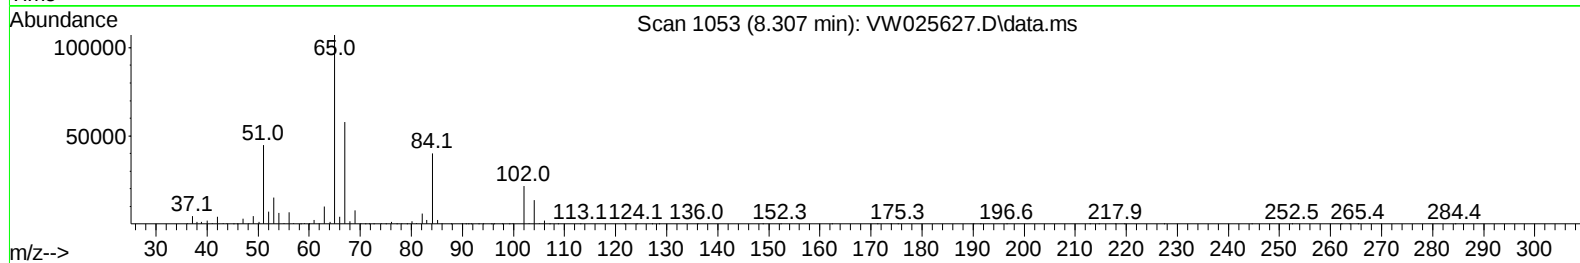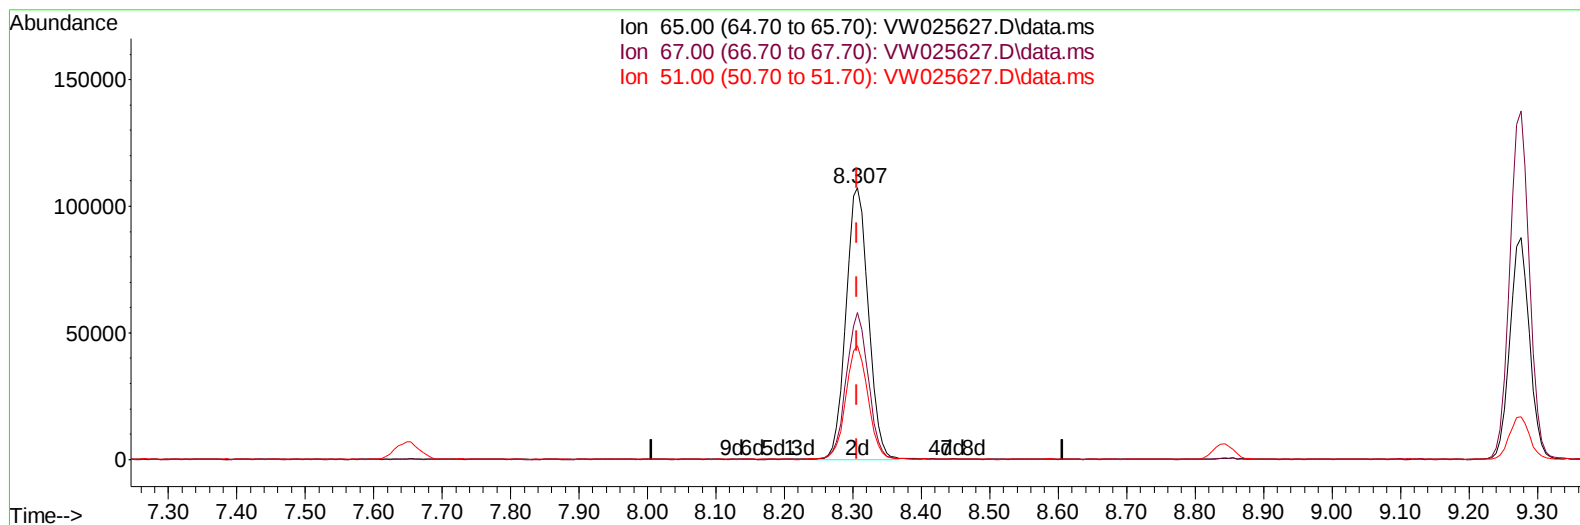

TIC: VW025627.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 28.05 ug/L m

response 241876

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.50	0.05#
51.00	124.00	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025627.D
 Acq On : 21 Apr 2023 12:27
 Operator : SY/MD
 Sample : 02418-08RE
 Misc : 3.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:04:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	590274	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	432849	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	127222	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	162241	16.891	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.560%	
7) Chloroethane-d5	2.899	69	148980	21.785	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.120%	
11) 1,1-Dichloroethene-d2	4.027	63	270919	13.947	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.800%	
21) 2-Butanone-d5	7.075	46	160051	74.691	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	149.380%#	
24) Chloroform-d	7.648	84	410471	24.767	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.080%	
26) 1,2-Dichloroethane-d4	8.307	65	241876m	28.053	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	112.200%	
32) Benzene-d6	8.276	84	782487	27.919	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	111.680%	
36) 1,2-Dichloropropane-d6	9.276	67	274957	31.463	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	125.840%#	
41) Toluene-d8	10.325	98	606504	24.773	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	99.080%	
43) trans-1,3-Dichloroprop...	10.581	79	81592	24.903	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	99.600%	
47) 2-Hexanone-d5	10.922	63	97382	81.525	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	163.040%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	194078	32.903	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	131.600%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	110688	25.325	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	101.320%	
Target Compounds						
13) Acetone	4.118	43	238436	131.472	ug/L	98
16) Methylene chloride	4.923	84	40255	4.290	ug/L	98
22) 2-Butanone	7.173	43	97069	37.650	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025627.D
Acq On : 21 Apr 2023 12:27
Operator : SY/MD
Sample : 02418-08RE
Misc : 3.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8Z4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:04:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

