




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025631.D
 Acq On : 21 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02417-08
 Misc : 5.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:05:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

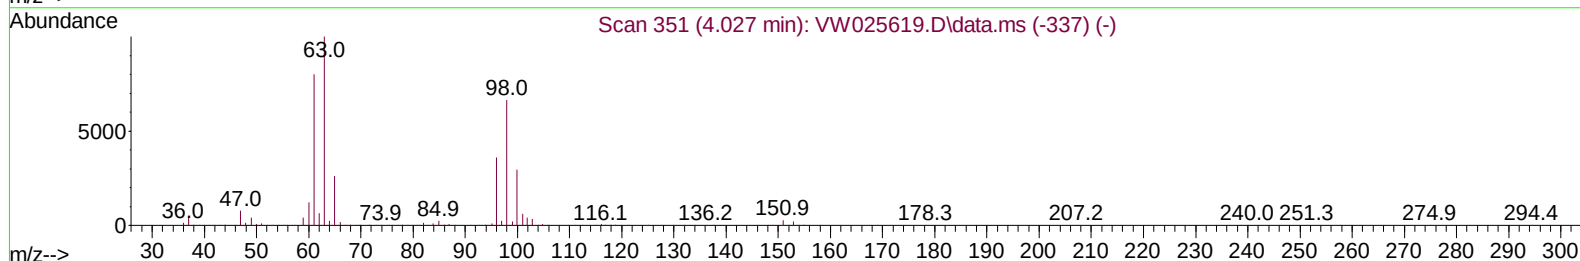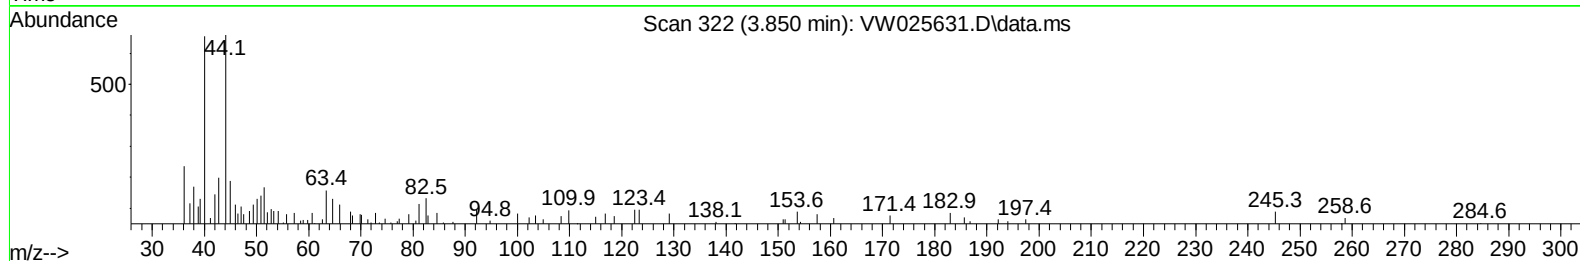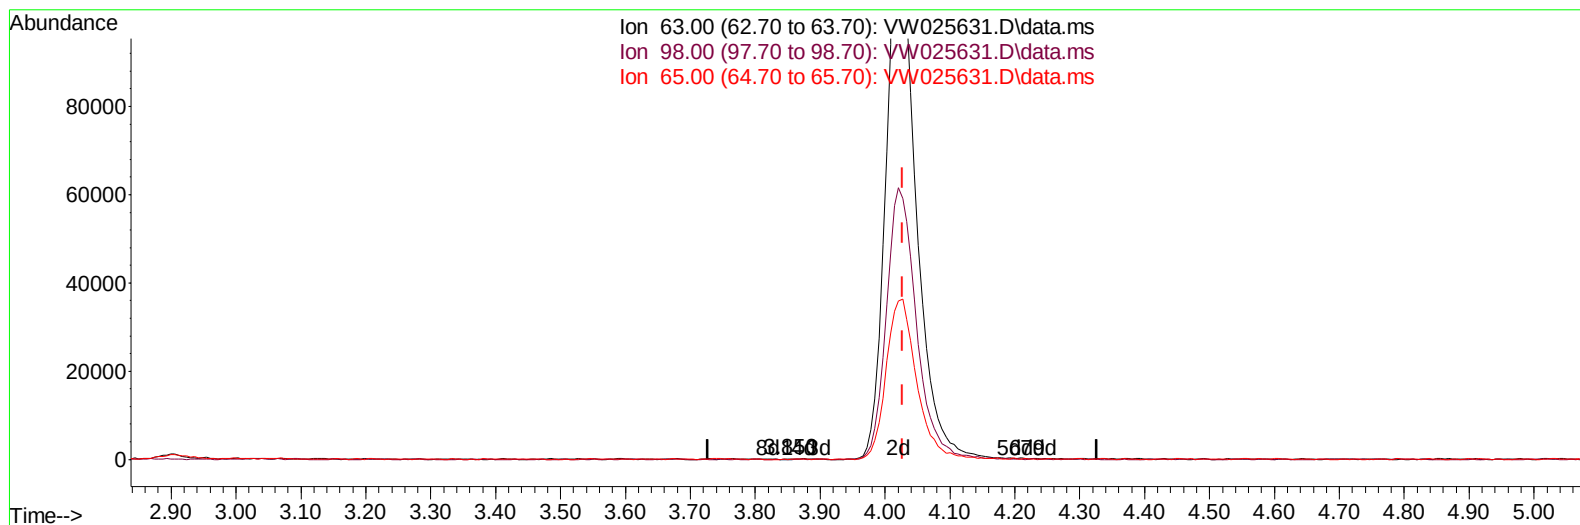

TIC: VW025631.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.850min (-0.176) 0.00 ug/L

response 129

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	58.14
65.00	23.30	29.46
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025631.D
 Acq On : 21 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02417-08
 Misc : 5.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:05:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

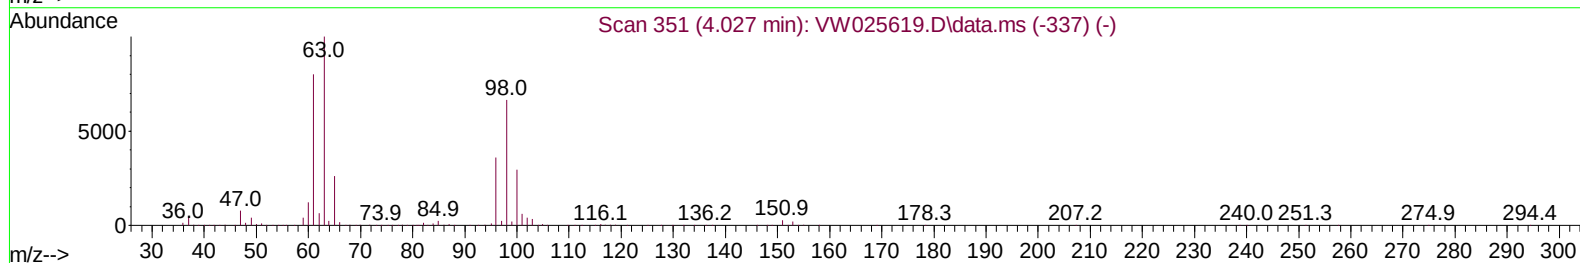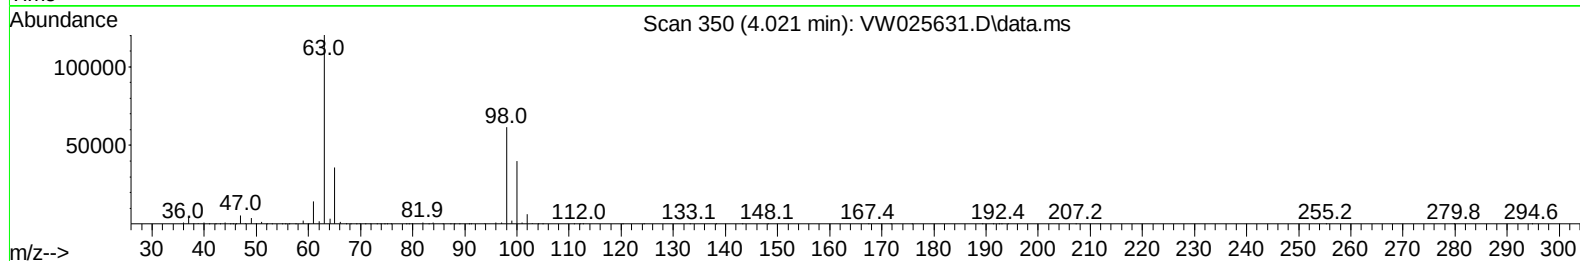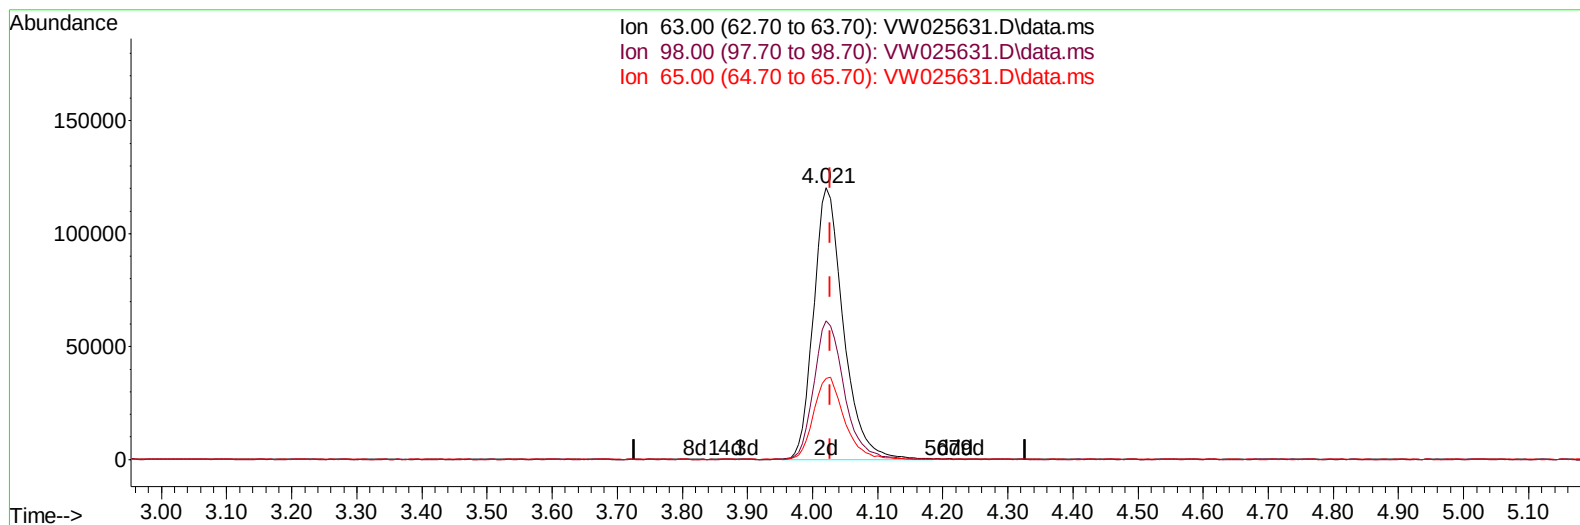

TIC: VW025631.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.006) 13.11 ug/L m

response 381641

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	0.02#
65.00	23.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025631.D
 Acq On : 21 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02417-08
 Misc : 5.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X4

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:05:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		884577	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		765532	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		346337	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		205103	14.249	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.000%	
7) Chloroethane-d5	2.899	69		184333	17.986	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.960%	
11) 1,1-Dichloroethene-d2	4.021	63		381641m	13.110	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.440%	
21) 2-Butanone-d5	7.075	46		195059	60.743	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.480%	
24) Chloroform-d	7.648	84		573329	23.084	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.320%	
26) 1,2-Dichloroethane-d4	8.307	65		332457	25.730	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.920%	
32) Benzene-d6	8.276	84		1124272	22.681	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.720%	
36) 1,2-Dichloropropane-d6	9.276	67		383586	24.818	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.280%	
41) Toluene-d8	10.325	98		940886	21.730	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.920%	
43) trans-1,3-Dichloroprop...	10.575	79		140036	24.166	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.680%	
47) 2-Hexanone-d5	10.922	63		127171	60.197	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.400%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		296482	28.421	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.680%	
66) 1,2-Dichlorobenzene-d4	13.849	152		297163	24.975	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.920%	
Target Compounds							
						Qvalue	
13) Acetone	4.119	43		13642	5.019	ug/L	91
16) Methylene chloride	4.923	84		42601	3.030	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025631.D
Acq On : 21 Apr 2023 14:02
Operator : SY/MD
Sample : 02417-08
Misc : 5.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW8X4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:05:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

