




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025641.D
 Acq On : 21 Apr 2023 18:01
 Operator : SY/MD
 Sample : 02418-28
 Misc : 3.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW902

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:07:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

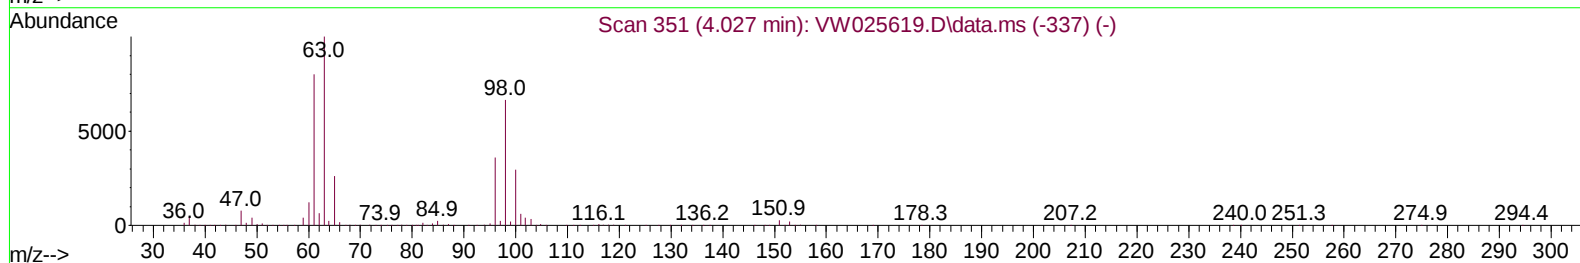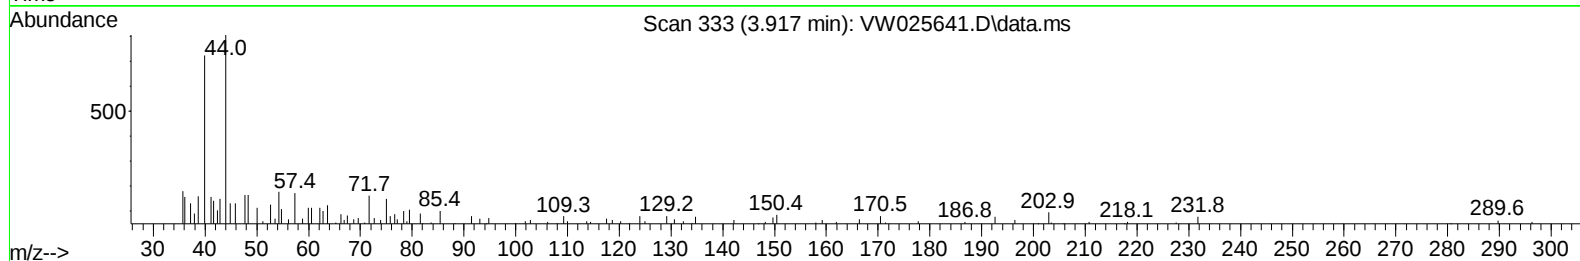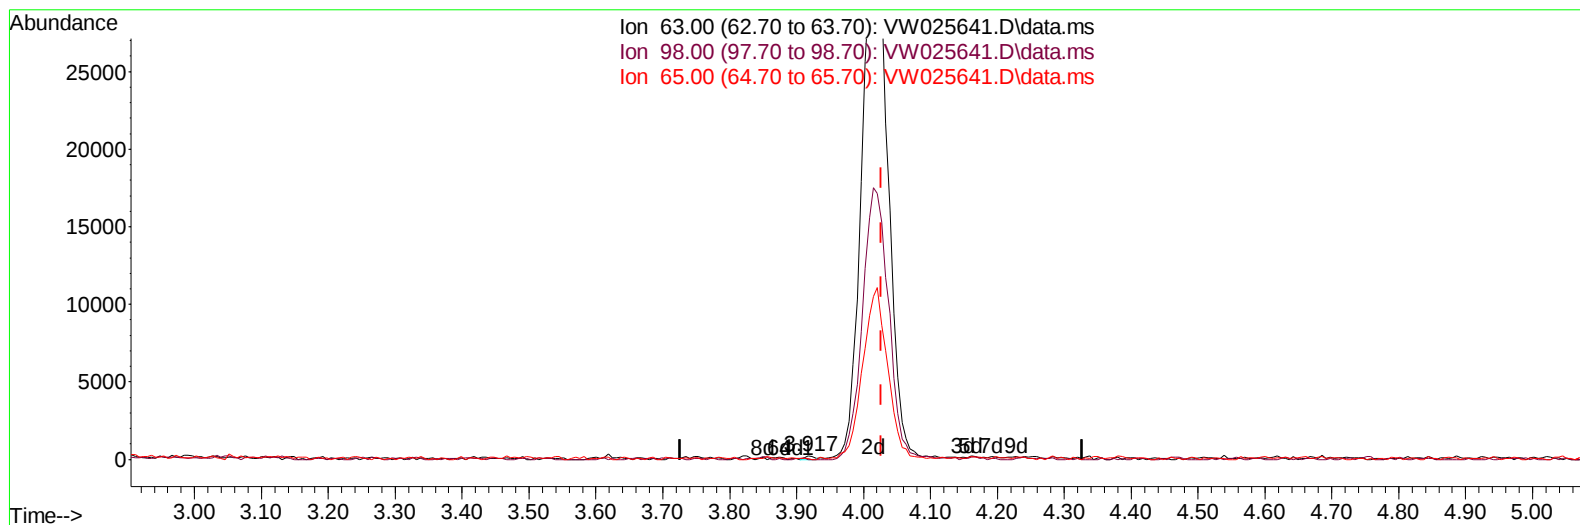

TIC: VW025641.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.917min (-0.109) 0.03 ug/L

response 198

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	46.97
65.00	23.30	22.73
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025641.D
 Acq On : 21 Apr 2023 18:01
 Operator : SY/MD
 Sample : 02418-28
 Misc : 3.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW902

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:07:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

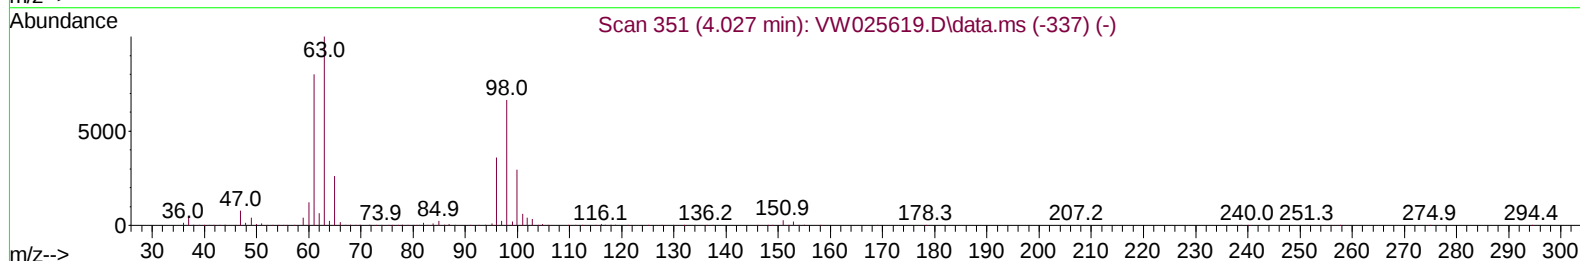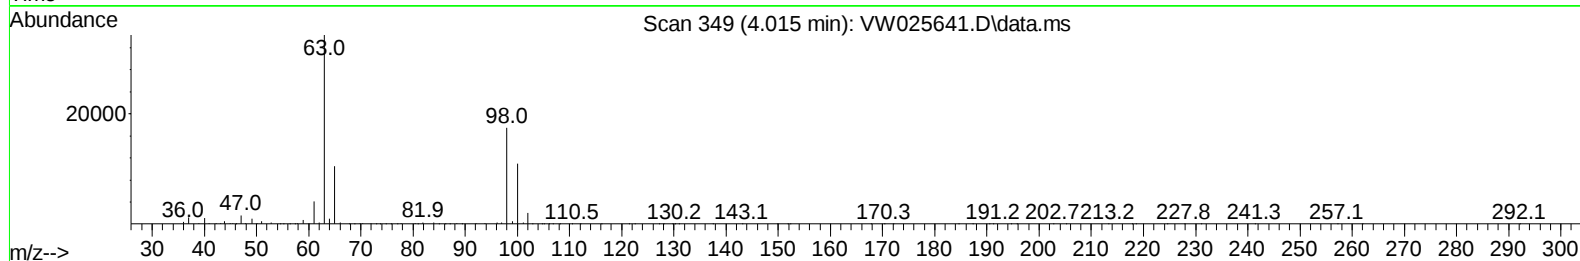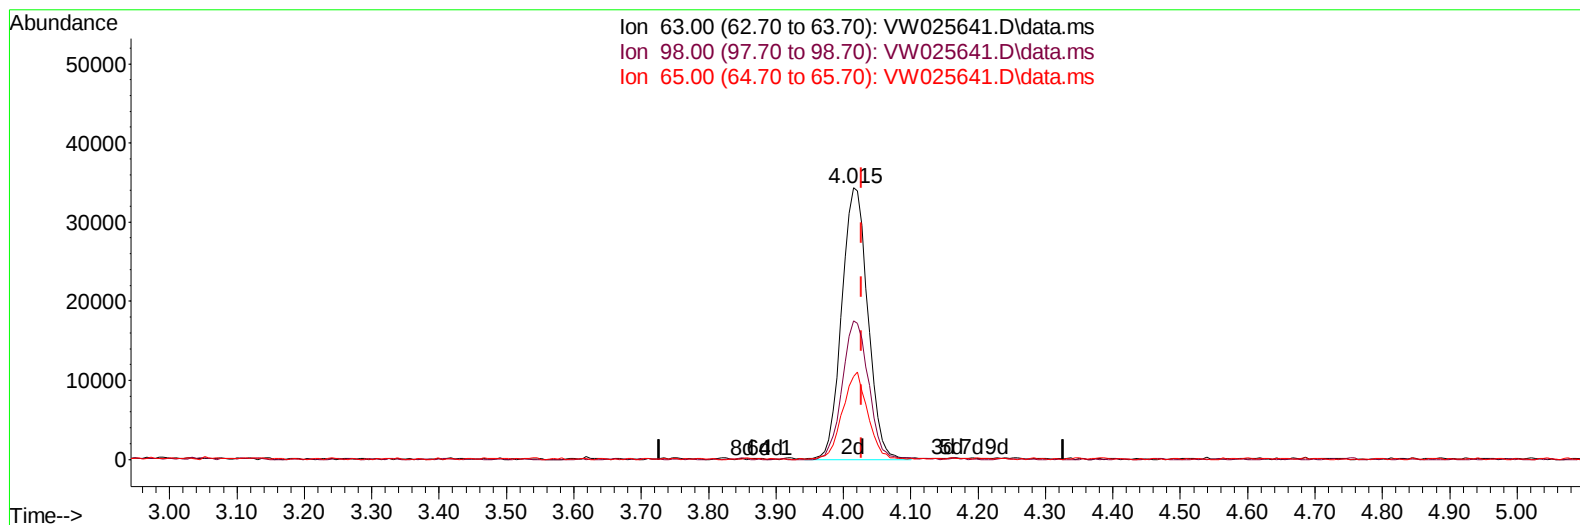

TIC: VW025641.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.015min (-0.012) 14.46 ug/L m

response 92095

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	0.10#
65.00	23.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025641.D
 Acq On : 21 Apr 2023 18:01
 Operator : SY/MD
 Sample : 02418-28
 Misc : 3.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW902

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:07:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	193578	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	142612	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	38853	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	53198	16.888	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	67.560%		
7) Chloroethane-d5	2.893	69	49083	21.885	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	87.560%		
11) 1,1-Dichloroethene-d2	4.015	63	92095m	14.457	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery =	57.840%		
21) 2-Butanone-d5	7.081	46	29890	42.534	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	85.060%		
24) Chloroform-d	7.648	84	133012	24.472	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	97.880%		
26) 1,2-Dichloroethane-d4	8.307	65	78062	27.607	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	110.440%		
32) Benzene-d6	8.276	84	244341	26.460	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	105.840%		
36) 1,2-Dichloropropane-d6	9.276	67	87551	30.407	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	121.640%#		
41) Toluene-d8	10.319	98	171481	21.259	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	85.040%		
43) trans-1,3-Dichloroprop...	10.581	79	21360	19.787	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	79.160%		
47) 2-Hexanone-d5	10.922	63	15903	40.408	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	80.820%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	62954	32.394	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	129.560%#		
66) 1,2-Dichlorobenzene-d4	13.855	152	31343	23.482	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	93.920%		
Target Compounds						
						Qvalue
13) Acetone	4.125	43	3029	5.093	ug/L	98
16) Methylene chloride	4.917	84	21734	7.063	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025641.D
Acq On : 21 Apr 2023 18:01
Operator : SY/MD
Sample : 02418-28
Misc : 3.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW902

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:07:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

