




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025642.D
Acq On : 21 Apr 2023 18:25
Operator : SY/MD
Sample : 02418-29
Misc : 5.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW903

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:07:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

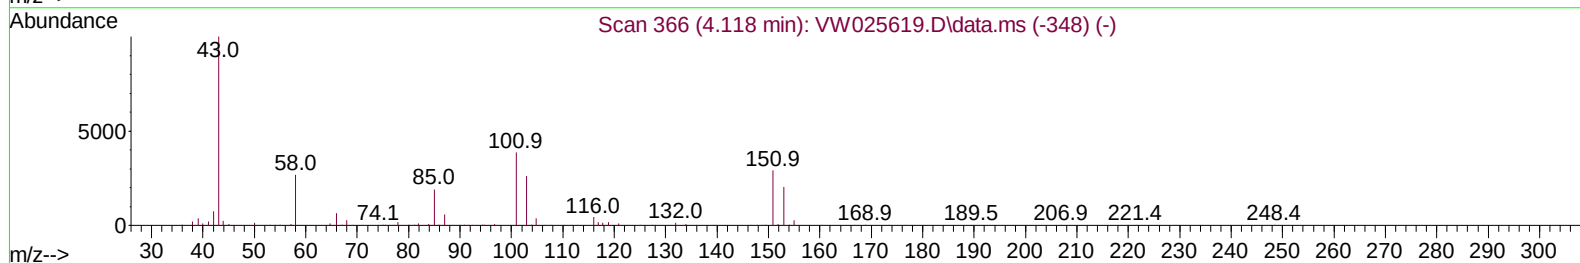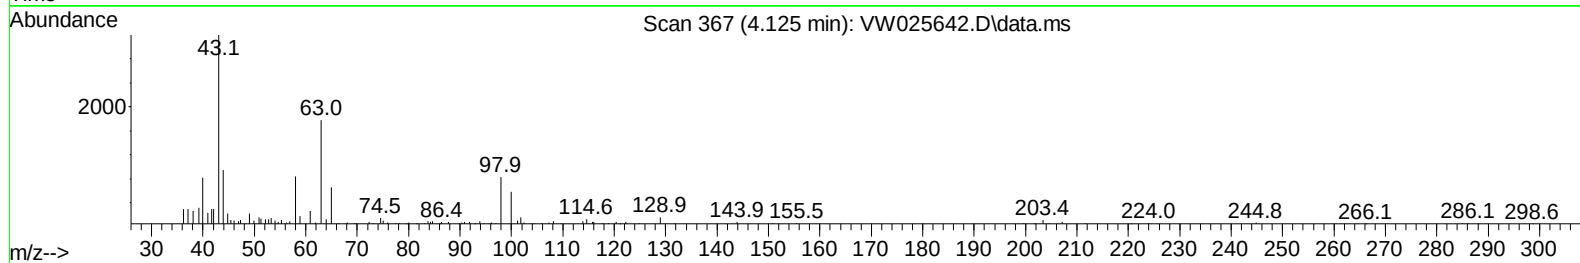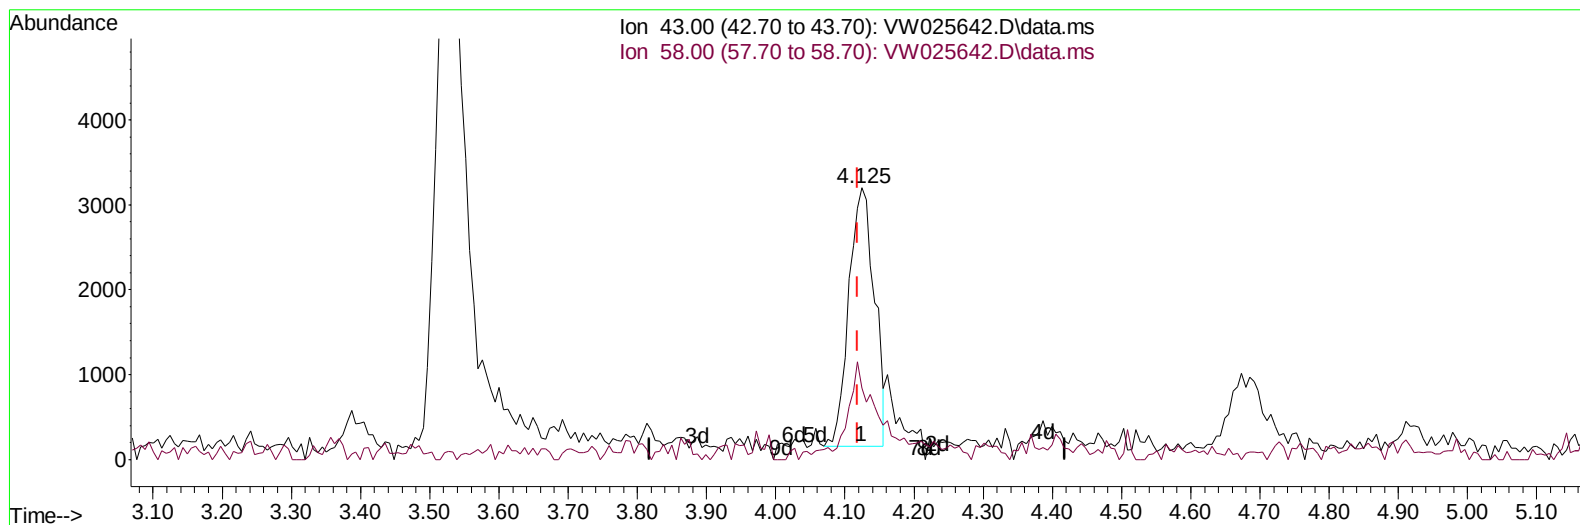

TIC: VW025642.D\data.ms

(13) Acetone (T)

4.125min (+ 0.007) 3.49 ug/L

response 7765

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.70	32.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025642.D
 Acq On : 21 Apr 2023 18:25
 Operator : SY/MD
 Sample : 02418-29
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW903

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:07:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

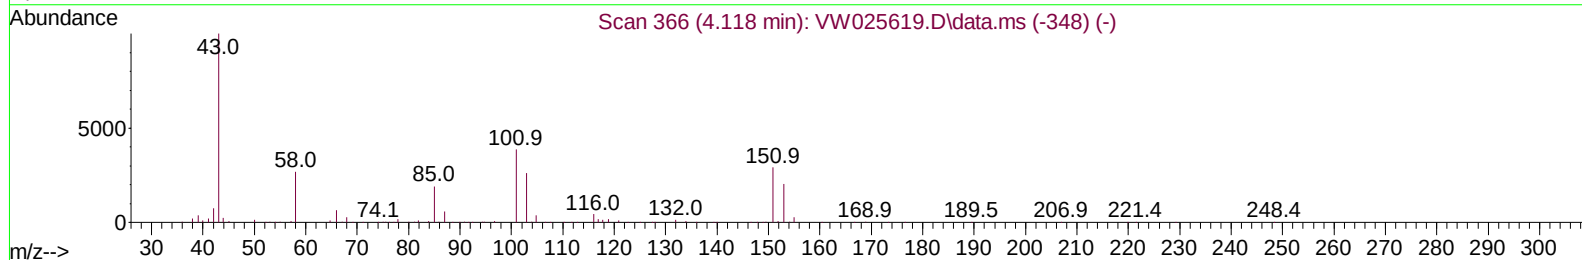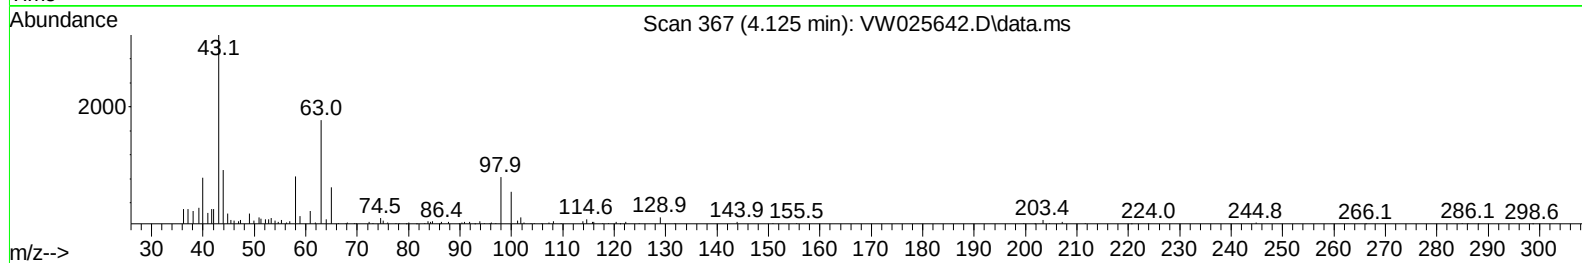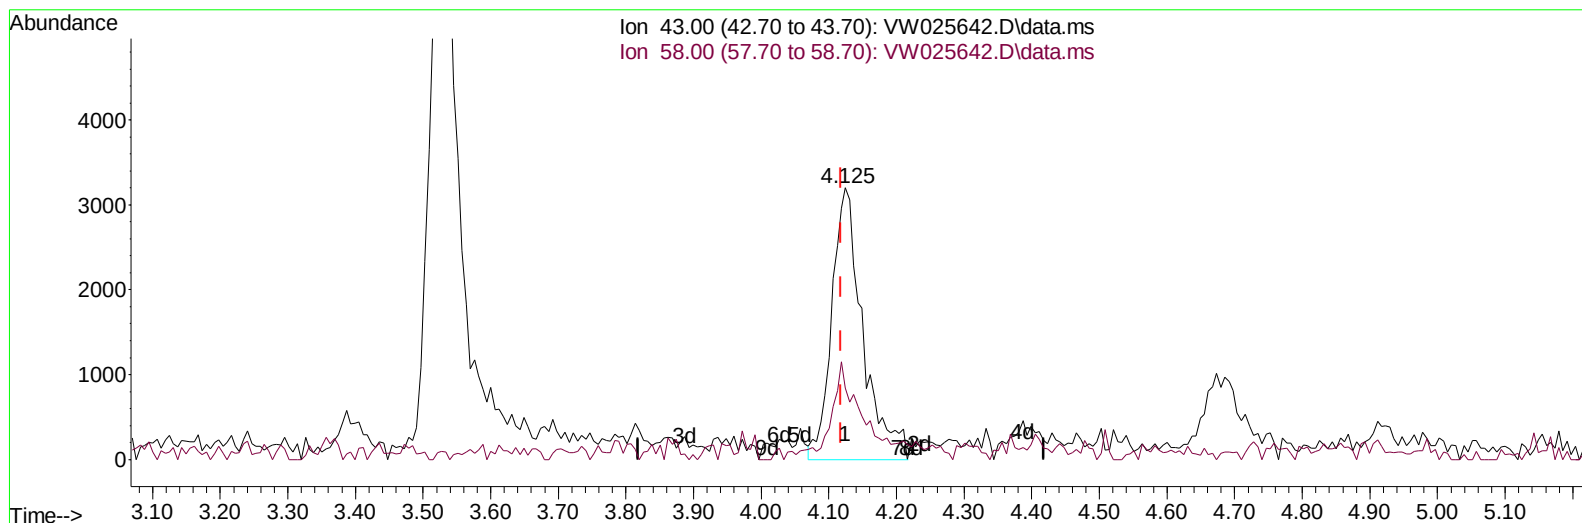

TIC: VW025642.D\data.ms

(13) Acetone (T)

4.125min (+ 0.007) 4.57 ug/L m

response 10161

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.70	24.64
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025642.D
 Acq On : 21 Apr 2023 18:25
 Operator : SY/MD
 Sample : 02418-29
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW903

Manual IntegrationsAPPROVED

Quant Time: Apr 22 05:07:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		724170	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		541522	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		151771	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		195319	16.575	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	66.280%		
7) Chloroethane-d5	2.899	69		179983	21.452	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	85.800%		
11) 1,1-Dichloroethene-d2	4.021	63		343532	14.415	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.640%		
21) 2-Butanone-d5	7.075	46		160557	61.073	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	122.140%		
24) Chloroform-d	7.648	84		534066	26.266	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	105.080%		
26) 1,2-Dichloroethane-d4	8.307	65		314828	29.762	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	119.040%		
32) Benzene-d6	8.276	84		1008411	28.759	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	115.040%		
36) 1,2-Dichloropropane-d6	9.270	67		358946	32.831	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	131.320%#		
41) Toluene-d8	10.325	98		792555	25.876	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	103.520%		
43) trans-1,3-Dichloroprop...	10.575	79		95758	23.361	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	93.440%		
47) 2-Hexanone-d5	10.922	63		89394	59.819	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	119.640%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		249175	33.767	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	135.080%#		
66) 1,2-Dichlorobenzene-d4	13.849	152		141137	27.069	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	108.280%		
Target Compounds							
13) Acetone	4.125	43		10161m	4.567	ug/L	
16) Methylene chloride	4.917	84		66777	5.801	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025642.D
Acq On : 21 Apr 2023 18:25
Operator : SY/MD
Sample : 02418-29
Misc : 5.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW903

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:07:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

