

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025627.D
 Acq On : 21 Apr 2023 12:27
 Operator : SY/MD
 Sample : 02418-08RE
 Misc : 3.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z4RE

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:04:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	590274	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	432849	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	127222	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	162241	16.891	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	67.560%	
7) Chloroethane-d5	2.899	69	148980	21.785	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	87.120%	
11) 1,1-Dichloroethene-d2	4.027	63	270919	13.947	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	55.800%	
21) 2-Butanone-d5	7.075	46	160051	74.691	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	149.380%#	
24) Chloroform-d	7.648	84	410471	24.767	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	99.080%	
26) 1,2-Dichloroethane-d4	8.307	65	241876m	28.053	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	112.200%	
32) Benzene-d6	8.276	84	782487	27.919	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	111.680%	
36) 1,2-Dichloropropane-d6	9.276	67	274957	31.463	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	125.840%#	
41) Toluene-d8	10.325	98	606504	24.773	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	99.080%	
43) trans-1,3-Dichloroprop...	10.581	79	81592	24.903	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	99.600%	
47) 2-Hexanone-d5	10.922	63	97382	81.525	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	163.040%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	194078	32.903	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	131.600%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	110688	25.325	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	101.320%	
Target Compounds						Qvalue
13) Acetone	4.118	43	238436	131.472	ug/L	98
16) Methylene chloride	4.923	84	40255	4.290	ug/L	98
22) 2-Butanone	7.173	43	97069	37.650	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025627.D
Acq On : 21 Apr 2023 12:27
Operator : SY/MD
Sample : 02418-08RE
Misc : 3.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW8Z4RE

Quant Time: Apr 22 05:04:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

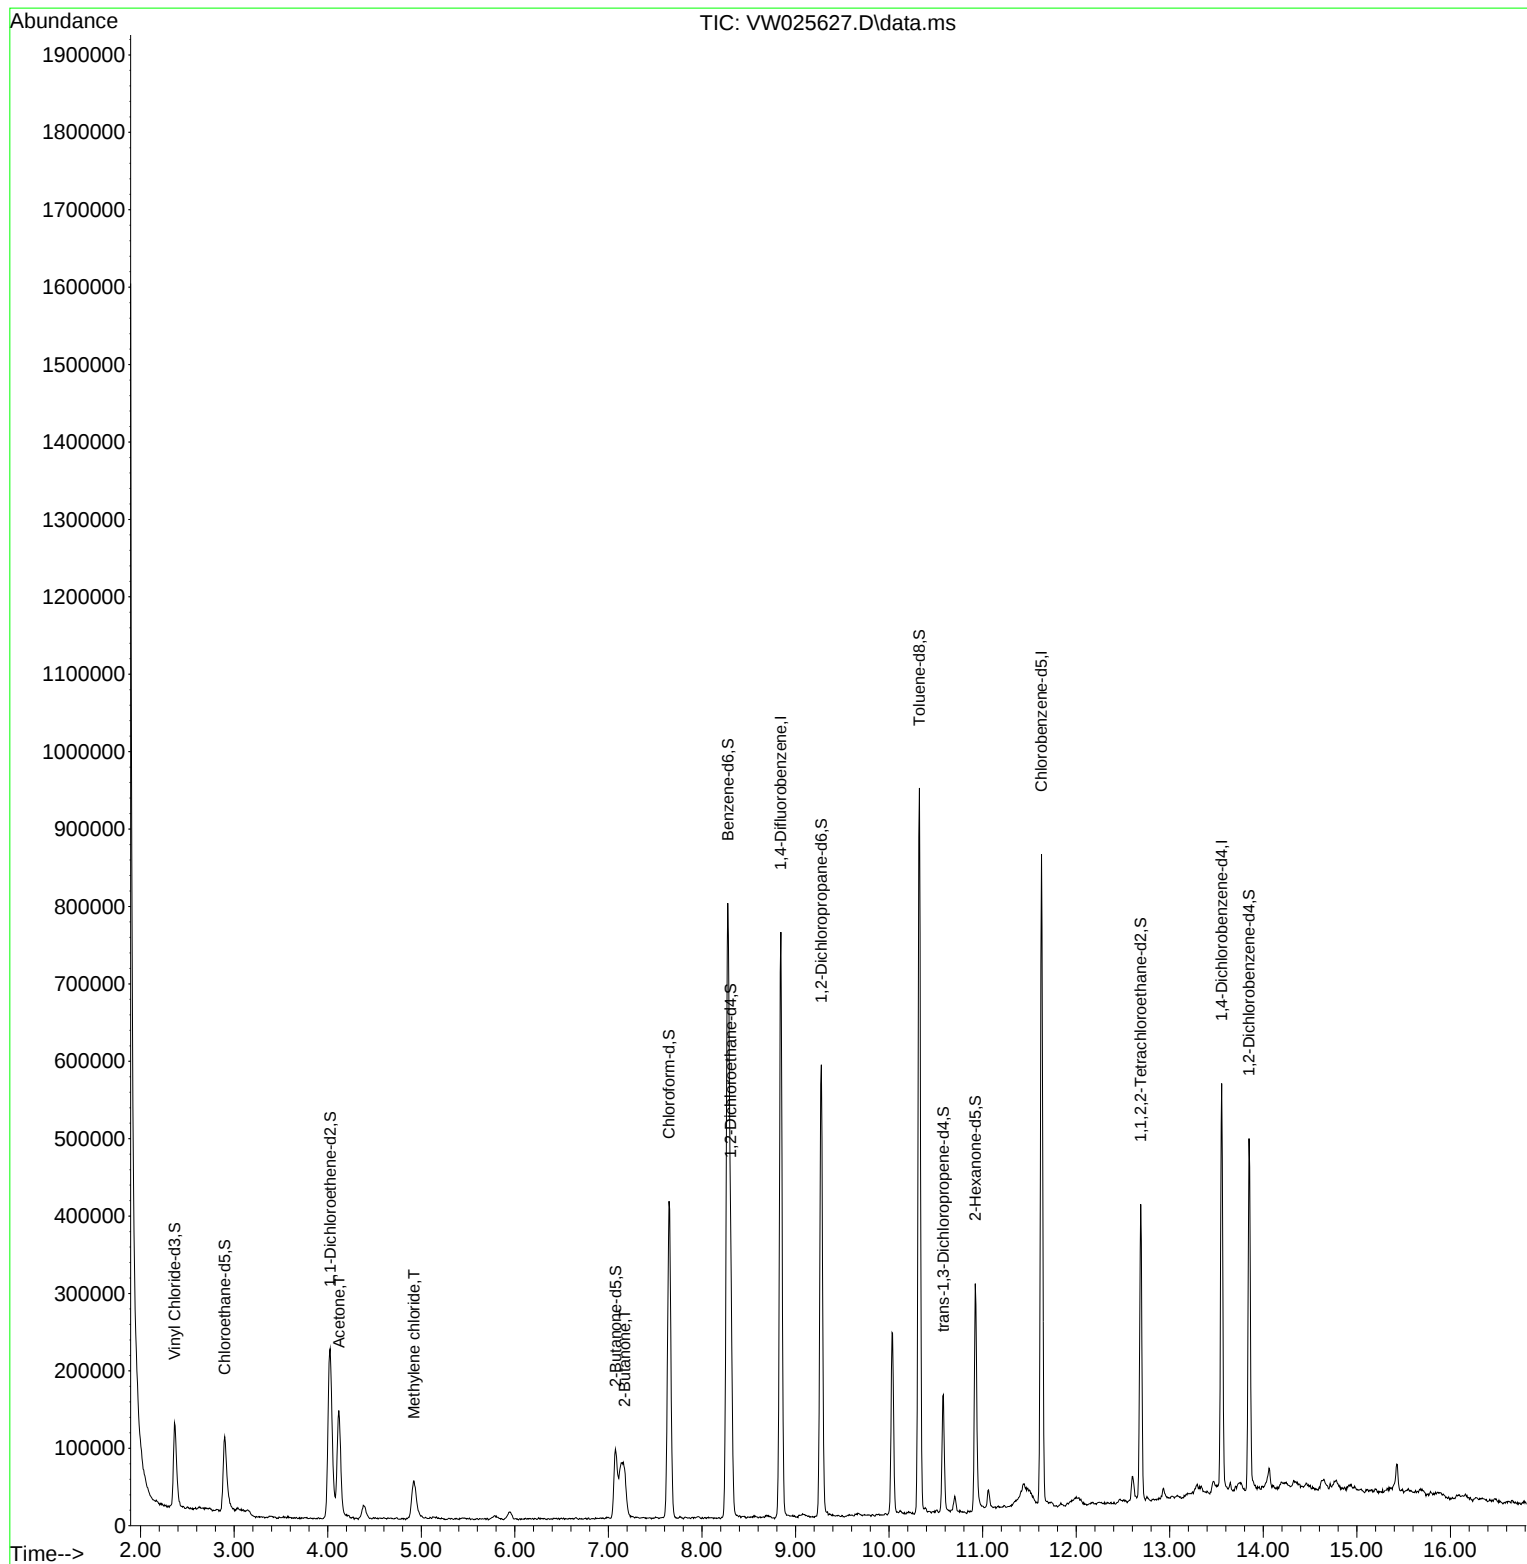

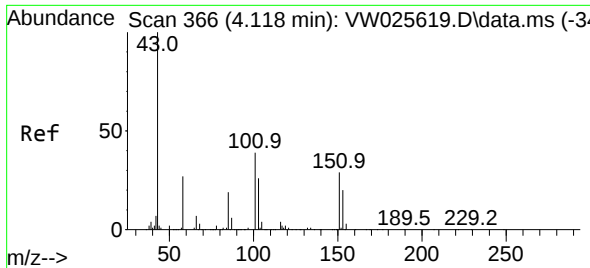





#13
Acetone
Concen: 131.472 ug/L
RT: 4.118 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW025627.D
Acq: 21 Apr 2023 12:27

Instrument :
MSVOA_W
ClientSampleId :
EW8Z4RE

Tgt Ion: 43 Resp: 238430
Ion Ratio Lower Upper
43 100
58 29.9 0.0 57.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

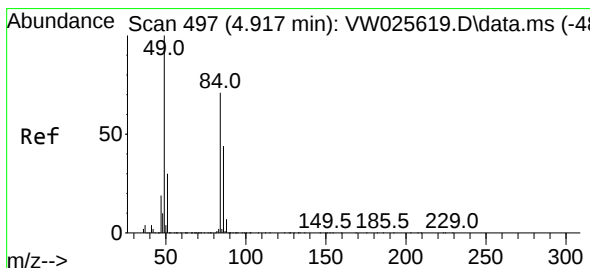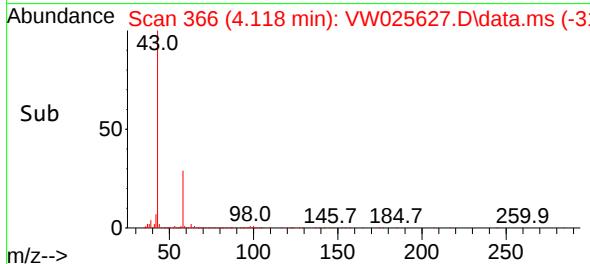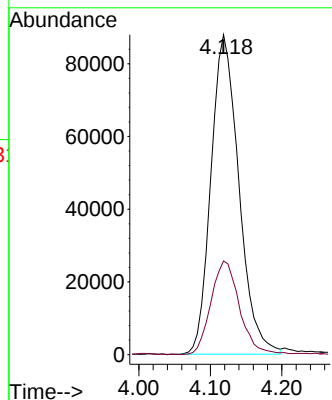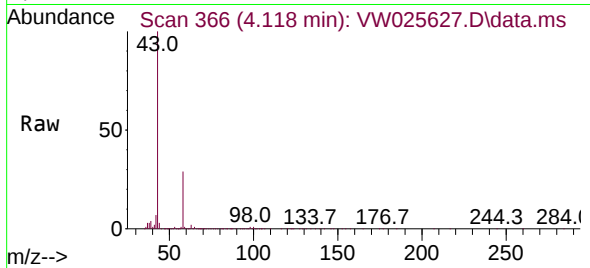

#16
Methylene chloride
Concen: 4.290 ug/L
RT: 4.923 min Scan# 498
Delta R.T. 0.006 min
Lab File: VW025627.D
Acq: 21 Apr 2023 12:27

Tgt Ion: 84 Resp: 40255
Ion Ratio Lower Upper
84 100
86 63.5 44.9 83.3
49 148.3 101.4 188.4

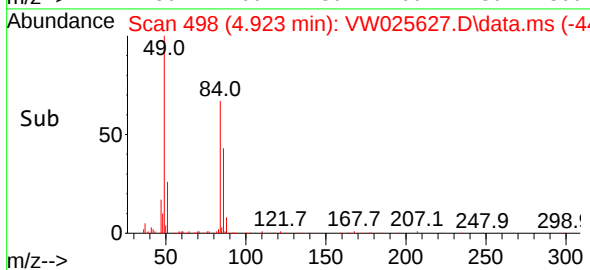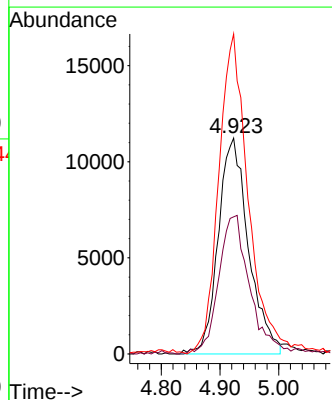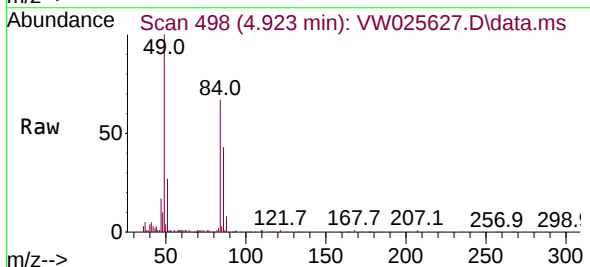

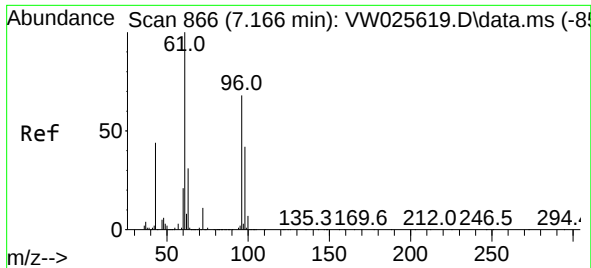

#22
 2-Butanone
 Concen: 37.650 ug/L
 RT: 7.173 min Scan# 80
 Delta R.T. 0.006 min
 Lab File: VW025627.D
 Acq: 21 Apr 2023 12:27

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8Z4RE

Tgt Ion: 43 Resp: 97069
 Ion Ratio Lower Upper
 43 100
 72 21.3 12.0 36.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

