

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
 Data File : VW025632.D
 Acq On : 21 Apr 2023 14:26
 Operator : SY/MD
 Sample : 02417-09
 Misc : 5.74g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/24/2023
 Supervised By : Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:05:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 05:02:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	64605	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	53953	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	16938	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	17060	16.227	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	64.920%	
7) Chloroethane-d5	2.887	69	18876	25.219	ug/L	-0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	100.880%	
11) 1,1-Dichloroethene-d2	4.021	63	32071	15.085	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	60.320%	
21) 2-Butanone-d5	7.088	46	16142m	68.826	ug/L	0.01
Spiked Amount	50.000	Range 20 - 135	Recovery	=	137.660%#	
24) Chloroform-d	7.648	84	50482	27.830	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	111.320%	
26) 1,2-Dichloroethane-d4	8.307	65	30651	32.480	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	129.920%	
32) Benzene-d6	8.276	84	90356	25.864	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	103.440%	
36) 1,2-Dichloropropane-d6	9.276	67	32962	30.260	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	121.040%#	
41) Toluene-d8	10.319	98	64013	20.976	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	83.920%	
43) trans-1,3-Dichloroprop...	10.581	79	10083	24.689	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	98.760%	
47) 2-Hexanone-d5	10.928	63	6741	45.275	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	90.540%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	25441	34.603	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	138.400%#	
66) 1,2-Dichlorobenzene-d4	13.855	152	14103	24.236	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	96.960%	
Target Compounds					Qvalue	
13) Acetone	4.131	43	3185	16.046	ug/L	81
16) Methylene chloride	4.923	84	4507m	4.389	ug/L	
34) Trichloroethene	9.093	95	2872	2.940	ug/L #	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042123\
Data File : VW025632.D
Acq On : 21 Apr 2023 14:26
Operator : SY/MD
Sample : 02417-09
Misc : 5.74g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW8X5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

Quant Time: Apr 22 05:05:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 05:02:40 2023
Response via : Initial Calibration

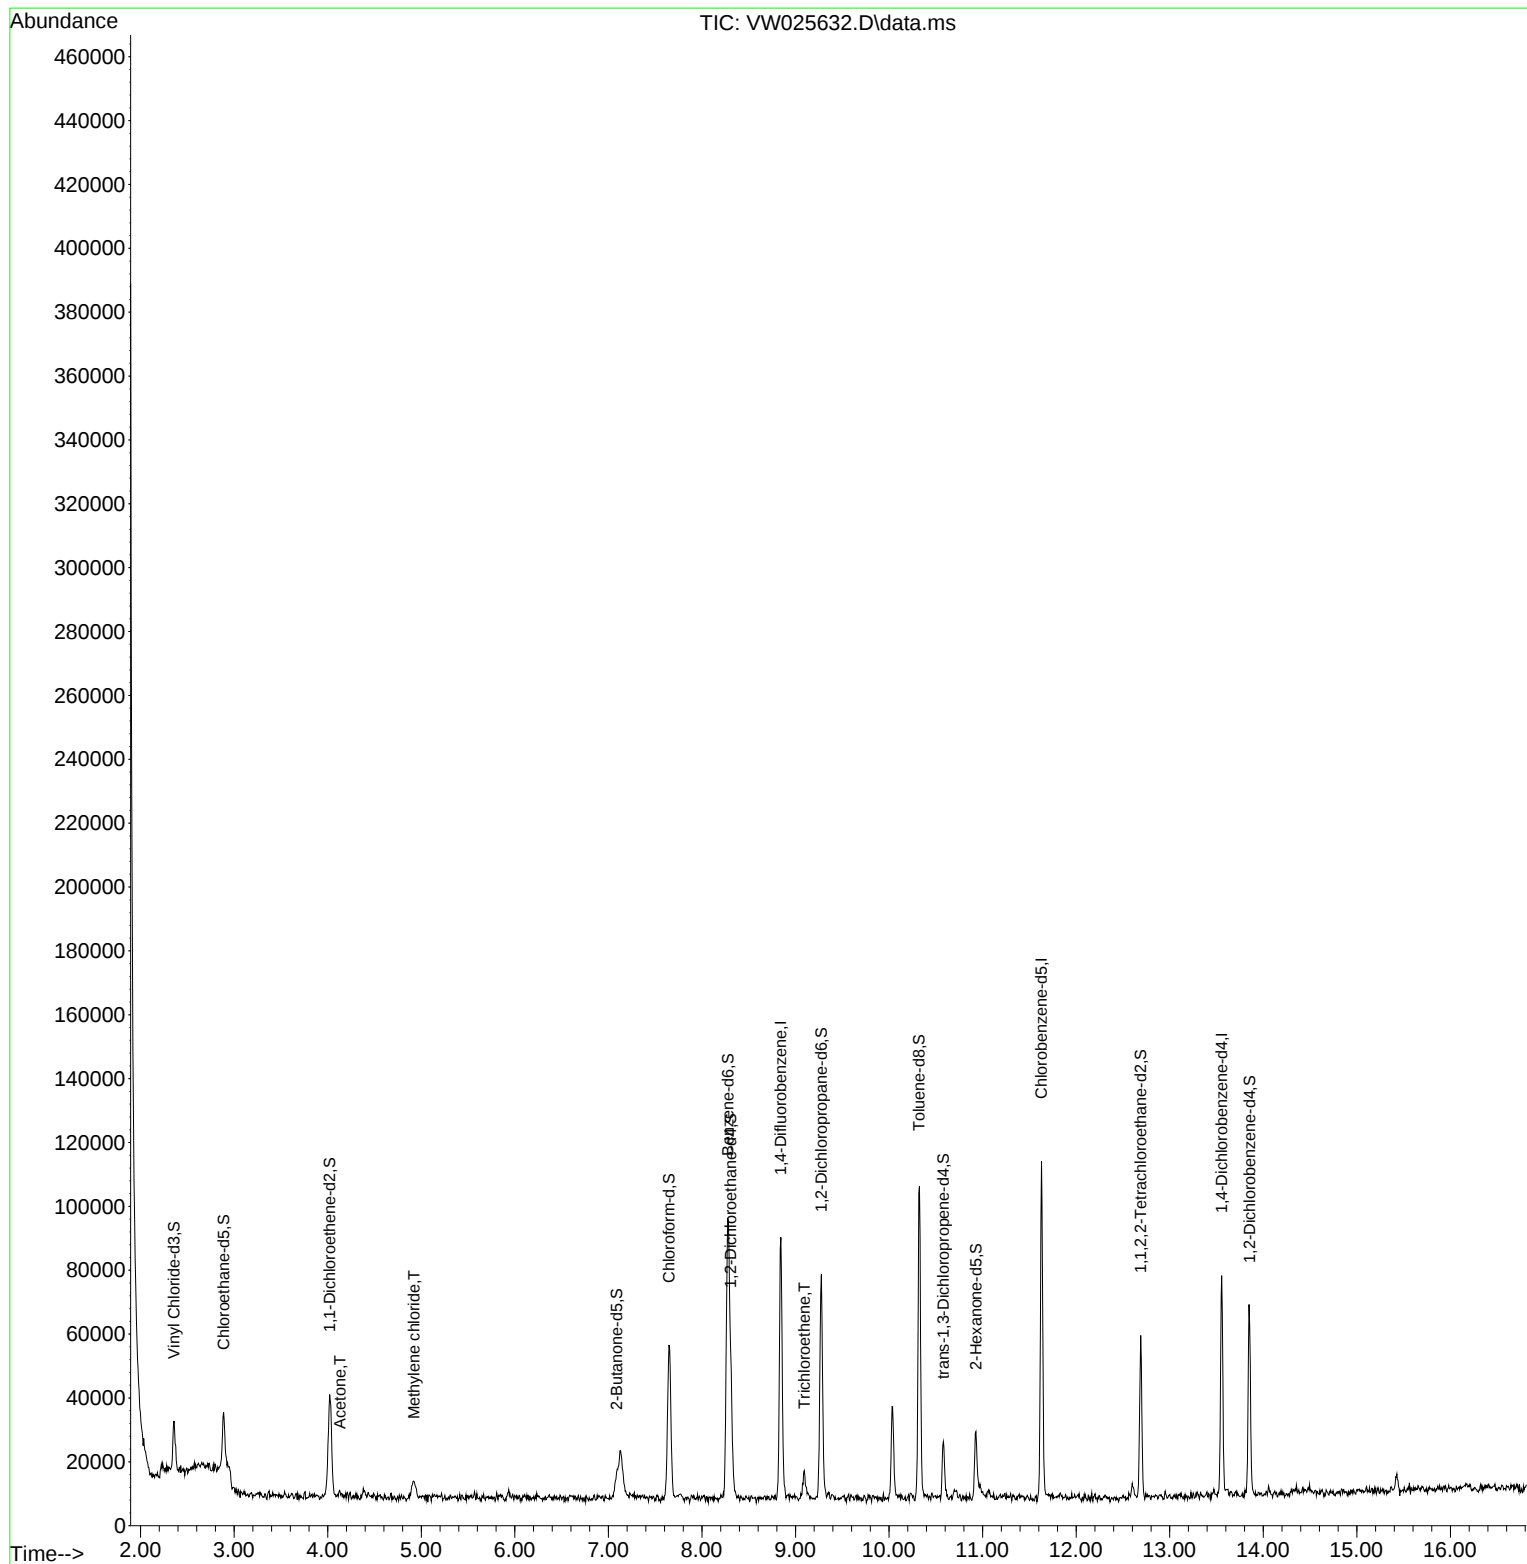

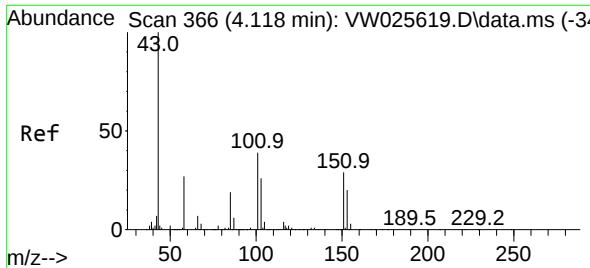





#13
Acetone
Concen: 16.046 ug/L
RT: 4.131 min Scan# 30
Delta R.T. 0.013 min
Lab File: VW025632.D
Acq: 21 Apr 2023 14:26

Instrument :
MSVOA_W
ClientSampleId :
EW8X5

Tgt Ion: 43 Resp: 318
Ion Ratio Lower Upper
43 100
58 18.5 0.0 57.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/24/2023
Supervised By :Mahesh Dadoda 04/24/2023

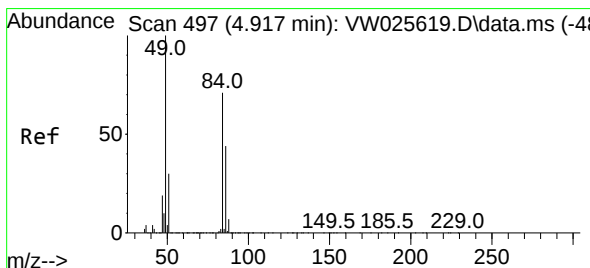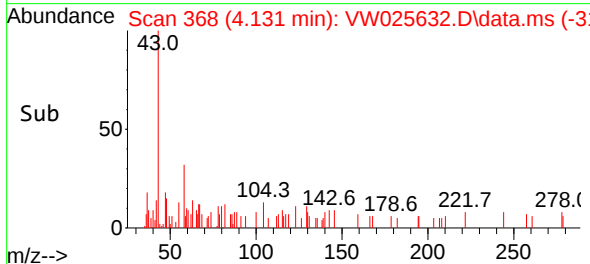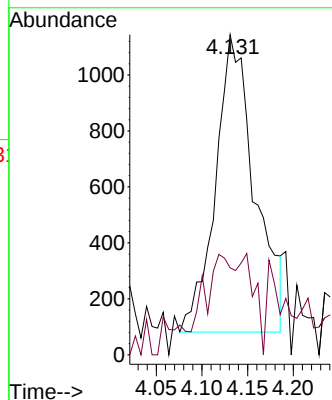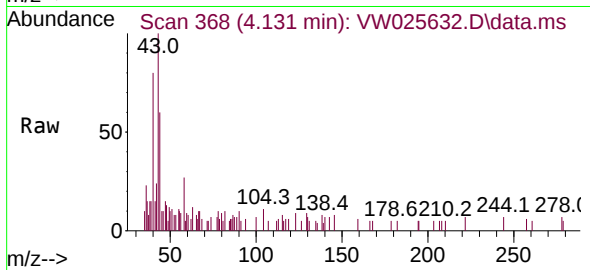

#16
Methylene chloride
Concen: 4.389 ug/L m
RT: 4.923 min Scan# 498
Delta R.T. 0.007 min
Lab File: VW025632.D
Acq: 21 Apr 2023 14:26


Tgt Ion: 84 Resp: 4507
Ion Ratio Lower Upper
84 100
86 87.1 44.9 83.3#
49 144.6 101.4 188.4

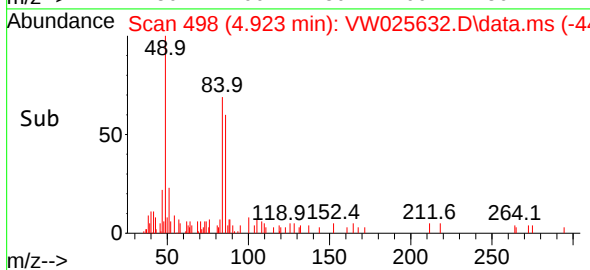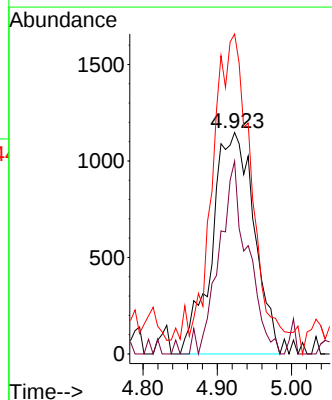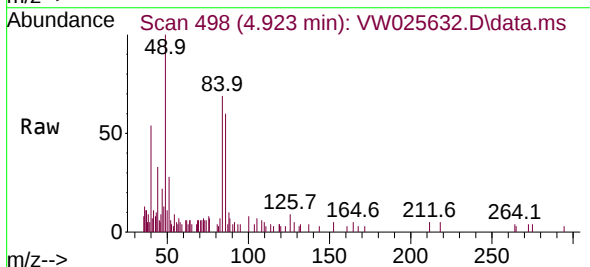

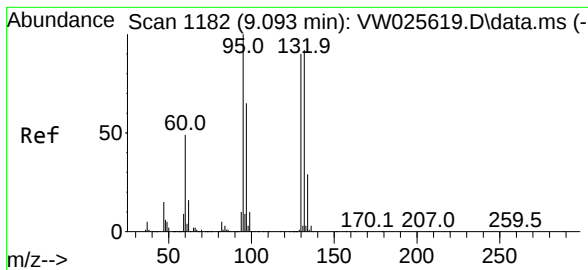

#34
 Trichloroethene
 Concen: 2.940 ug/L
 RT: 9.093 min Scan# 1182
 Delta R.T. 0.000 min
 Lab File: VW025632.D
 Acq: 21 Apr 2023 14:26

Instrument :
 MSVOA_W
 ClientSampleId :
 EW8X5

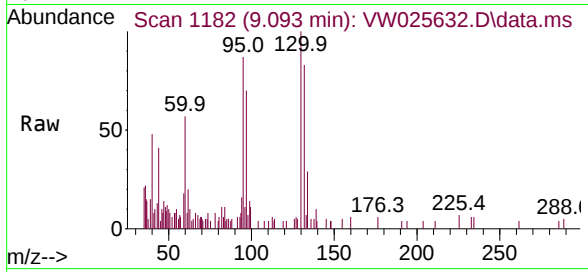

Tgt Ion: 95	Resp:	287
Ion Ratio	Lower	Upper
95	100	
97	80.3	42.5 78.9
132	95.2	59.8 111.1
130	114.6	65.7 122.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2023
 Supervised By :Mahesh Dadoda 04/24/2023

