


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW042219\
Data File : VW010083.D
Acq On : 22 Apr 2019 15:09
Operator : SY/VA
Sample : K2455-10
Misc : 5.10G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHR0

Manual Integrations
APPROVED

MMDadoda
4/24/2019 12:34:02 AM

Quant Time: Apr 23 07:19:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 23 06:06:04 2019
Response via : Initial Calibration

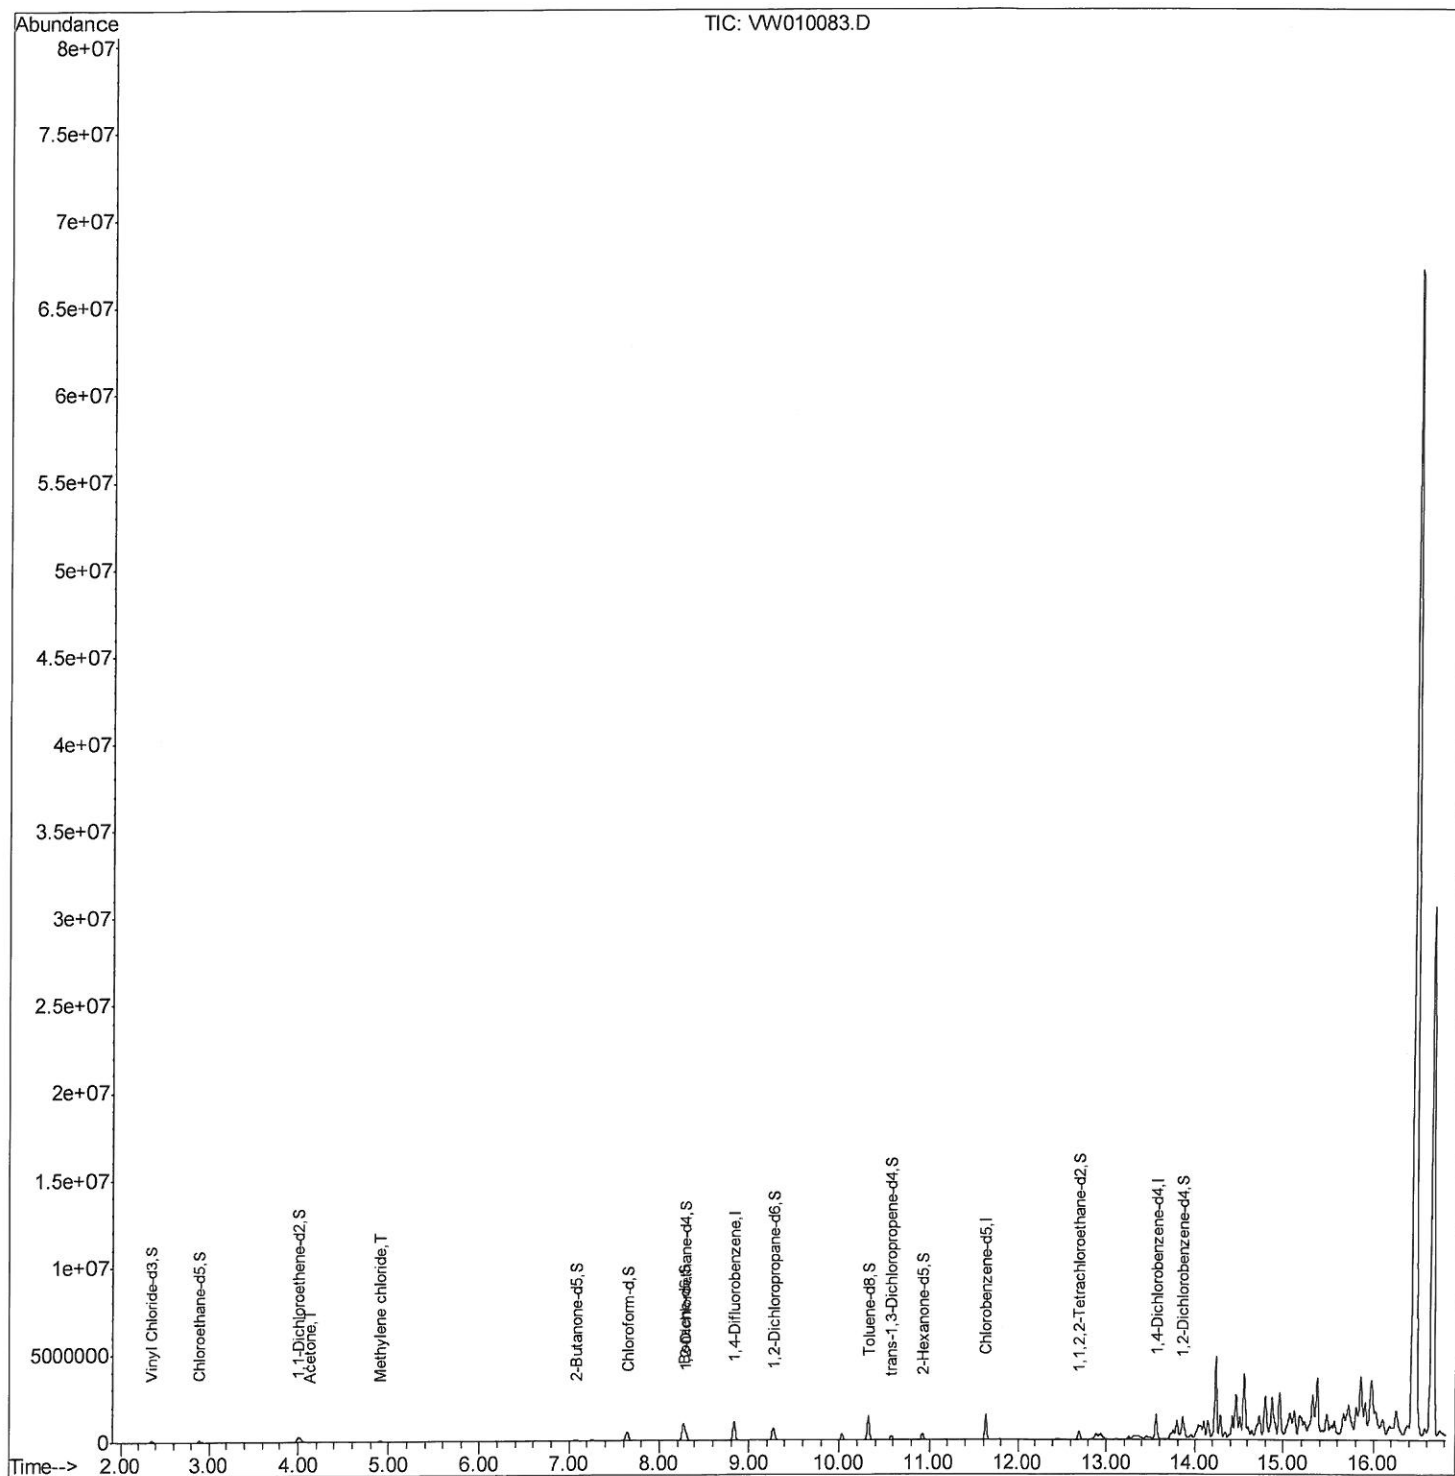

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW042219\
 Data File : VW010083.D
 Acq On : 22 Apr 2019 15:09
 Operator : SY/VA
 Sample : K2455-10
 Misc : 5.10G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 GAHR0

Manual Integrations
APPROVED

MMDadoda
 4/24/2019 12:34:02 AM

Quant Time: Apr 23 06:09:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 23 06:06:04 2019
 Response via : Initial Calibration

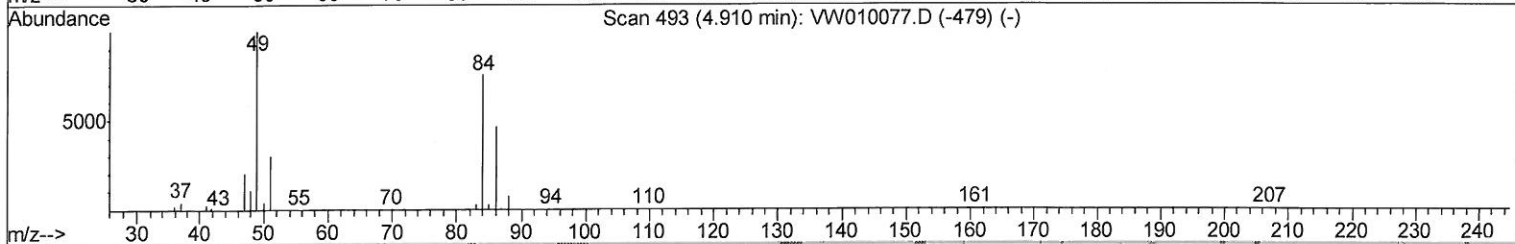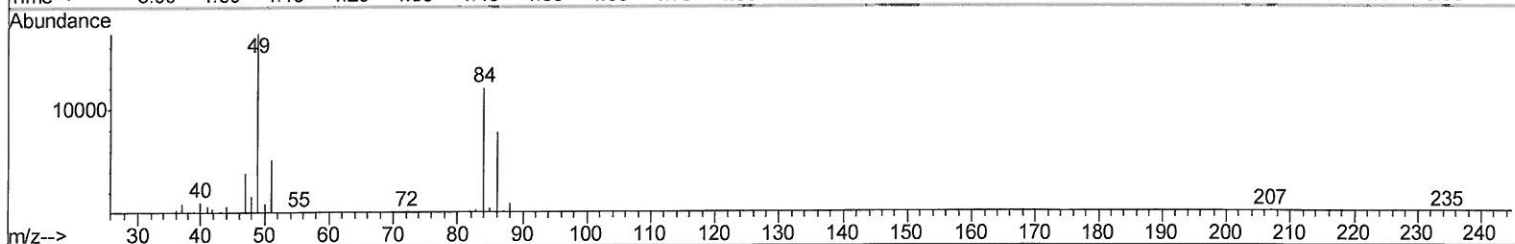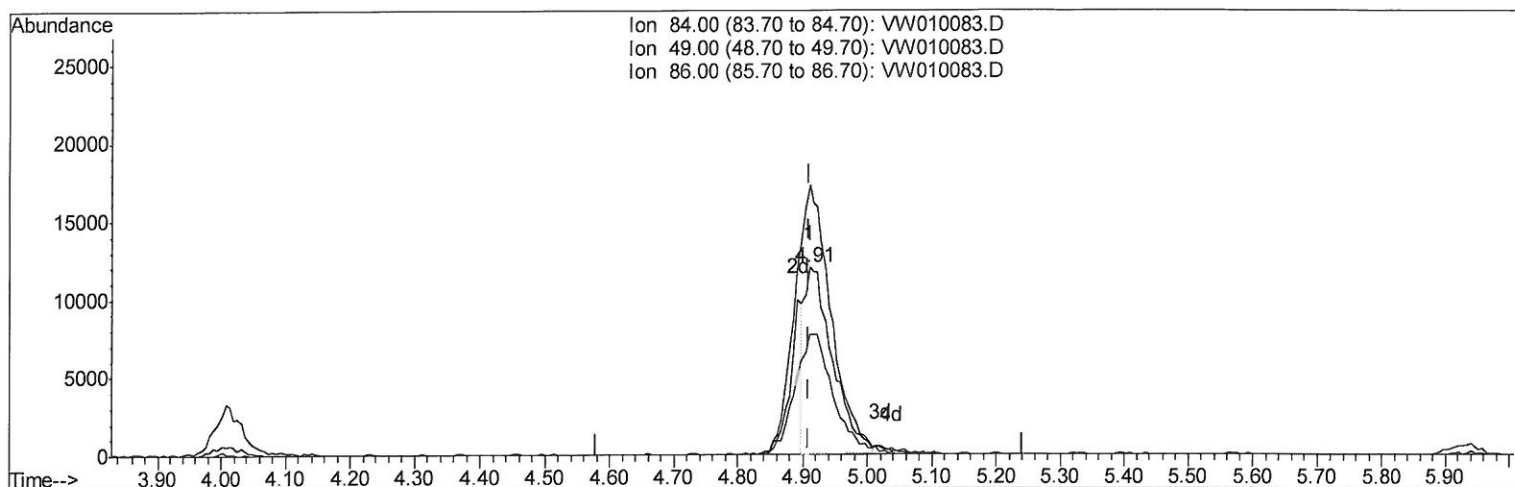

TIC: VW010083.D

(16) Methylene chloride (T)

4.909min (-0.000) 2.26ug/L

response 35565

Ion	Exp%	Act%
84.00	100	100
49.00	143.90	143.89
86.00	62.50	64.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW042219\
 Data File : VW010083.D
 Acq On : 22 Apr 2019 15:09
 Operator : SY/VA
 Sample : K2455-10
 Misc : 5.10G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHR0

Manual Integrations
 APPROVED

MMDadoda
 4/24/2019 12:34:02 AM

Quant Time: Apr 23 06:09:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 23 06:06:04 2019
 Response via : Initial Calibration

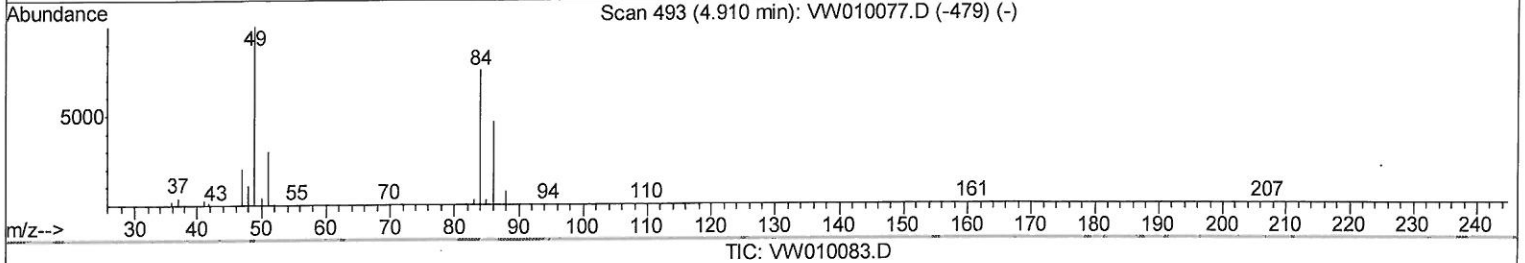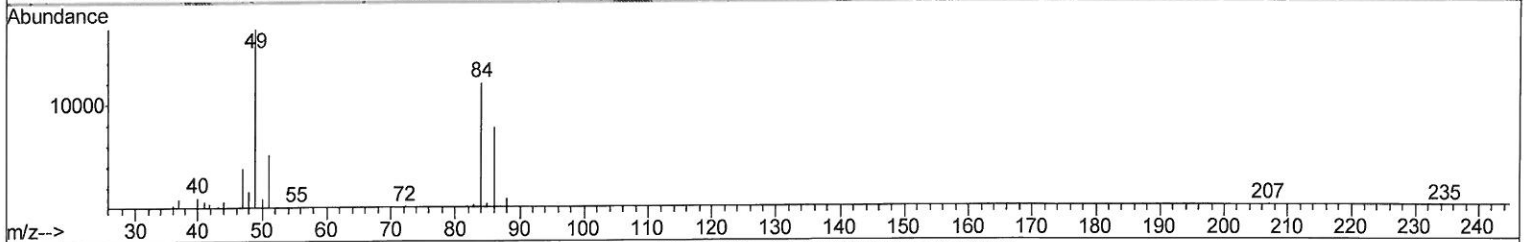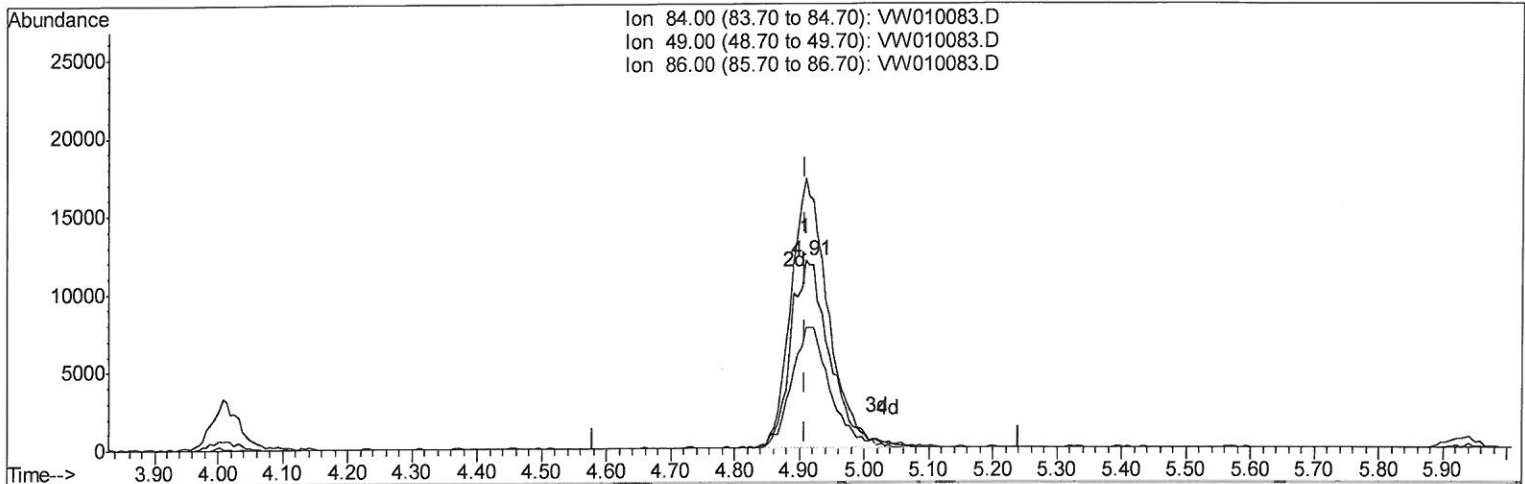

(16) Methylene chloride (T)

4.909min (-0.000) 3.19ug/L m

response 50293

MMD
4/26/19

Ion	Exp%	Act%
84.00	100	100
49.00	143.90	143.89
86.00	62.50	64.39
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW042219\
 Data File : VW010083.D
 Acq On : 22 Apr 2019 15:09
 Operator : SY/VA
 Sample : K2455-10
 Misc : 5.10G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHR0

Manual Integrations
 APPROVED

MMDadoda
 4/24/2019 12:34:02 AM

Quant Time: Apr 23 07:19:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041519S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 23 06:06:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	869920	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	790193	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	354878	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	170474	20.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.96%
7) Chloroethane-d5	2.89	69	142930	17.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.68%
10) 1,1-Dichloroethene-d2	4.01	63	358473	15.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.88%
20) 2-Butanone-d5	7.08	46	148644	33.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.86%
24) Chloroform-d	7.64	84	506877	20.15	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.60%
26) 1,2-Dichloroethane-d4	8.30	65	285981	18.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.32%
29) Benzene-d6	8.27	84	992410	22.85	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.40%
33) 1,2-Dichloropropane-d6	9.27	67	310089	22.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.68%
37) Toluene-d8	10.32	98	890585	22.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.92%
38) trans-1,3-Dichloropropene-	10.58	79	127529	19.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.80%
39) 2-Hexanone-d5	10.93	63	112850	36.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.64%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	225458	17.43	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	69.72%
61) 1,2-Dichlorobenzene-d4	13.86	152	293679	22.01	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.04%

Target Compounds

					Qvalue
13) Acetone	4.12	43	11323	2.863	ug/L 96
16) Methylene chloride	4.91	84	50293m	3.193	ug/L

> MD
 4/26/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed