

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042221\
 Data File : VW018732.D
 Acq On : 22 Apr 2021 13:30
 Operator : SY/VA
 Sample : M2129-08
 Misc : 5.82G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AC4

Manual Integrations
 APPROVED

MMDadoda
 4/26/2021 5:29:24 PM

Quant Time: Apr 23 02:02:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 23 01:53:36 2021
 Response via : Initial Calibration

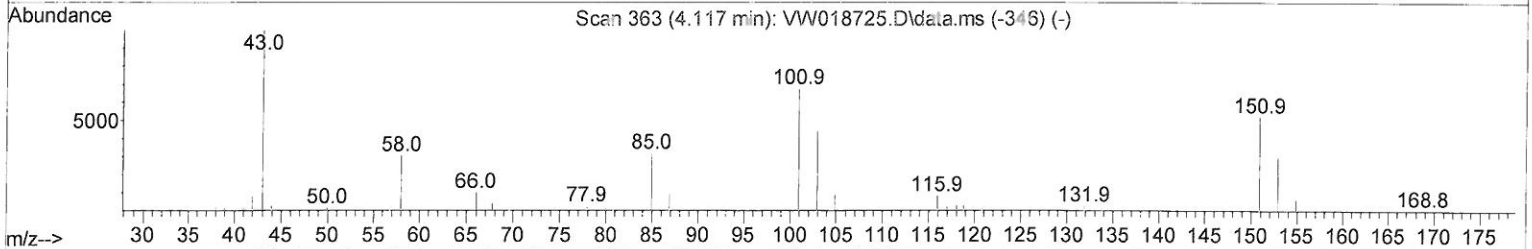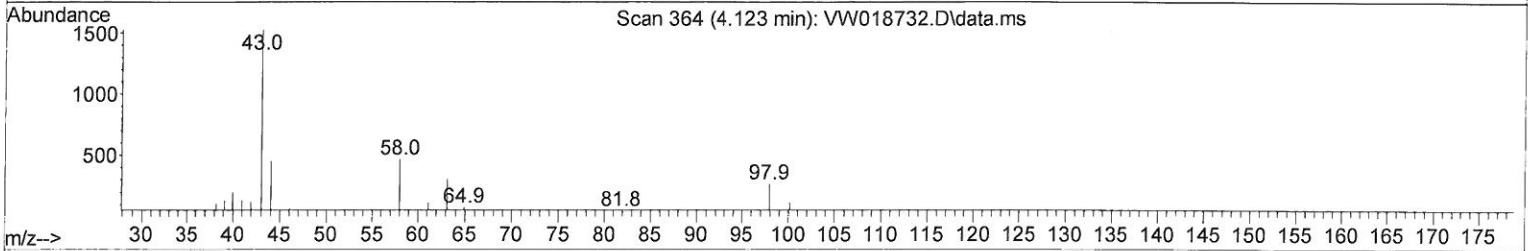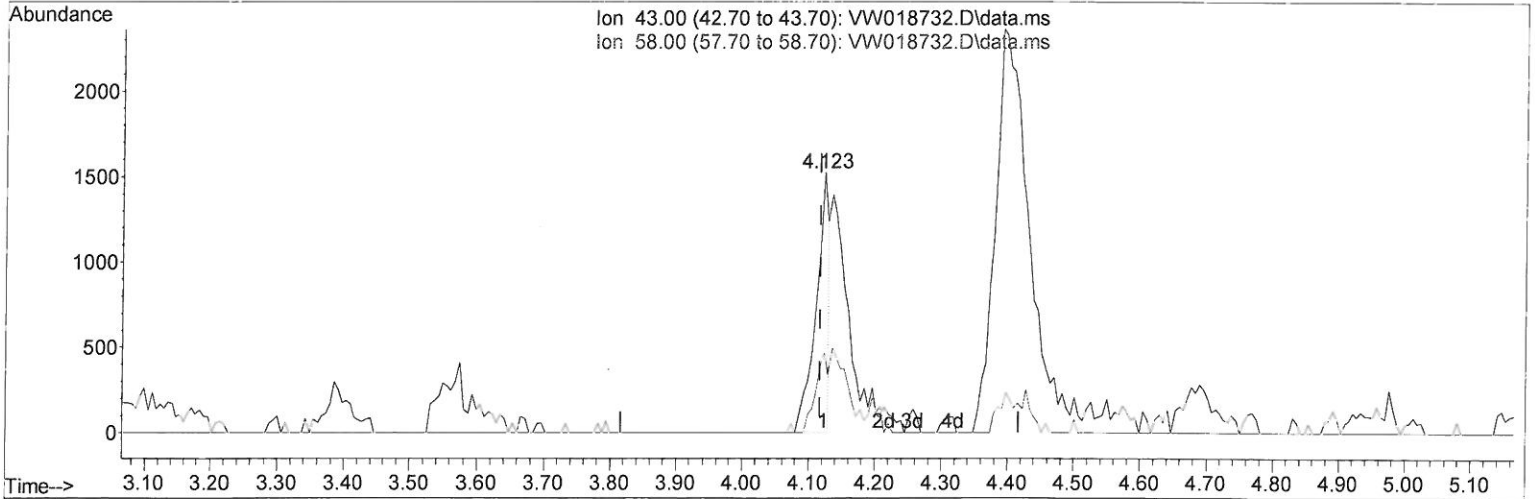

TIC: VW018732.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 1.50 ug/L

response 2062

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	29.49
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042221\
 Data File : VW018732.D
 Acq On : 22 Apr 2021 13:30
 Operator : SY/VA
 Sample : M2129-08
 Misc : 5.82G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AC4

Manual Integrations
 APPROVED

MMDadoda
 4/26/2021 5:29:24 PM

Quant Time: Apr 23 02:02:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 23 01:53:36 2021
 Response via : Initial Calibration

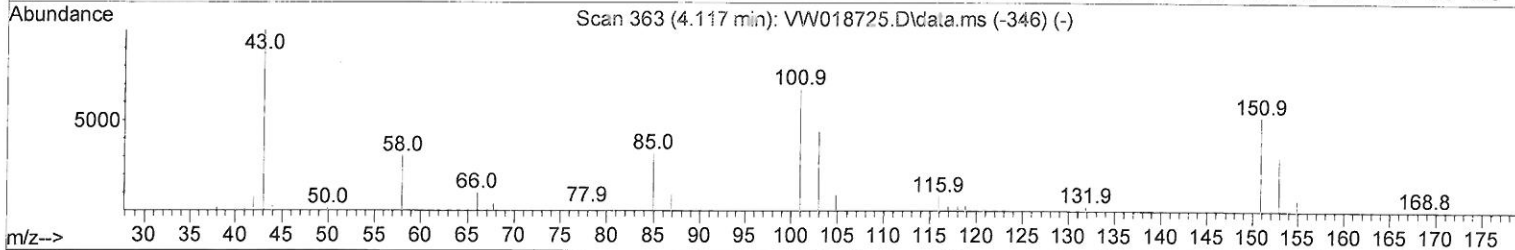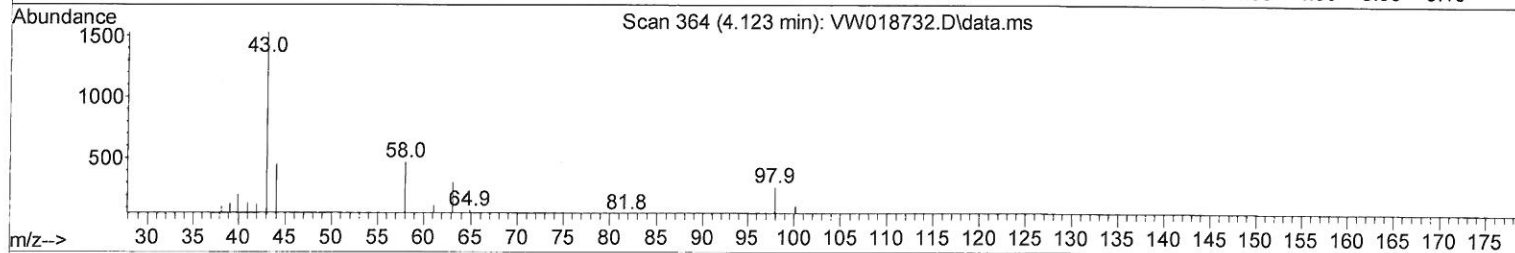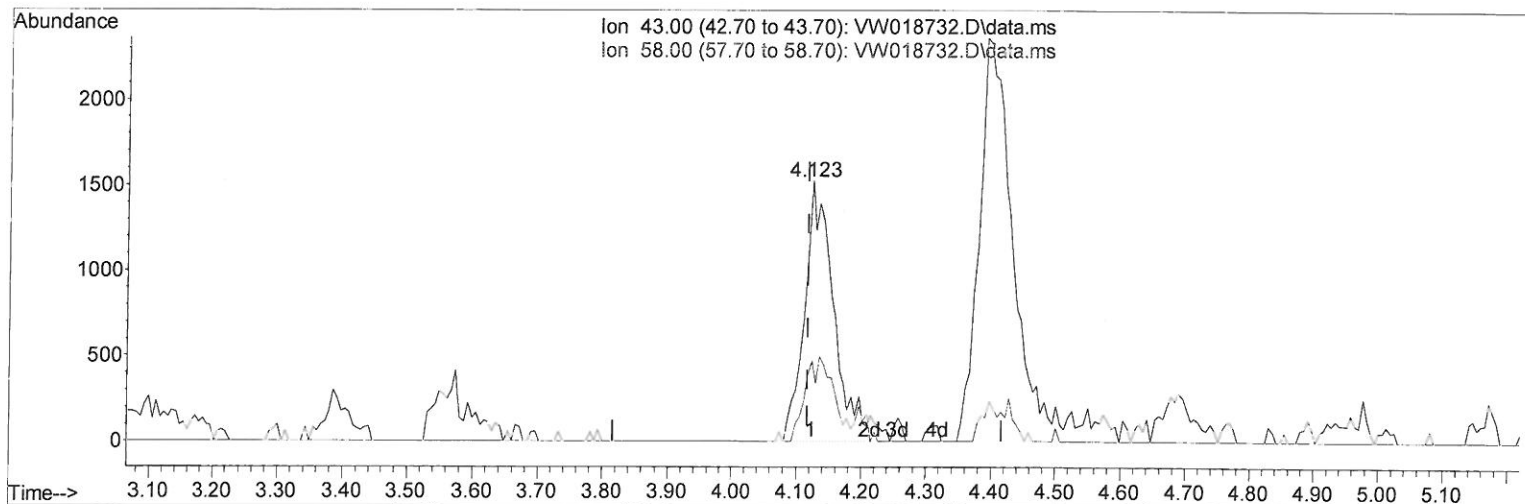

TIC: VW018732.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.46 ug/L m

response 4761

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	12.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042221\
 Data File : VW018732.D
 Acq On : 22 Apr 2021 13:30
 Operator : SY/VA
 Sample : M2129-08
 Misc : 5.82G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0AC4

Manual Integrations
 APPROVED

MMDadoda
 4/26/2021 5:29:24 PM

Quant Time: Apr 23 02:02:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 23 01:53:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	547967	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	440853	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	172640	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	97049	11.65	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	46.60%	
7) Chloroethane-d5	2.891	69	89519	12.13	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	48.52%	
11) 1,1-Dichloroethene-d2	4.019	63	131578	9.10	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	36.40%#	
21) 2-Butanone-d5	7.086	46	47305	24.96	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	49.92%	
24) Chloroform-d	7.647	84	270850	18.01	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	72.04%	
26) 1,2-Dichloroethane-d4	8.305	65	147894	17.49	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	69.96%#	
32) Benzene-d6	8.274	84	442743	17.12	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	68.48%	
36) 1,2-Dichloropropane-d6	9.274	67	157692	20.23	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	80.92%	
41) Toluene-d8	10.323	98	359803	15.21	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	60.84%	
43) trans-1,3-Dichloroprop...	10.579	79	46995	14.16	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	56.64%	
47) 2-Hexanone-d5	10.926	63	39261	28.97	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	57.94%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	121690	18.70	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	74.80%	
66) 1,2-Dichlorobenzene-d4	13.853	152	119276	19.67	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	78.68%	

Target Compounds

13) Acetone	4.123	43	4761m	>	3.46 ug/L	Qvalue
-------------	-------	----	-------	---	-----------	--------

04/28/21 SY

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042221\
Data File : VW018732.D
Acq On : 22 Apr 2021 13:30
Operator : SY/VA
Sample : M2129-08
Misc : 5.82G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0AC4

Manual Integrations
APPROVED

MMDadoda
4/26/2021 5:29:24 PM

Quant Time: Apr 23 02:02:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 23 01:53:36 2021
Response via : Initial Calibration

