

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042320\
 Data File : VW015322.D
 Acq On : 23 Apr 2020 10:41
 Operator : SY/VA
 Sample : VW0423SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0423SBL01

Quant Time: Apr 24 07:01:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W042020S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 21 06:39:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	217506	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	295985	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	262292	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	114228	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	85619	48.14	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.28%	
35) Dibromofluoromethane	7.88	113	85781	52.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.64%	
50) Toluene-d8	10.32	98	354865	51.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.90%	
62) 4-Bromofluorobenzene	12.62	95	116805	44.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.78%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW042320\
Data File : VW015322.D
Acq On : 23 Apr 2020 10:41
Operator : SY/VA
Sample : VW0423SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0423SBL01

Quant Time: Apr 24 07:01:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W042020S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 21 06:39:58 2020
Response via : Initial Calibration

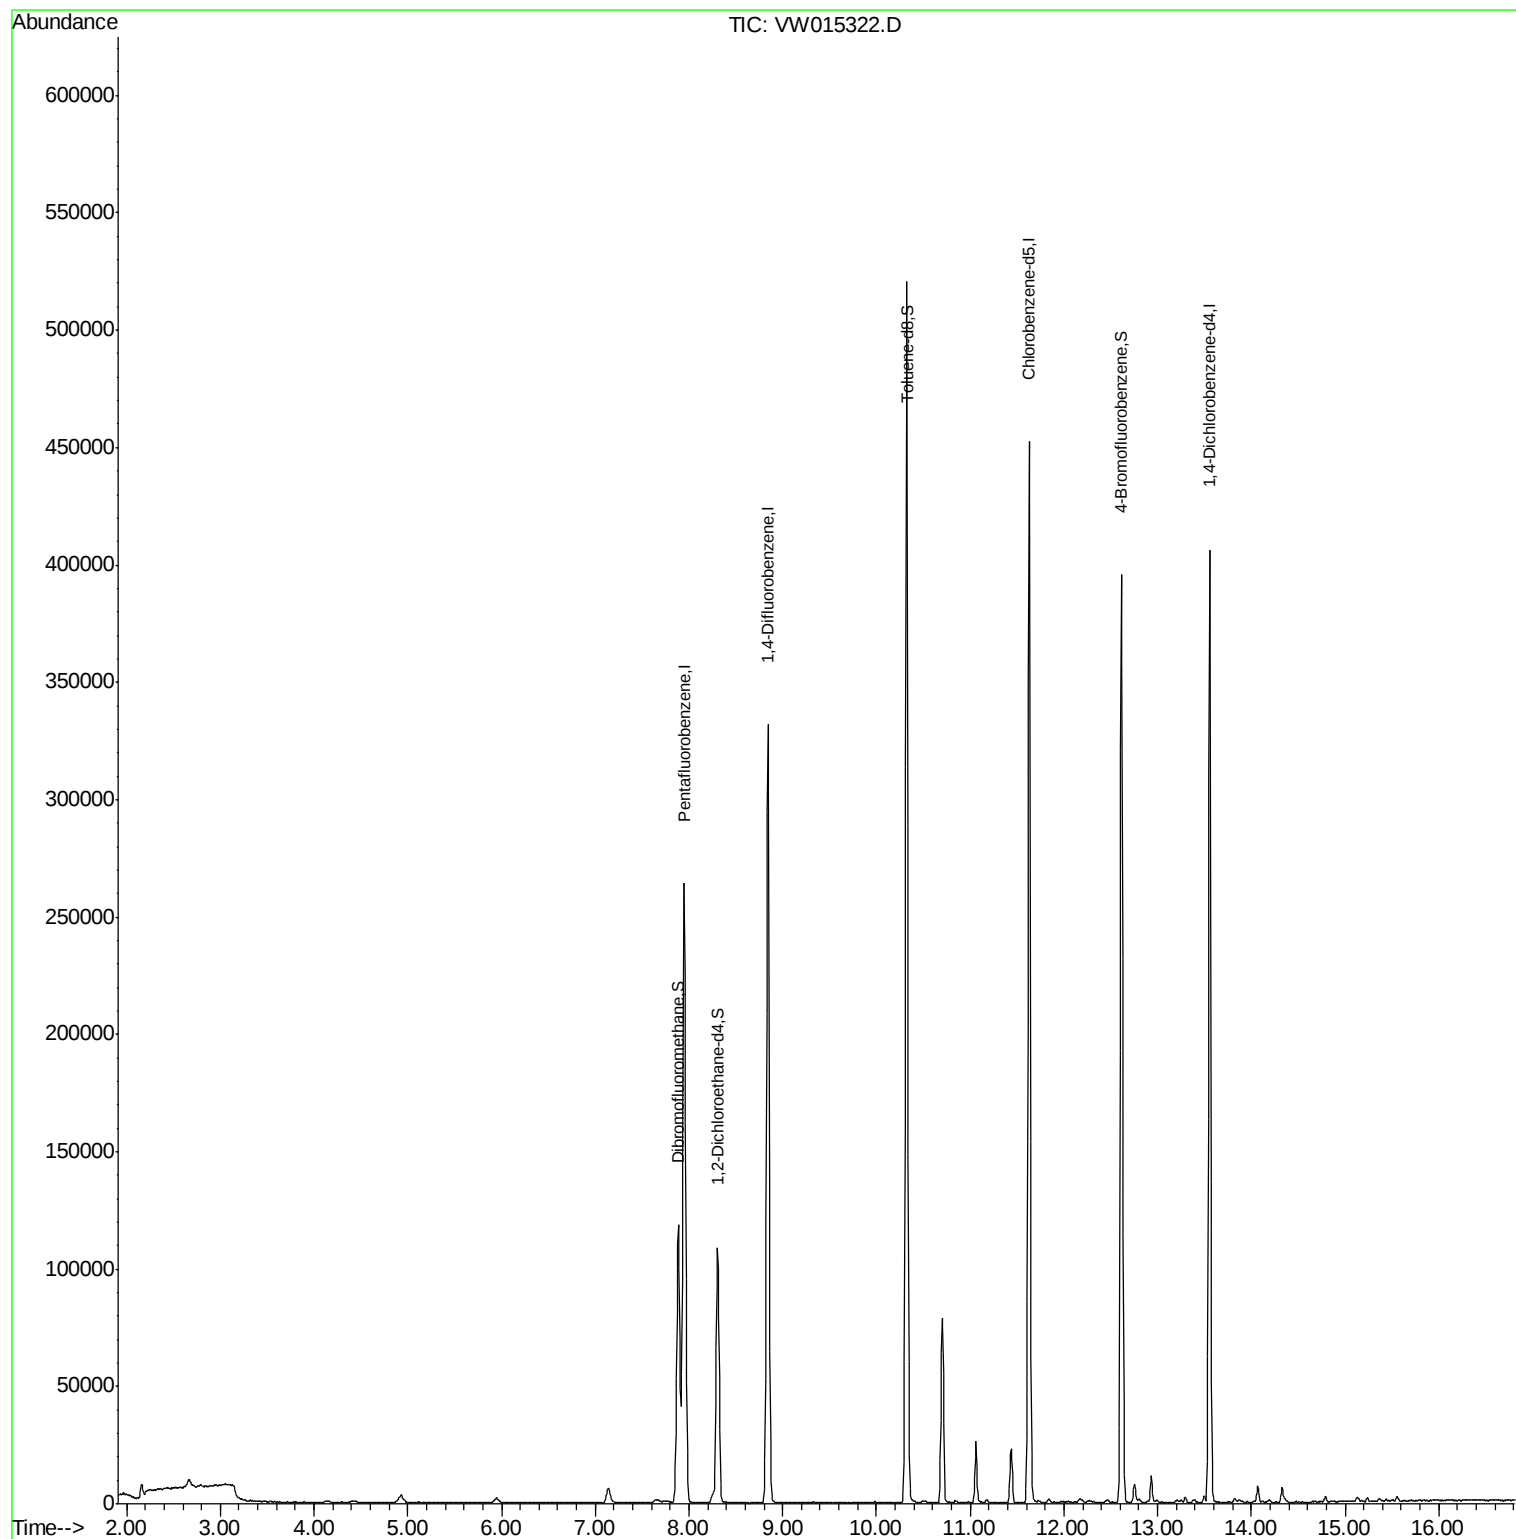

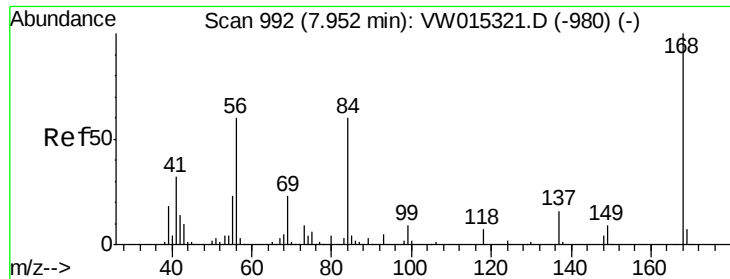

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41

Instrument :

MSVOA_W

ClientSampled :


VW0423SBL01

Tot Ion:168 Resp: 217506

Ion Ratio Lower Upper




168 100

99 49.3 48.5 72.7

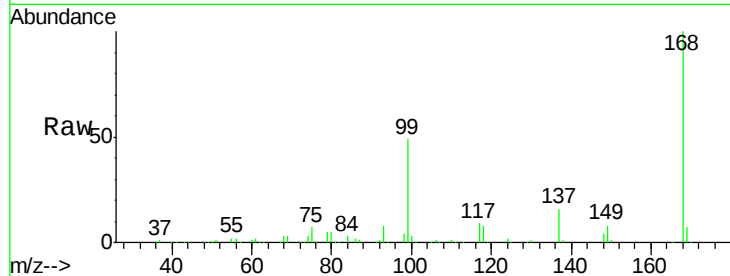

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

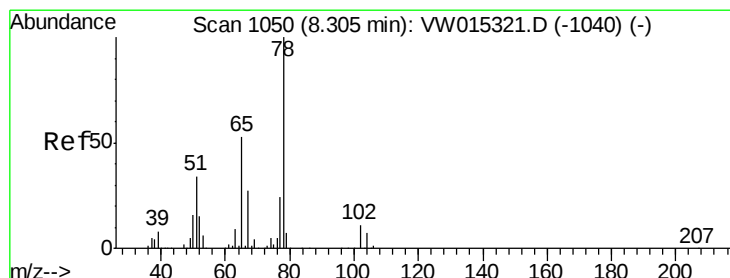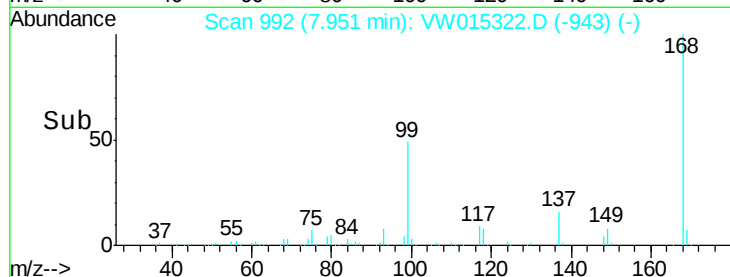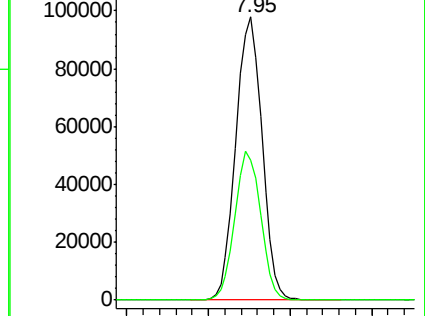

#33

1,2-Dichloroethane-d4

Concen: 48.137 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW015322.D


Acq: 23 Apr 2020 10:41

Tgt Ion: 65 Resp: 85619

Ion Ratio Lower Upper



65 100


67 50.6 0.0 107.0

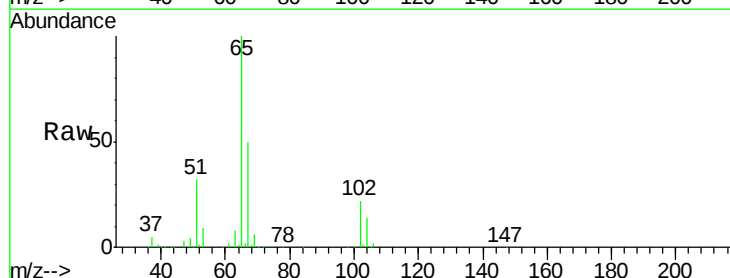

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

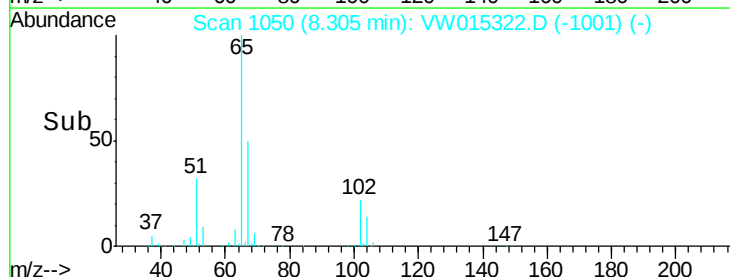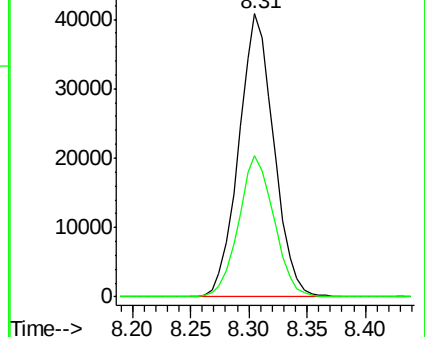

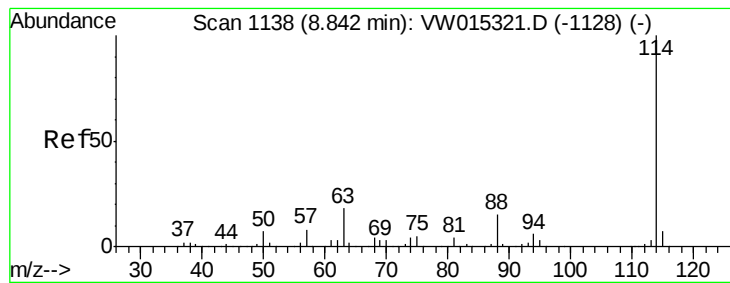

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. 0.00 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41

Instrument :

MSVOA_W

ClientSampleId :

VW0423SBL01


Tot Ion:114 Resp: 295985

Ion Ratio Lower Upper

114 100

63 18.7 0.0 39.8




88 16.2 0.0 30.2

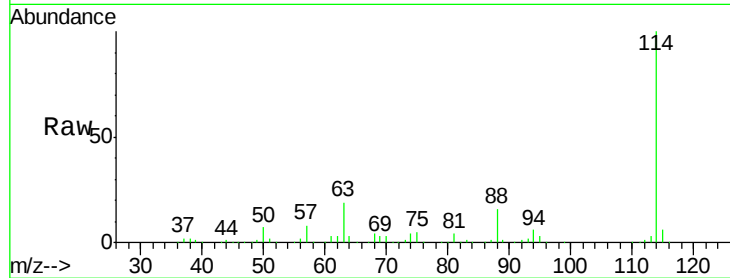

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

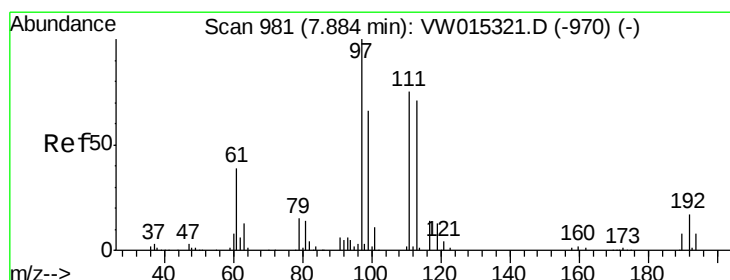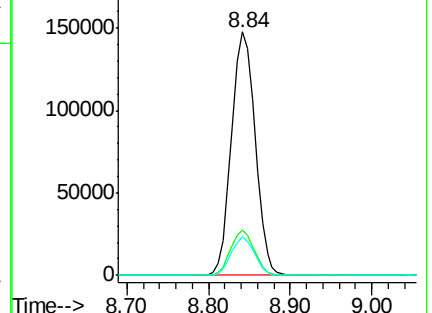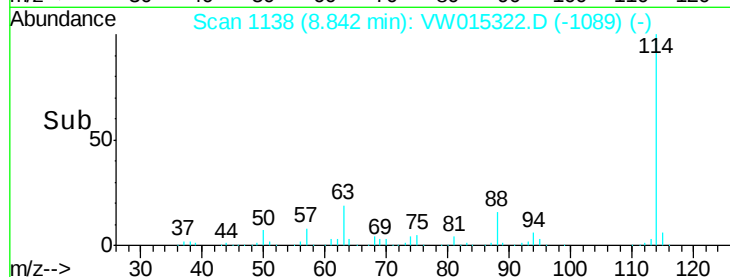

#35

Dibromofluoromethane

Concen: 52.321 ug/l

RT: 7.88 min Scan# 981

Delta R.T. 0.00 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41


Tgt Ion:113 Resp: 85781

Ion Ratio Lower Upper

113 100

111 100.9 83.0 124.4



192 23.0 15.1 22.7#

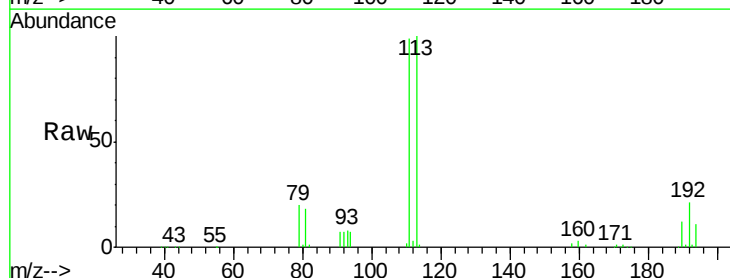


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

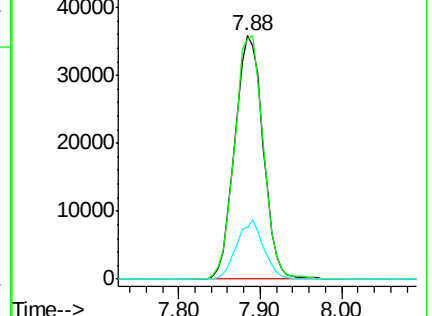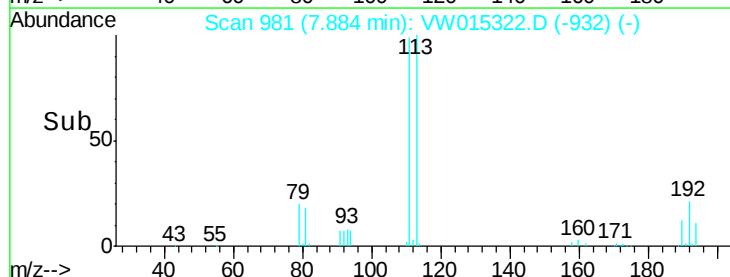

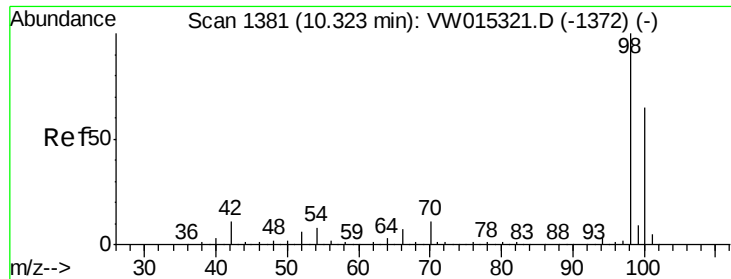

#50

Toluene-d8

Concen: 51.452 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41

Instrument :

MSVOA_W

ClientSampleId :


VW0423SBL01

Tot Ion: 98 Resp: 354865

Ion Ratio Lower Upper




98 100

100 66.3 52.9 79.3

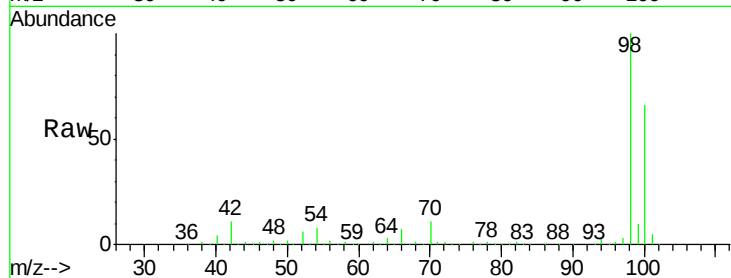

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

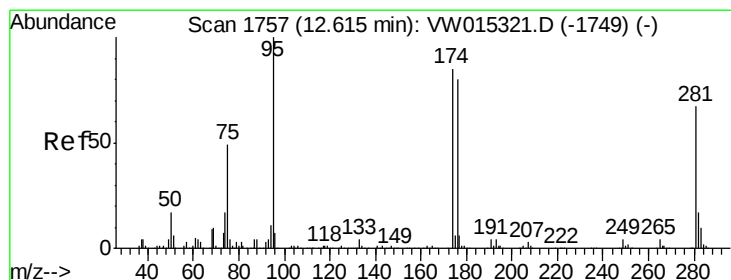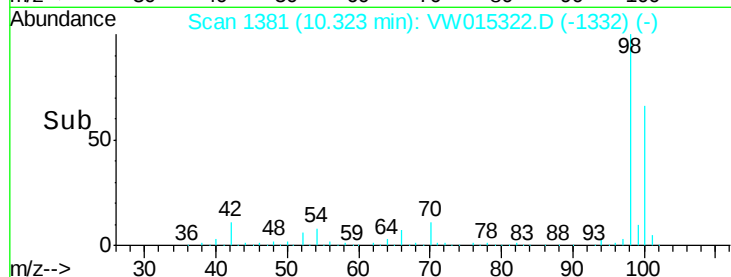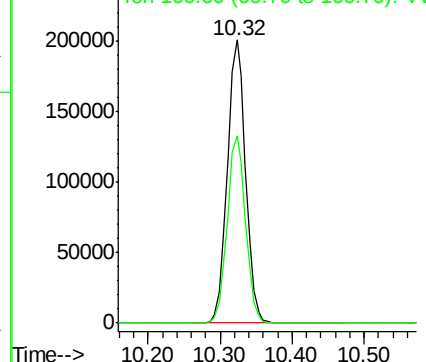

#62

4-Bromofluorobenzene

Concen: 44.387 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41


Tgt Ion: 95 Resp: 116805

Ion Ratio Lower Upper

95 100

174 90.7 0.0 144.4



176 87.3 0.0 140.6

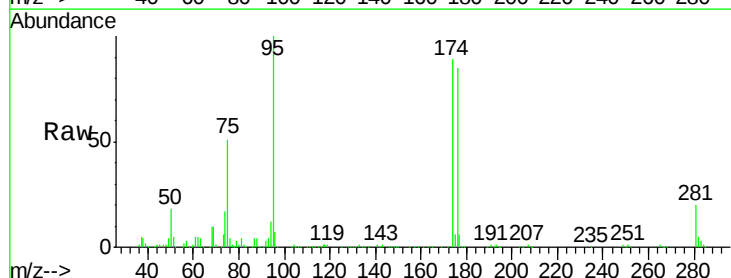


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

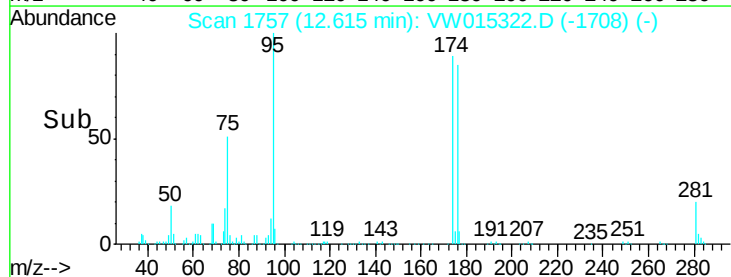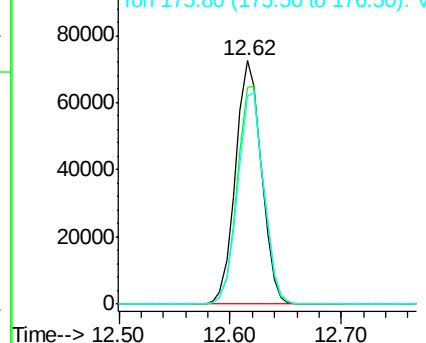

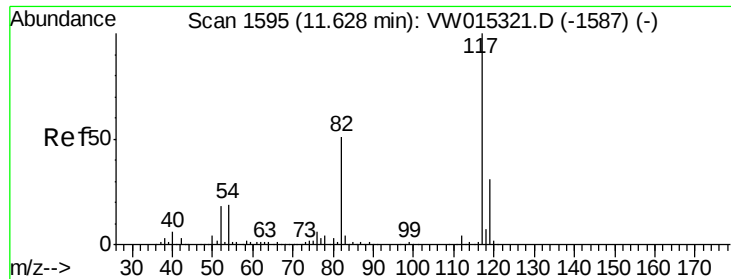

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1595

Delta R.T. -0.01 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41

Instrument :

MSVOA_W

ClientSampleId :

VW0423SBL01


Tot Ion:117 Resp: 262292

Ion Ratio Lower Upper

117 100

82 52.9 44.1 66.1




119 32.4 24.9 37.3

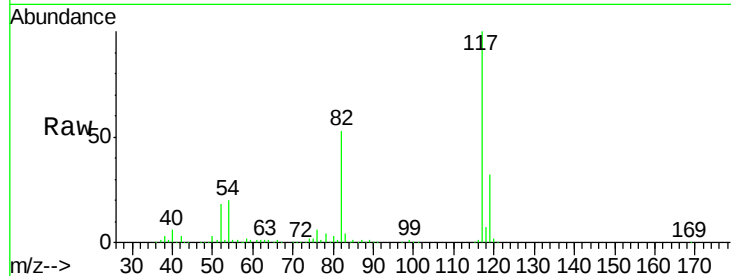

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): V

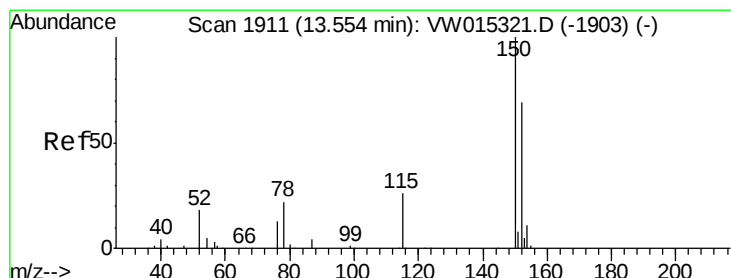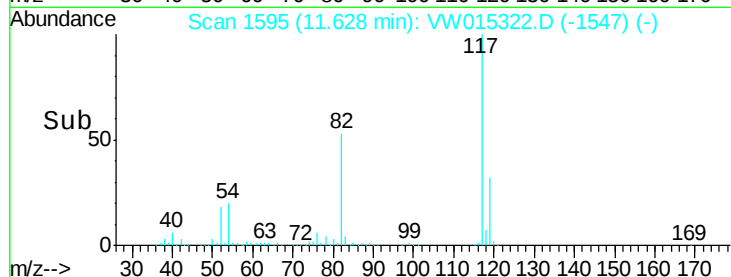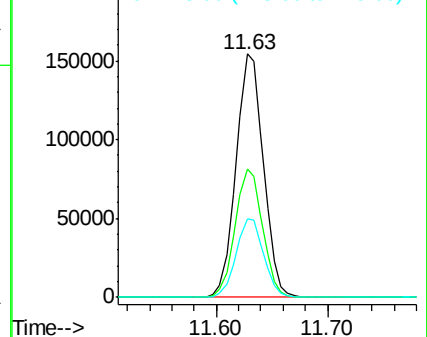

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW015322.D

Acq: 23 Apr 2020 10:41


Tgt Ion:152 Resp: 114228

Ion Ratio Lower Upper

152 100

115 56.9 31.3 93.9

150 157.8 0.0 343.4

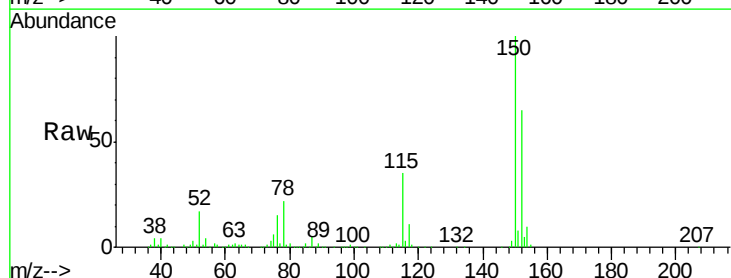

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

