

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
 Data File : VW028513.D
 Acq On : 23 Apr 2024 10:25
 Operator : SY/MD
 Sample : VW0423SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK470


Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt


04/24/2024
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 24 01:23:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 24 01:22:53 2024
 Response via : Initial Calibration


Ion 65.00 (64.70 to 65.70): VW028513.D\data.ms
 Ion 67.00 (66.70 to 67.70): VW028513.D\data.ms
 Ion 51.00 (50.70 to 51.70): VW028513.D\data.ms

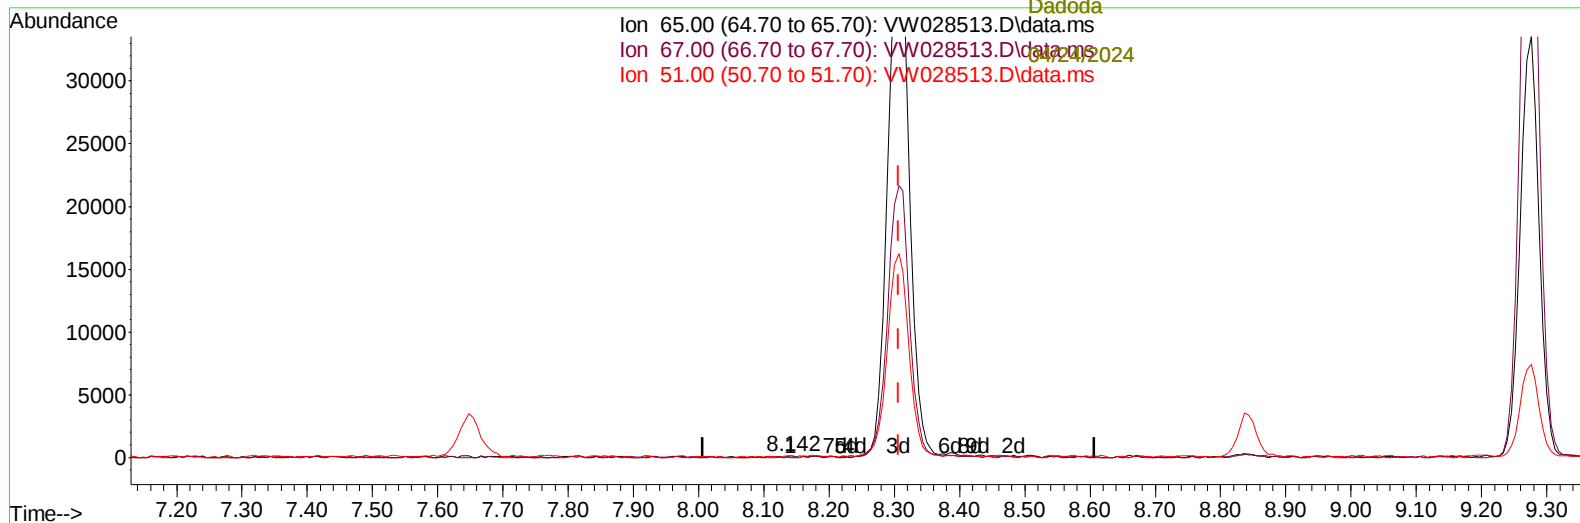

Scan 1026 (8.142 min): VW028513.D\data.ms

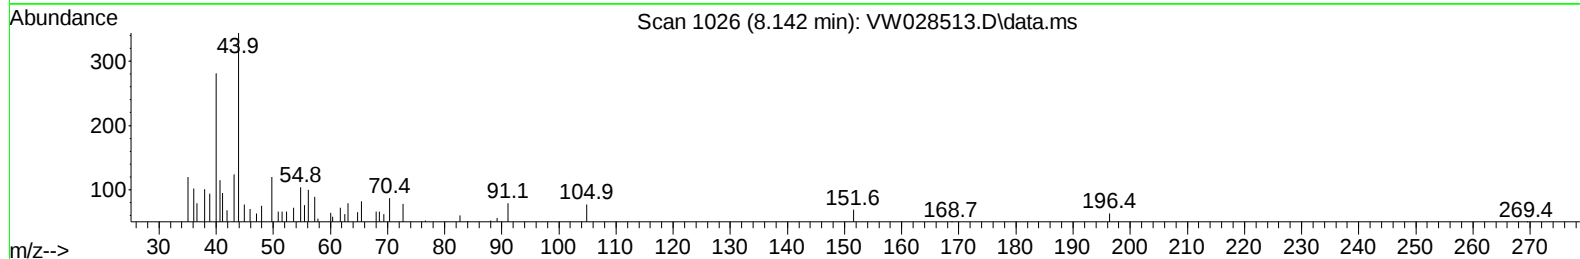

Scan 1053 (8.307 min): VW028512.D\data.ms (-1043) (-)

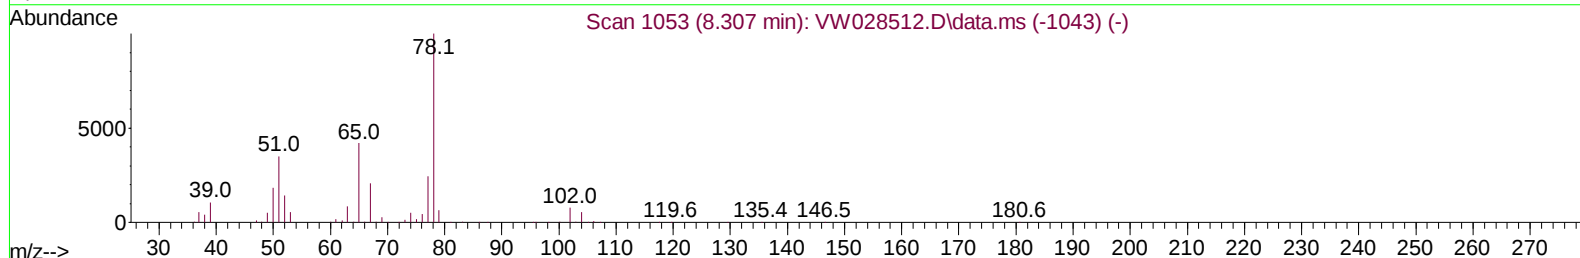

TIC: VW028513.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.142min (-0.165) 0.03 ug/L

response 105

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	64.76
51.00	108.40	115.24
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
Data File : VW028513.D
Acq On : 23 Apr 2024 10:25
Operator : SY/MD
Sample : VW0423SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK470


Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt


04/24/2024
Supervised By :Mahesh
Dadoda

Quant Time: Apr 24 01:23:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 24 01:22:53 2024
Response via : Initial Calibration


Ion 65.00 (64.70 to 65.70): VW028513.D\data.ms
Ion 67.00 (66.70 to 67.70): VW028513.D\data.ms
Ion 51.00 (50.70 to 51.70): VW028513.D\data.ms

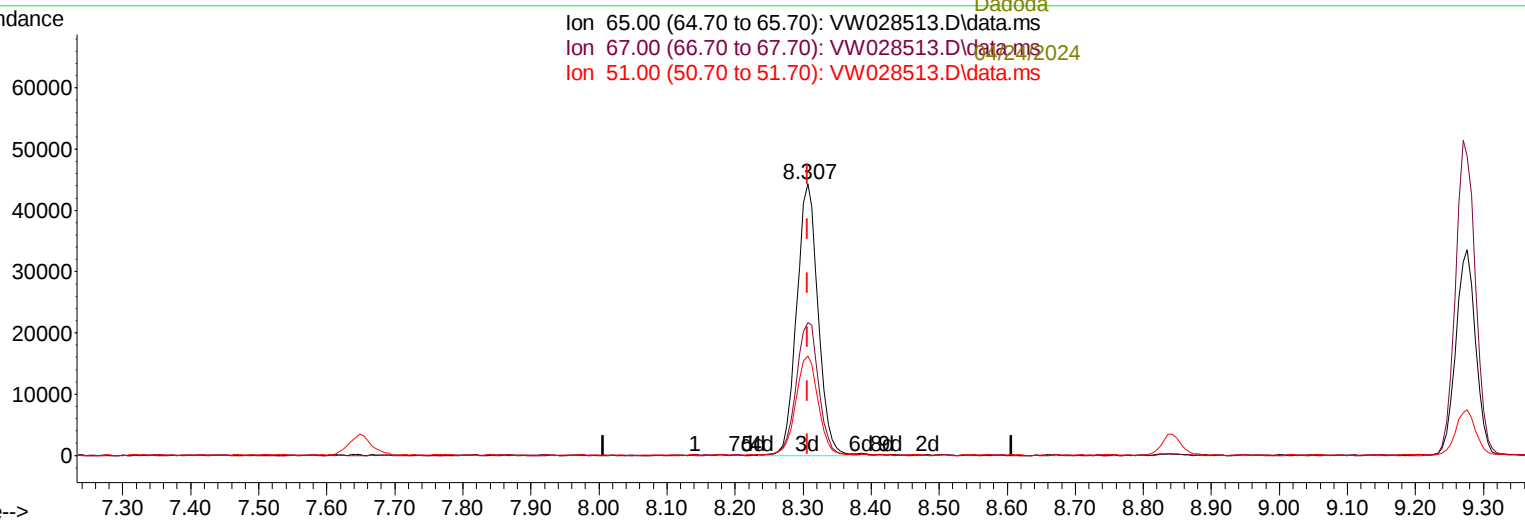

Scan 1053 (8.307 min): VW028513.D\data.ms

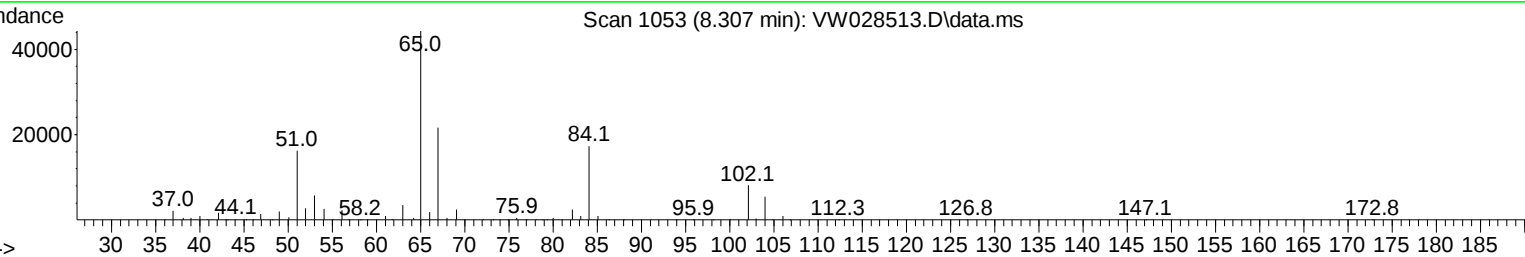

Scan 1053 (8.307 min): VW028512.D\data.ms (-1043) (-)

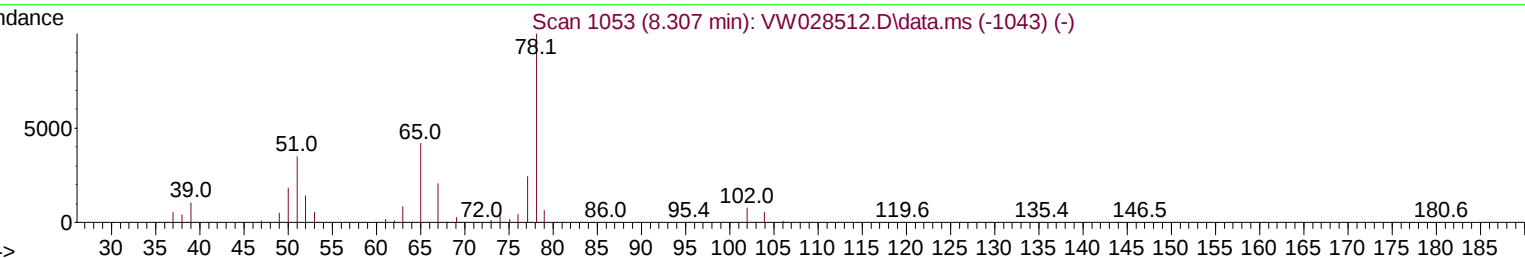

TIC: VW028513.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 24.41 ug/L m

response 97454

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.07#
51.00	108.40	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
 Data File : VW028513.D
 Acq On : 23 Apr 2024 10:25
 Operator : SY/MD
 Sample : VW0423SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK470

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

04/24/2024
 Supervised By :Mahesh
 Dadoda

Quant Time: Apr 24 01:23:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 24 01:22:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/24/2024						
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	294444	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	263649	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	126778	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	85449	18.102	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.400%	
7) Chloroethane-d5	2.905	69	72473	20.257	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.040%	
11) 1,1-Dichloroethene-d2	4.021	65	39358	19.689	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	78.760%	
21) 2-Butanone-d5	7.081	46	43371	49.100	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.200%	
24) Chloroform-d	7.648	84	177682	23.126	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.520%	
26) 1,2-Dichloroethane-d4	8.307	65	97454m	24.407	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.640%	
32) Benzene-d6	8.276	84	345343	23.977	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	95.920%	
36) 1,2-Dichloropropane-d6	9.270	67	104553	24.422	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	97.680%	
41) Toluene-d8	10.325	98	301568	23.026	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	92.120%	
43) trans-1,3-Dichloroprop...	10.574	79	38778	22.780	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.120%	
47) 2-Hexanone-d5	10.922	63	28879	48.698	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.400%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	77748	25.740	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.960%	
66) 1,2-Dichlorobenzene-d4	13.848	152	97545	24.329	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.320%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
Data File : VW028513.D
Acq On : 23 Apr 2024 10:25
Operator : SY/MD
Sample : VW0423SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK470

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

04/24/2024
Supervised By :Mahesh
Dadoda

04/24/2024

