




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
Data File : VW028519.D
Acq On : 23 Apr 2024 14:57
Operator : SY/MD
Sample : VIBLK433
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK433

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2024
Supervised By :Mahesh Dadoda 04/24/2024

Quant Time: Apr 24 01:24:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 24 01:22:53 2024
Response via : Initial Calibration

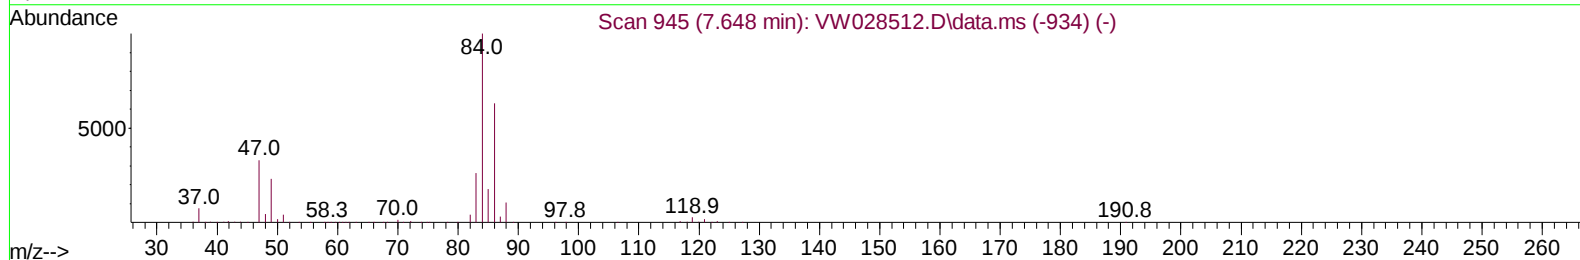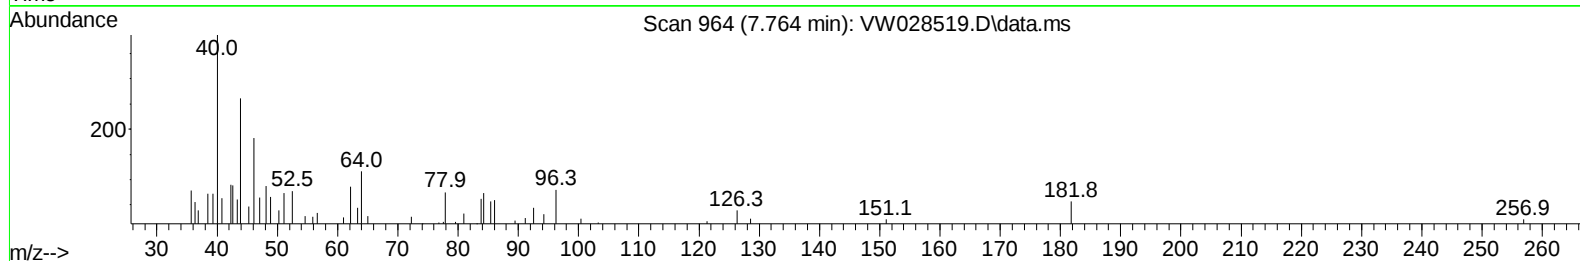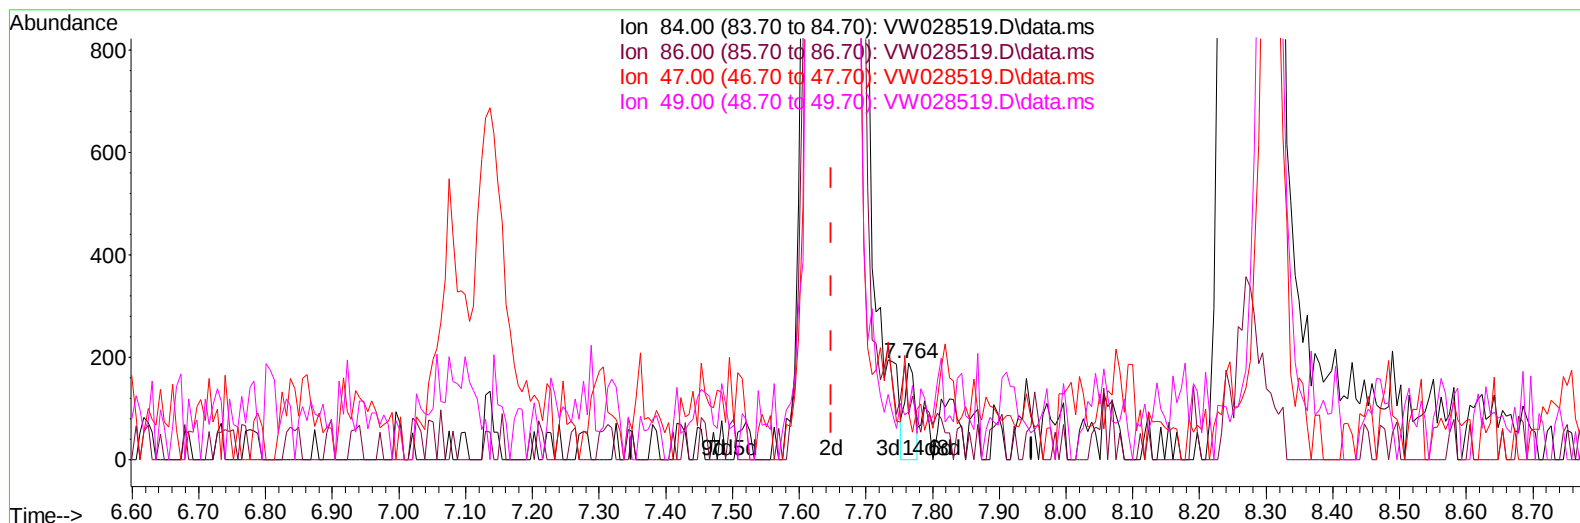

TIC: VW028519.D\data.ms

(24) Chloroform-d (S)

7.764min (+ 0.116) 0.02 ug/L

response 195

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.10	73.33
47.00	50.70	35.90
49.00	29.10	25.64




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
 Data File : VW028519.D
 Acq On : 23 Apr 2024 14:57
 Operator : SY/MD
 Sample : VIBLK433
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK433

Manual IntegrationsAPPROVED

Quant Time: Apr 24 01:24:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 24 01:22:53 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/24/2024
 Supervised By :Mahesh Dadoda 04/24/2024

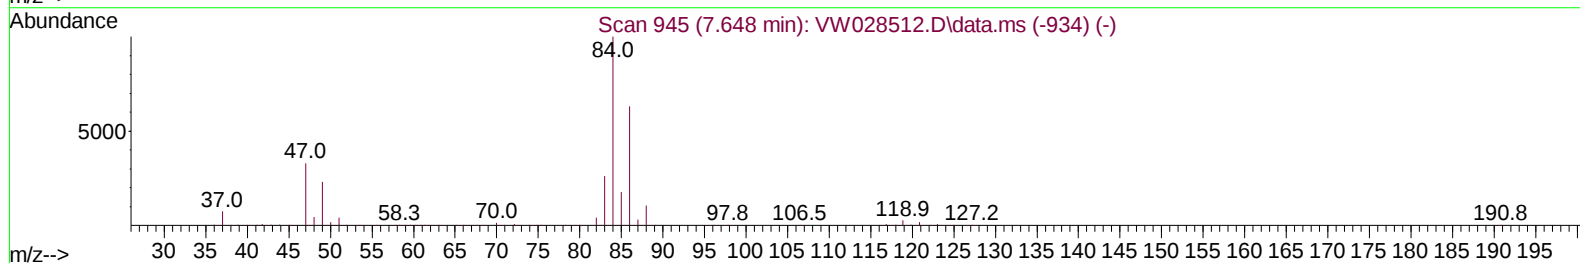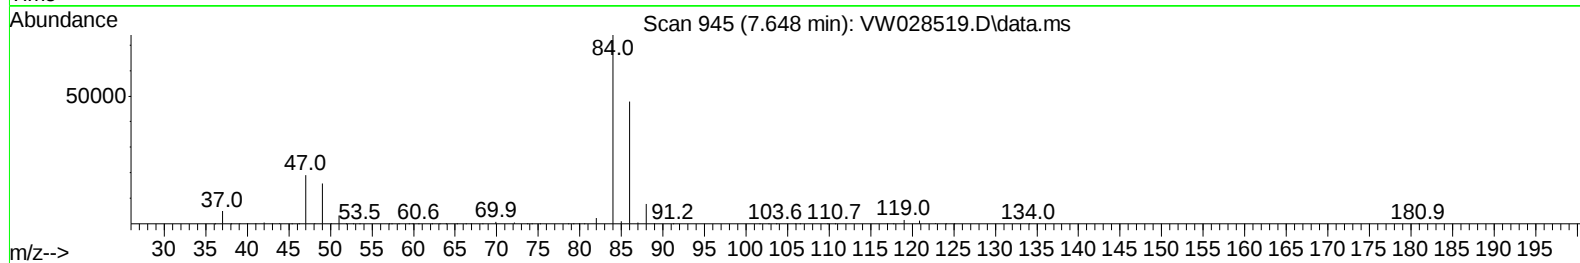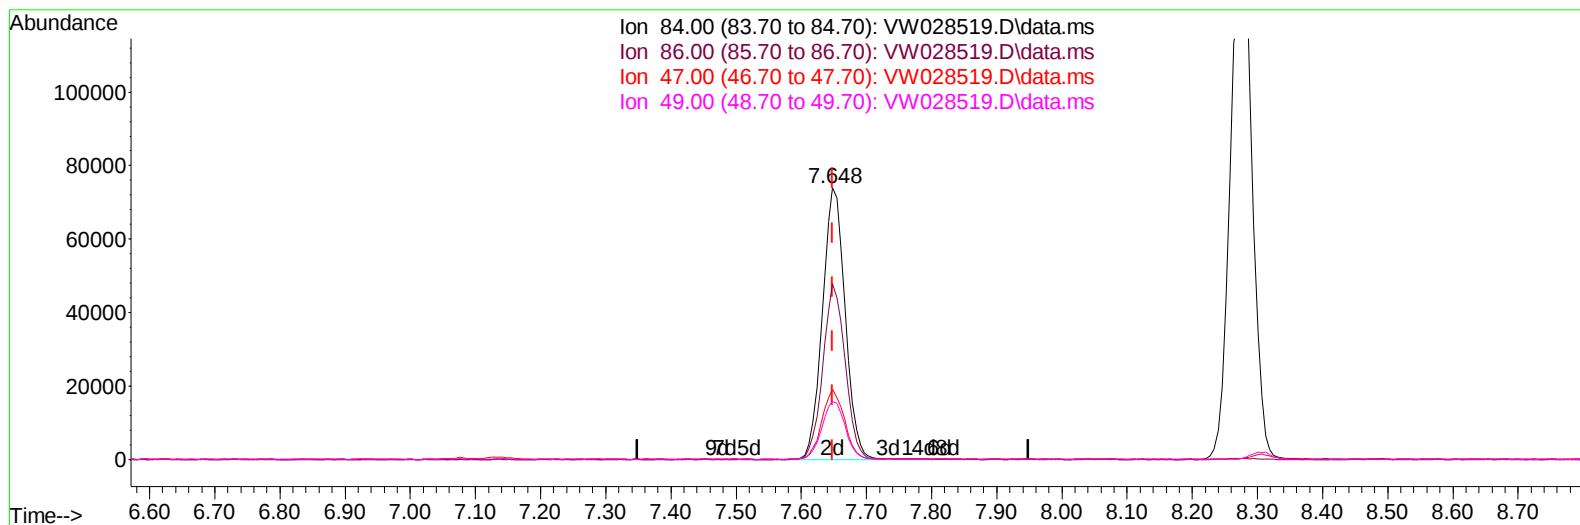

TIC: VW028519.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 22.20 ug/L m

response 179397

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.10	0.08#
47.00	50.70	0.04#
49.00	29.10	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
 Data File : VW028519.D
 Acq On : 23 Apr 2024 14:57
 Operator : SY/MD
 Sample : VIBLK433
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK433

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2024
 Supervised By :Mahesh Dadoda 04/24/2024

Quant Time: Apr 24 01:24:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 24 01:22:53 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		309706	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		277629	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		132815	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		84013	16.921	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.680%		
7) Chloroethane-d5	2.905	69		71951	19.120	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	76.480%		
11) 1,1-Dichloroethene-d2	4.027	65		39708	18.885	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	75.560%		
21) 2-Butanone-d5	7.081	46		41444	44.607	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	89.220%		
24) Chloroform-d	7.648	84		179397m	22.198	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	88.800%		
26) 1,2-Dichloroethane-d4	8.307	65		97809	23.289	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	93.160%		
32) Benzene-d6	8.276	84		343855	22.672	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	90.680%		
36) 1,2-Dichloropropane-d6	9.270	67		106789	23.688	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	94.760%		
41) Toluene-d8	10.325	98		311395	22.579	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	90.320%		
43) trans-1,3-Dichloroprop...	10.575	79		38510	21.483	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	85.920%		
47) 2-Hexanone-d5	10.922	63		27173	43.514	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	87.020%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		76276	23.981	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	95.920%		
66) 1,2-Dichlorobenzene-d4	13.848	152		101548	24.176	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	96.720%		
Target Compounds							
16) Methylene chloride	4.923	84		27826	5.938	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042324\
Data File : VW028519.D
Acq On : 23 Apr 2024 14:57
Operator : SY/MD
Sample : VIBLK433
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK433

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/24/2024
Supervised By :Mahesh Dadoda 04/24/2024

Quant Time: Apr 24 01:24:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 24 01:22:53 2024
Response via : Initial Calibration

