

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW042419\
 Data File : VW010115.D
 Acq On : 24 Apr 2019 16:18
 Operator : SY/VA
 Sample : K2456-02
 Misc : 5.01G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHQ2RE

Quant Time: Apr 25 01:39:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 01:36:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	249778	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	215680	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	60260	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	65851	27.58	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.32%
7) Chloroethane-d5	2.89	69	56911	28.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.36%
10) 1,1-Dichloroethene-d2	3.99	63	152292	21.73	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.92%
20) 2-Butanone-d5	7.08	46	69169	61.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.70%
24) Chloroform-d	7.64	84	206212	31.01	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	124.04%
26) 1,2-Dichloroethane-d4	8.49	65	59	0.02	ug/L	0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.08%#
29) Benzene-d6	8.27	84	403101	33.00	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	132.00%
33) 1,2-Dichloropropane-d6	9.27	67	130098	34.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	136.64%#
37) Toluene-d8	10.32	98	337337	30.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	121.60%
38) trans-1,3-Dichloropropene-	10.58	79	50787	28.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	115.76%
39) 2-Hexanone-d5	10.93	63	49564	61.94	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.88%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	82393	26.06	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.24%
61) 1,2-Dichlorobenzene-d4	13.86	152	62429	27.98	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.92%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.12	43	1602	1.883	ug/L	79
16) Methylene chloride	4.90	84	10487	2.996	ug/L	94
35) Trichloroethene	8.84	95	6999	2.023	ug/L #	6
36) Methylcyclohexane	9.27	83	31505	5.433	ug/L #	17
44) Toluene	10.38	91	209899	15.114	ug/L	99
45) trans-1,3-Dichloropropene	10.57	75	2734	0.602	ug/L	99
53) Ethylbenzene	11.73	91	81625	5.237	ug/L	94
54) m,p-Xylene	11.84	106	212691	36.890	ug/L	98
55) o-xylene	12.16	106	160243	29.310	ug/L	94
56) Styrene	12.18	104	193931	20.857	ug/L	96
66) 1,2-Dibromo-3-chloropropan	14.47	75	112015	339.809	ug/L #	6
69) Naphthalene	15.47	128	27720	4.907	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW042419\
Data File : VW010115.D
Acq On : 24 Apr 2019 16:18
Operator : SY/VA
Sample : K2456-02
Misc : 5.01G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHQ2RE

Quant Time: Apr 25 01:39:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 25 01:36:45 2019
Response via : Initial Calibration




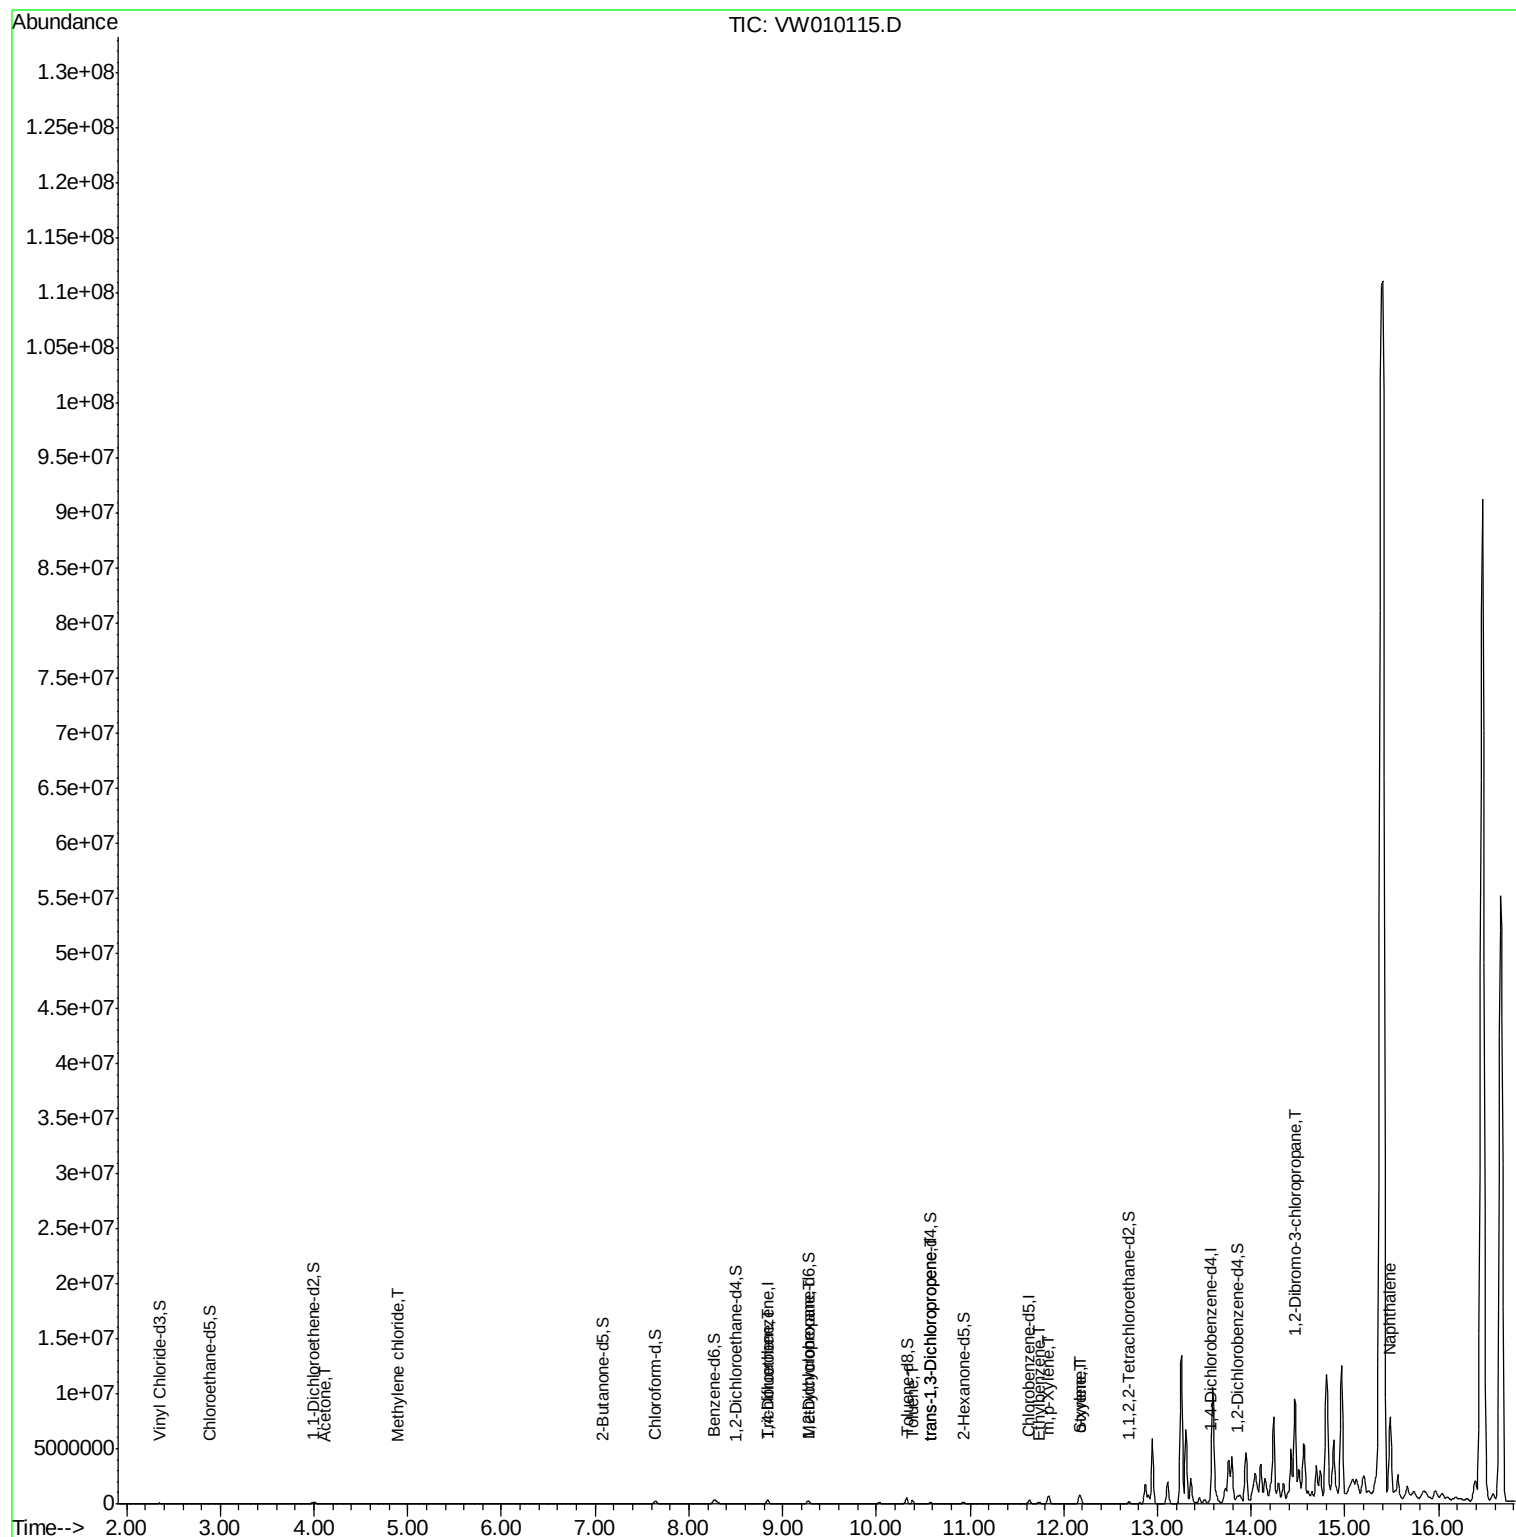


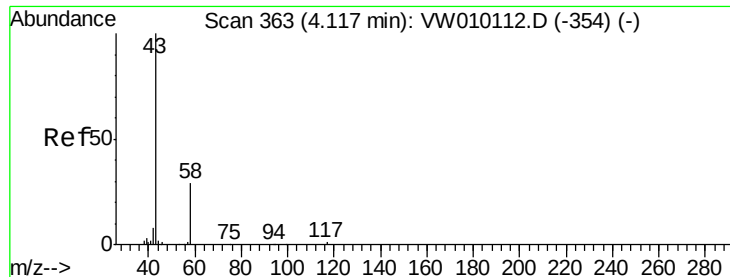

#13
Acetone
Concen: 1.883 ug/L
RT: 4.12 min Scan# 363
Delta R.T. 0.00 min
Lab File: VW010115.D
Acq: 24 Apr 2019 16:18




Instrument :
MSVOA_W
ClientSampleId :
GAHQ2RE


Tgt Ion: 43 Resp: 1602
Ion Ratio Lower Upper
43 100
58 17.6 0.0 58.2

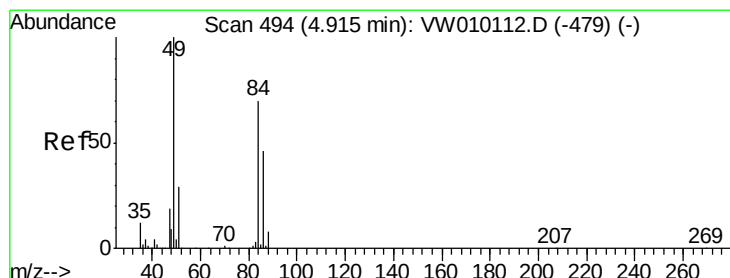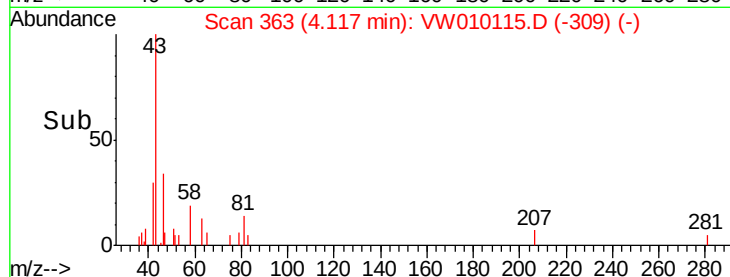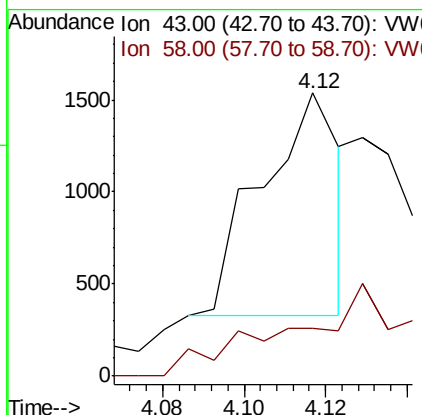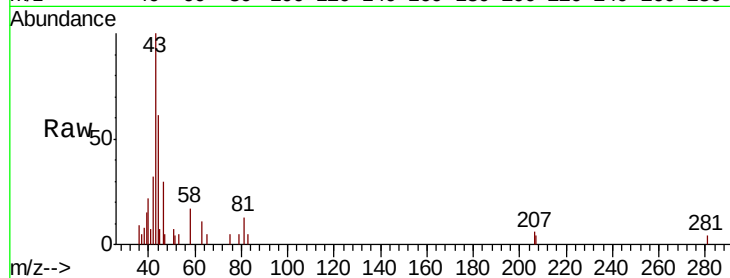

#16
Methylene chloride
Concen: 2.996 ug/L
RT: 4.90 min Scan# 491
Delta R.T. -0.02 min
Lab File: VW010115.D
Acq: 24 Apr 2019 16:18

Tgt Ion: 84 Resp: 10487
Ion Ratio Lower Upper
84 100
49 135.6 93.5 173.7
86 53.4 44.9 83.5

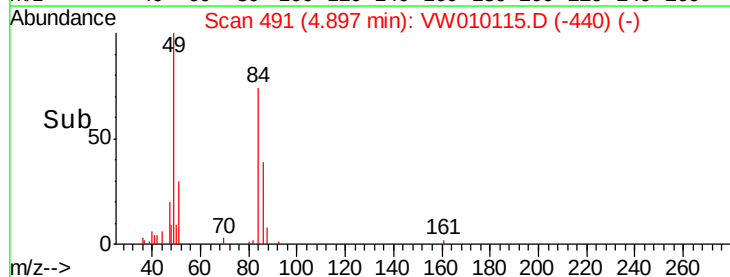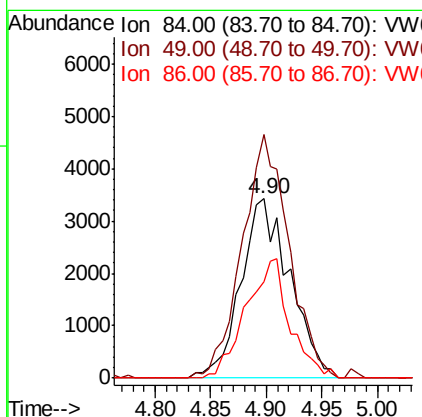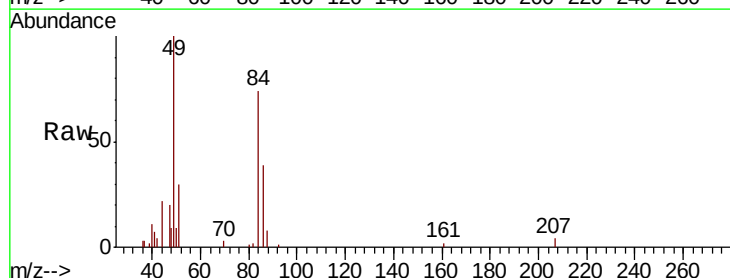

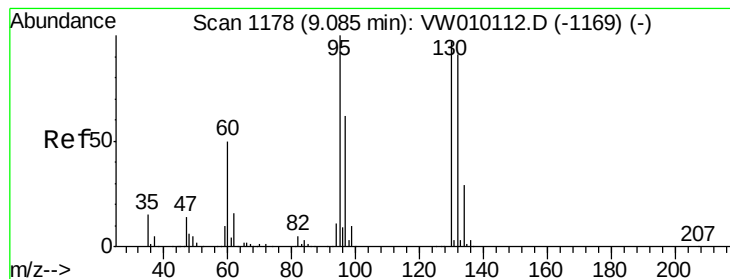

#35

Trichloroethene

Concen: 2.023 ug/L

RT: 8.84 min Scan# 1138

Delta R.T. -0.25 min

Lab File: VW010115.D

Acq: 24 Apr 2019 16:18

Instrument :

MSVOA_W

ClientSampleId :

GAHQ2RE

Tgt Ion: 95 Resp: 6999


Ion Ratio Lower Upper

95 100

97 1.4 45.1 83.9#

132 0.0 67.2 124.8#

130 0.6 70.0 130.0#

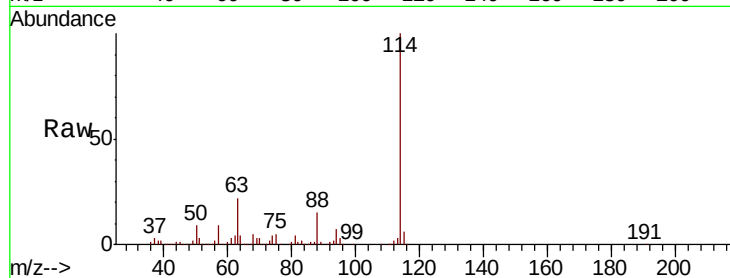

Abundance


Ion 95.00 (94.70 to 95.70): VW

Ion 97.00 (96.70 to 97.70): VW


Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

Time-->

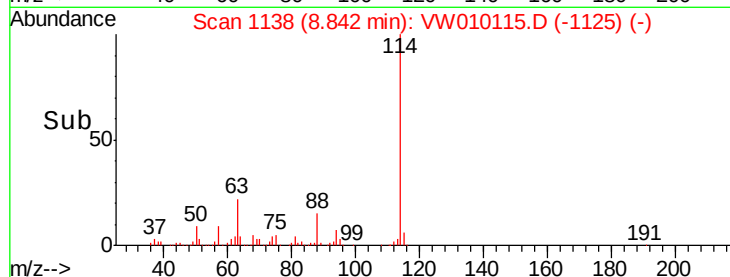

Time-->

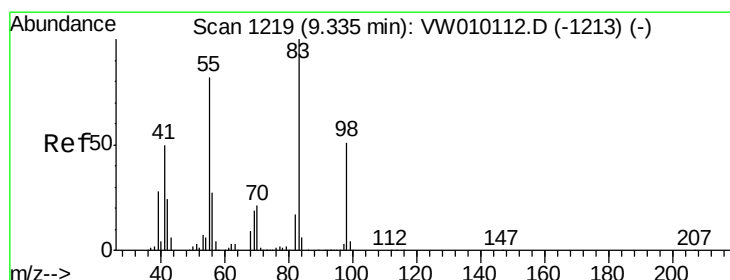

#36

Methylcyclohexane

Concen: 5.433 ug/L

RT: 9.27 min Scan# 1208

Delta R.T. -0.07 min

Lab File: VW010115.D

Acq: 24 Apr 2019 16:18


Tgt Ion: 83 Resp: 31505

Ion Ratio Lower Upper

83 100

55 1.2 66.6 100.0#

98 1.3 39.1 58.7#

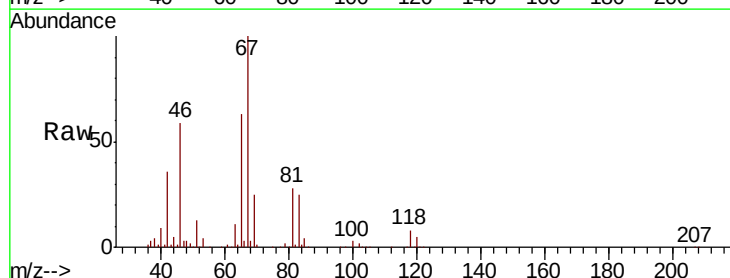


Abundance

Ion 83.00 (82.70 to 83.70): VW


Ion 55.00 (54.70 to 55.70): VW

Ion 98.00 (97.70 to 98.70): VW

Time-->

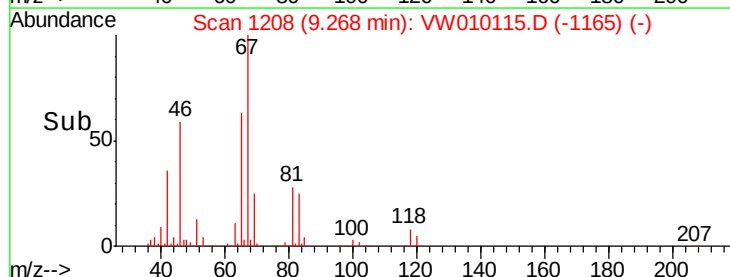

Time-->

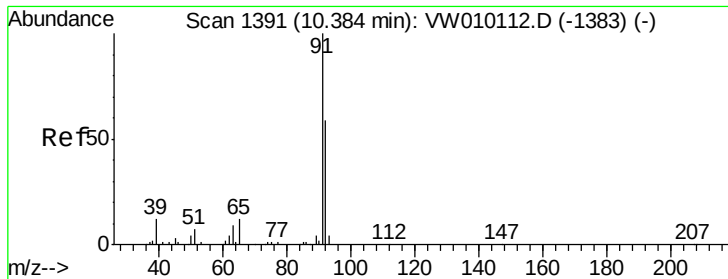

#44

Toluene

Concen: 15.114 ug/L

RT: 10.38 min Scan# 1391

Delta R.T. 0.00 min

Lab File: VW010115.D

Acq: 24 Apr 2019 16:18

Instrument :

MSVOA_W

ClientSampled :


GAHQ2RE

Tgt Ion: 91 Resp: 209899

Ion Ratio Lower Upper




91 100

92 57.0 40.3 74.9

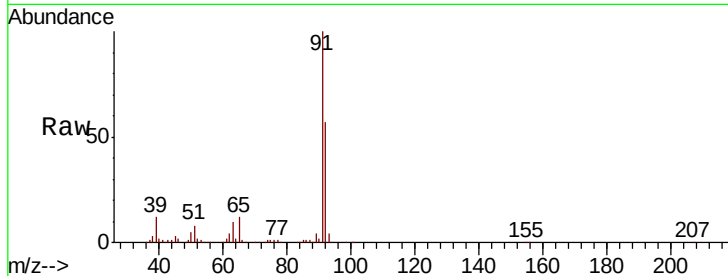

Abundance Ion 91.00 (90.70 to 91.70): VW

Ion 92.00 (91.70 to 92.70): VW

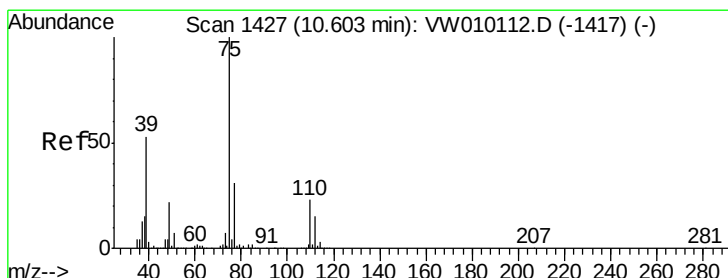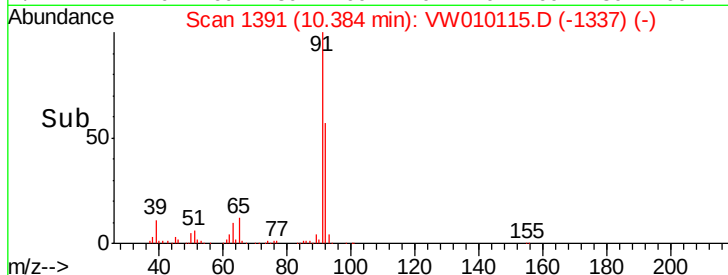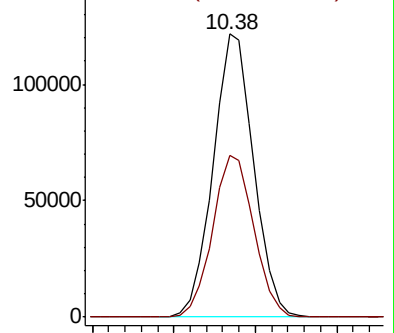

#45

trans-1,3-Dichloropropene

Concen: 0.602 ug/L

RT: 10.57 min Scan# 1422

Delta R.T. -0.03 min

Lab File: VW010115.D


Acq: 24 Apr 2019 16:18

Tgt Ion: 75 Resp: 2734

Ion Ratio Lower Upper



75 100


77 31.2 22.2 41.2

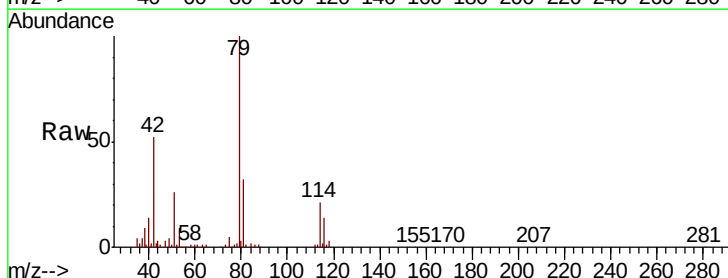

Abundance Ion 75.00 (74.70 to 75.70): VW

Ion 77.00 (76.70 to 77.70): VW



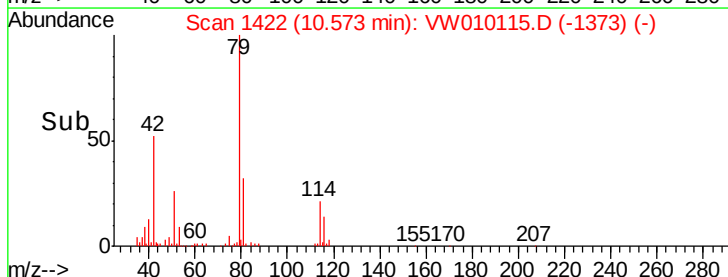
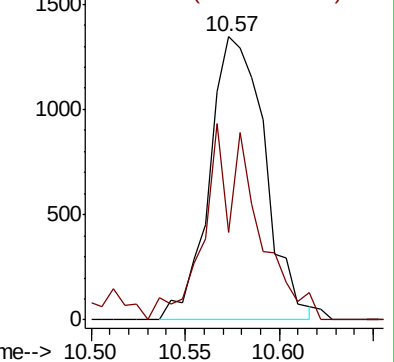


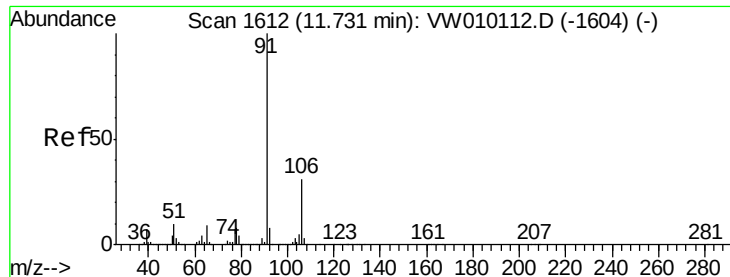

#53
Ethylbenzene
Concen: 5.237 ug/L
RT: 11.73 min Scan# 1612
Delta R.T. 0.00 min
Lab File: VW010115.D
Acq: 24 Apr 2019 16:18




Instrument :
MSVOA_W
ClientSampleId :
GAHQ2RE


Tgt Ion: 91 Resp: 81625
Ion Ratio Lower Upper
91 100
106 27.4 21.5 39.9

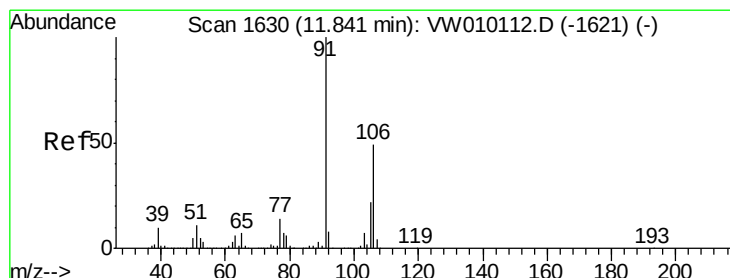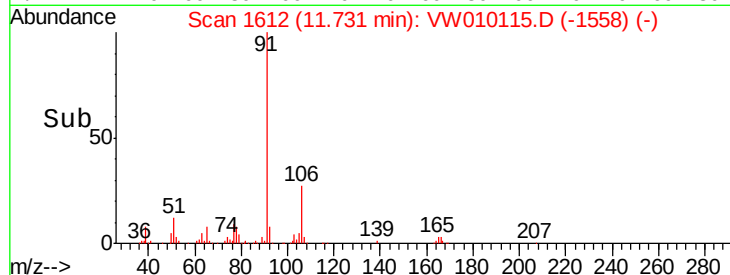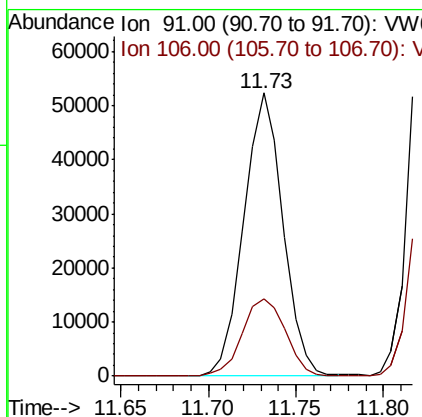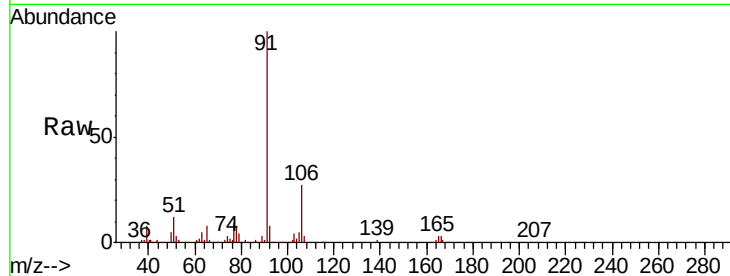

#54
m,p-Xylene
Concen: 36.890 ug/L
RT: 11.84 min Scan# 1629
Delta R.T. -0.01 min
Lab File: VW010115.D
Acq: 24 Apr 2019 16:18

Tgt Ion: 106 Resp: 212691
Ion Ratio Lower Upper
106 100
91 207.6 143.4 266.4

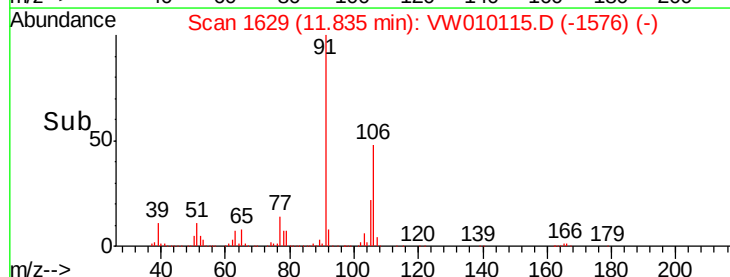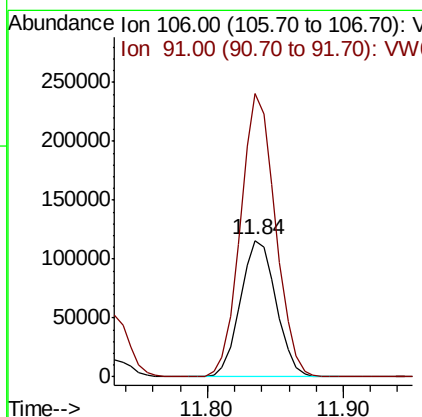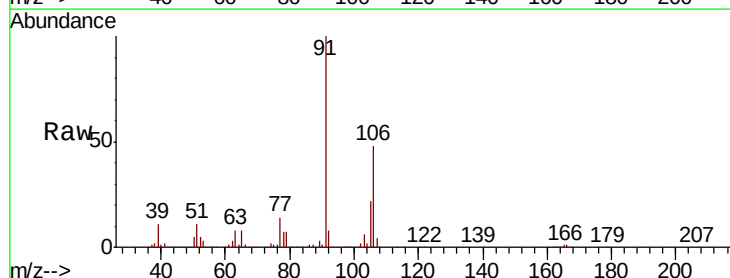

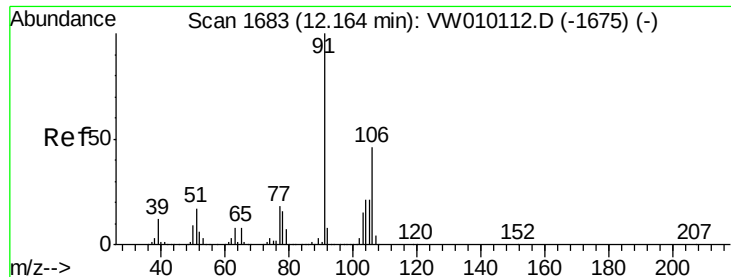

#55

o-xylene

Concen: 29.310 ug/L

RT: 12.16 min Scan# 1683

Delta R.T. -0.01 min

Lab File: VW010115.D

Acq: 24 Apr 2019 16:18

Instrument :

MSVOA_W

ClientSampleId :


GAHQ2RE

Tgt Ion:106 Resp: 160243

Ion Ratio Lower Upper

106 100

91 226.1 151.4 281.2

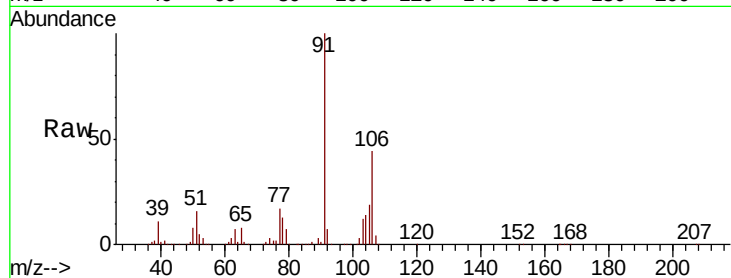

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

250000

200000

150000



100000

50000

0

12.10 12.15 12.20

Time-->

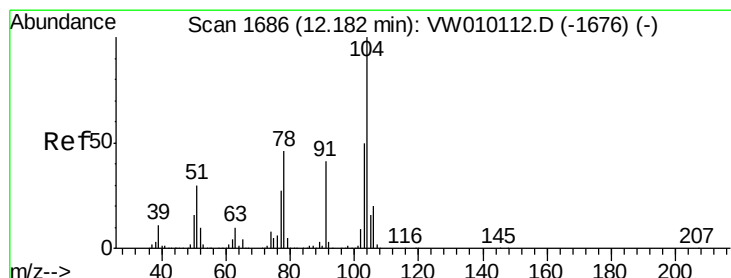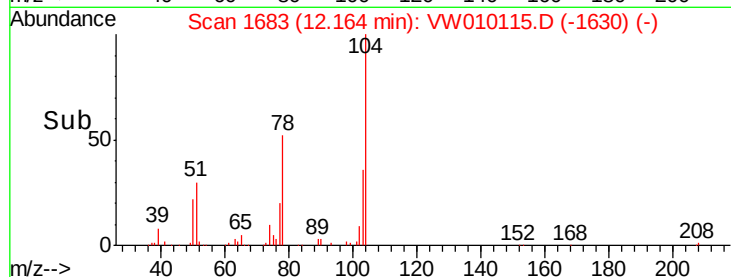

#56

Styrene

Concen: 20.857 ug/L

RT: 12.18 min Scan# 1686

Delta R.T. 0.00 min

Lab File: VW010115.D


Acq: 24 Apr 2019 16:18

Tgt Ion:104 Resp: 193931

Ion Ratio Lower Upper

104 100

78 50.3 33.4 62.0

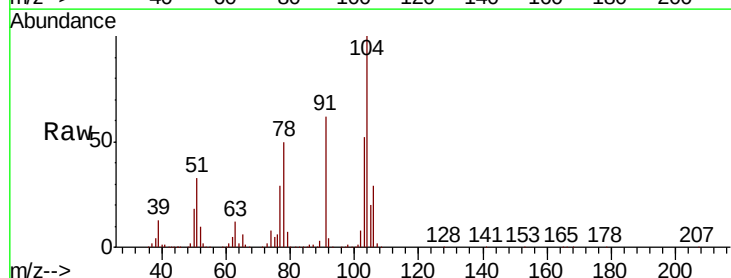

Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VW


100000


50000

0

12.10 12.20

Time-->




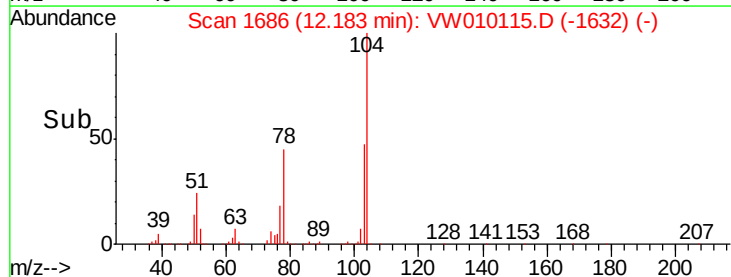


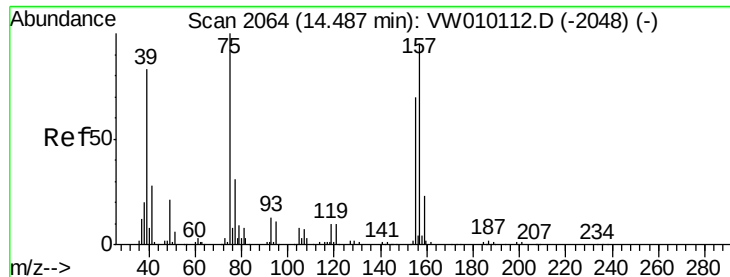

#66
 1,2-Dibromo-3-chloropropane
 Concen: 339.809 ug/L
 RT: 14.47 min Scan# 2061
 Delta R.T. -0.02 min
 Lab File: VW010115.D
 Acq: 24 Apr 2019 16:18

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHQ2RE

Tgt Ion: 75 Resp: 112015
 Ion Ratio Lower Upper
 75 100
 157 0.0 78.4 117.6#
 155 0.1 60.2 90.2#

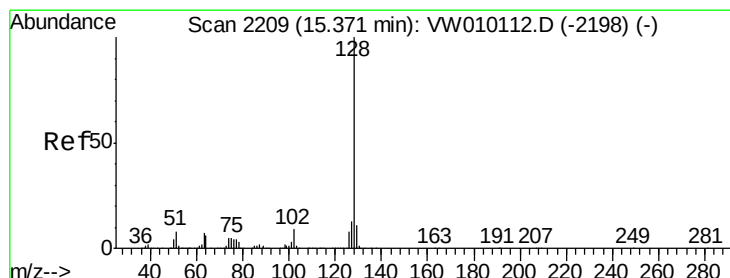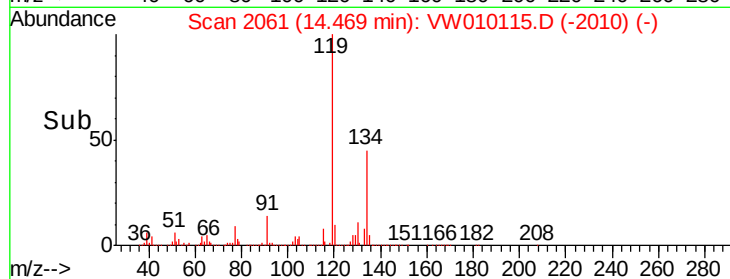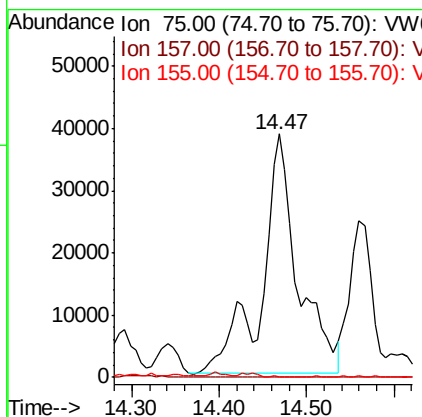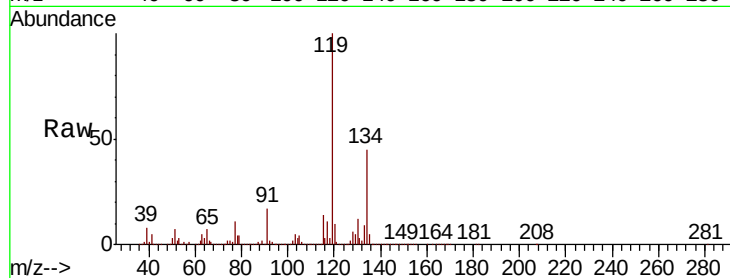

#69
 Naphthalene
 Concen: 4.907 ug/L
 RT: 15.47 min Scan# 2226
 Delta R.T. 0.10 min
 Lab File: VW010115.D
 Acq: 24 Apr 2019 16:18

Tgt Ion: 128 Resp: 27720
 Ion Ratio Lower Upper
 128 100
 129 102.6 8.6 13.0#
 127 26.6 10.8 16.2#

