

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW042419\
 Data File : VW010117.D
 Acq On : 24 Apr 2019 18:41
 Operator : SY/VA
 Sample : K2481-11
 Misc : 5.06G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHW4

Quant Time: Apr 25 01:39:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 01:36:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	753616	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	693629	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	306131	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	105750	14.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.72%
7) Chloroethane-d5	2.89	69	95756	16.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.36%
10) 1,1-Dichloroethene-d2	4.01	63	224274	10.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.44%#
20) 2-Butanone-d5	7.07	46	132898	39.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.14%
24) Chloroform-d	7.64	84	390018	19.44	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.76%
26) 1,2-Dichloroethane-d4	8.31	65	229456	19.56	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.24%
29) Benzene-d6	8.27	84	744006	18.94	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.76%
33) 1,2-Dichloropropane-d6	9.27	67	255285	20.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.36%
37) Toluene-d8	10.32	98	668222	18.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.92%
38) trans-1,3-Dichloropropene-	10.57	79	94892	16.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.28%
39) 2-Hexanone-d5	10.93	63	99549	38.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.36%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	219631	21.60	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	242766	21.42	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.68%

Target Compounds


					Qvalue
13) Acetone	4.12	43	11884	4.629 ug/L	97
66) 1,2-Dibromo-3-chloropropan	14.54	75	30790	18.386 ug/L #	6
69) Naphthalene	15.37	128	398368	13.881 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW042419\
Data File : VW010117.D
Acq On : 24 Apr 2019 18:41
Operator : SY/VA
Sample : K2481-11
Misc : 5.06G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHW4

Quant Time: Apr 25 01:39:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 25 01:36:45 2019
Response via : Initial Calibration




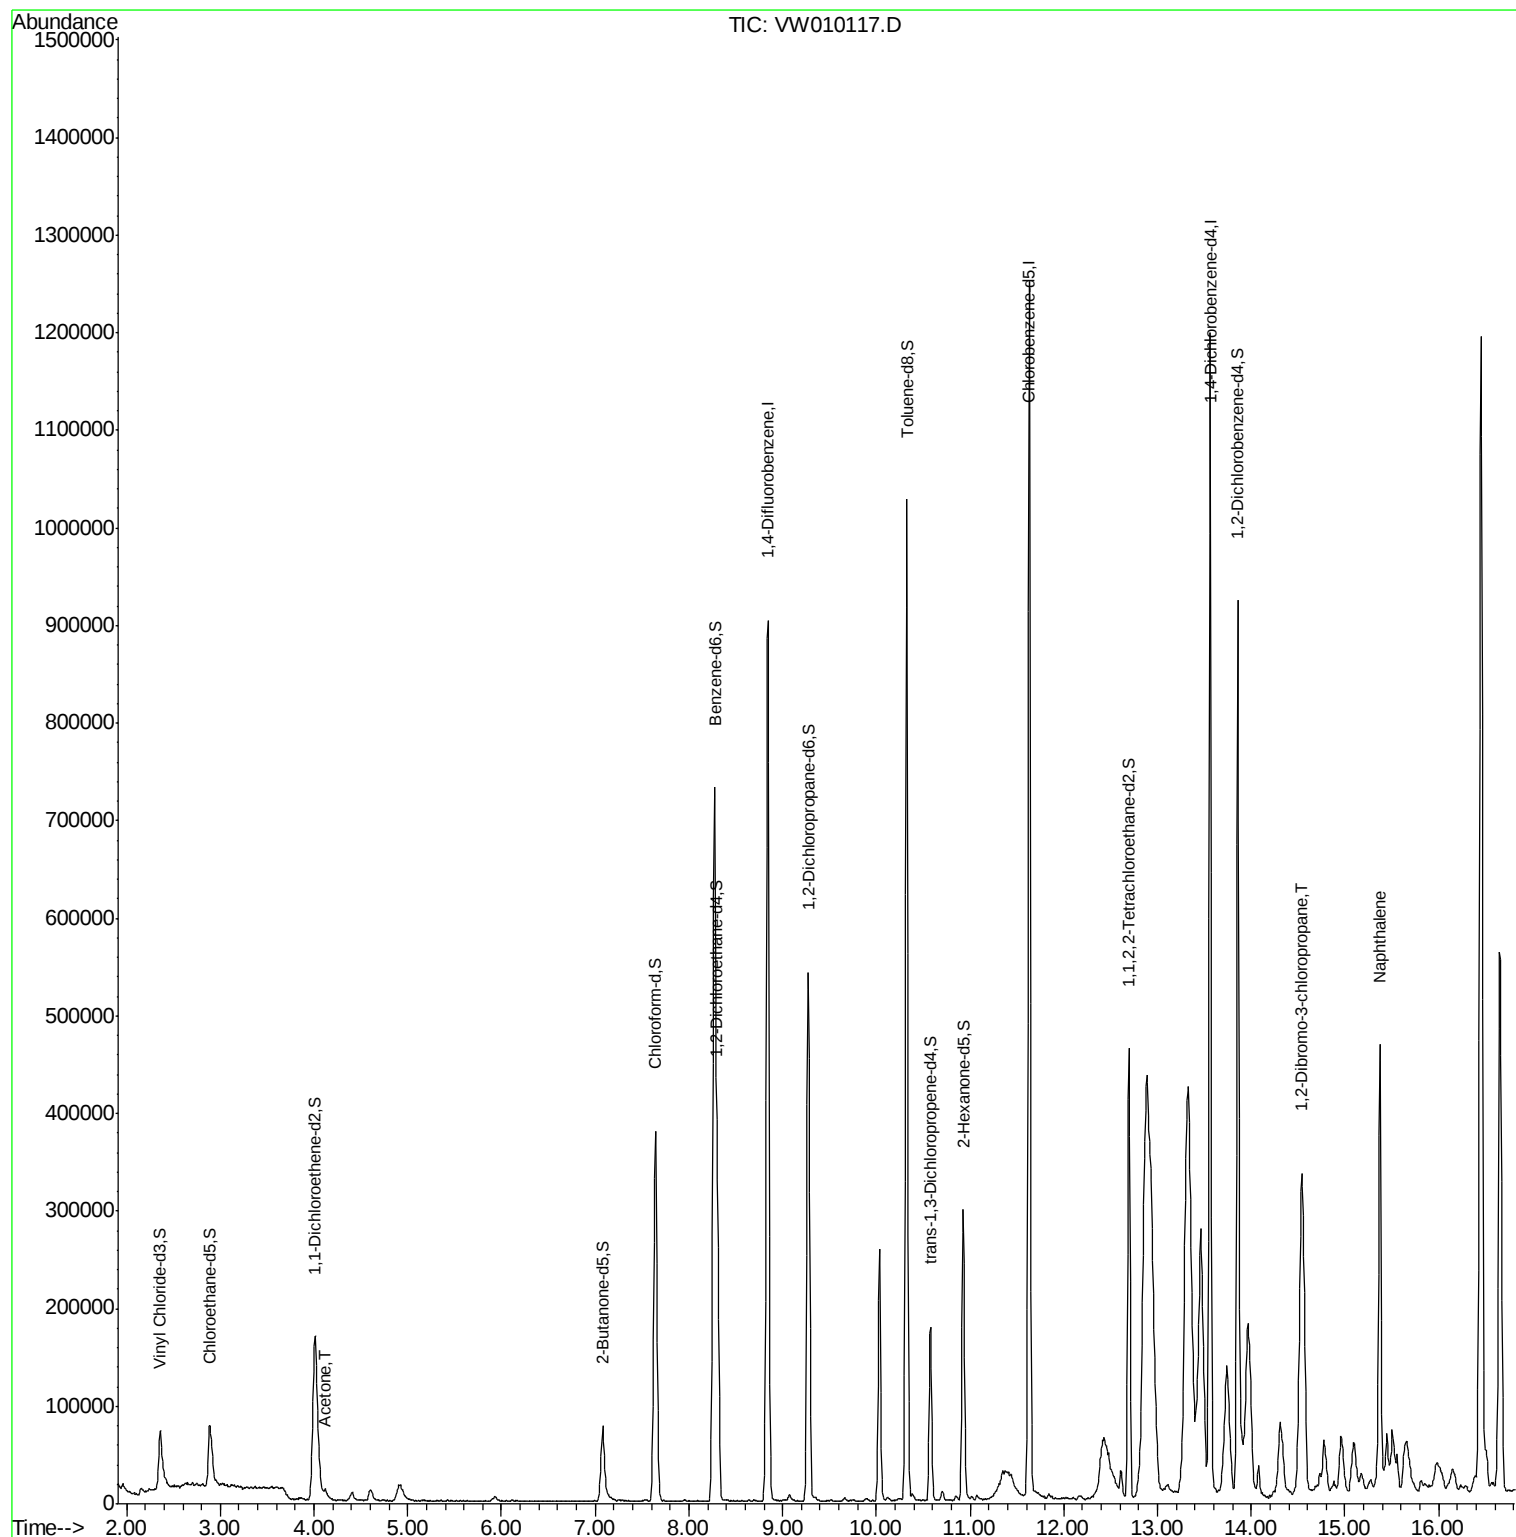


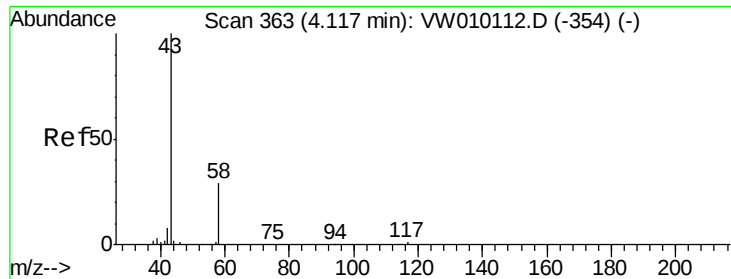

#13
Acetone
Concen: 4.629 ug/L
RT: 4.12 min Scan# 363
Delta R.T. 0.00 min
Lab File: VW010117.D
Acq: 24 Apr 2019 18:41




Instrument :
MSVOA_W
ClientSampled :
GAHW4


Tgt Ion: 43 Resp: 11884
Ion Ratio Lower Upper
43 100
58 27.5 0.0 58.2

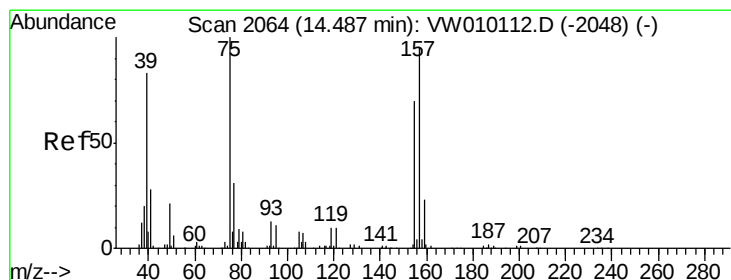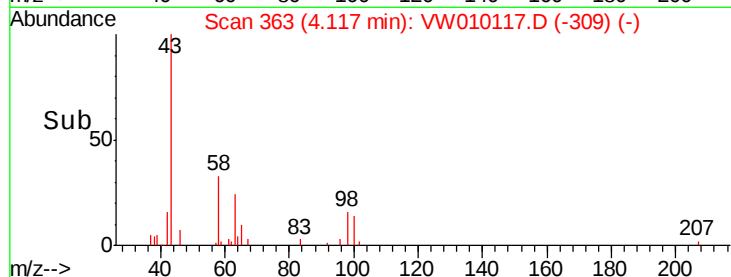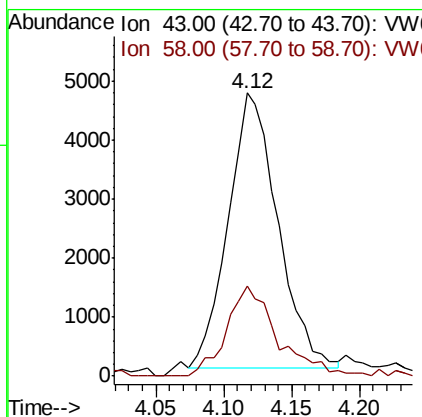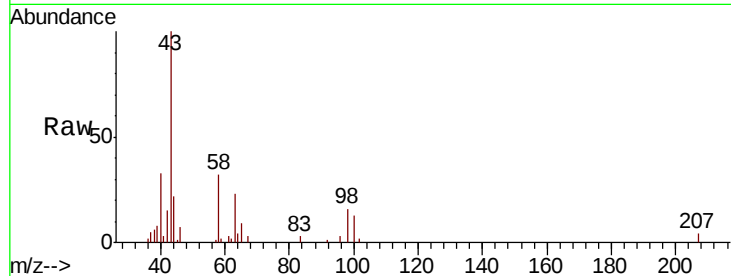

#66
1,2-Dibromo-3-chloropropane
Concen: 18.386 ug/L
RT: 14.54 min Scan# 2072
Delta R.T. 0.05 min
Lab File: VW010117.D
Acq: 24 Apr 2019 18:41

Tgt Ion: 75 Resp: 30790
Ion Ratio Lower Upper
75 100
157 0.0 78.4 117.6#
155 1.6 60.2 90.2#

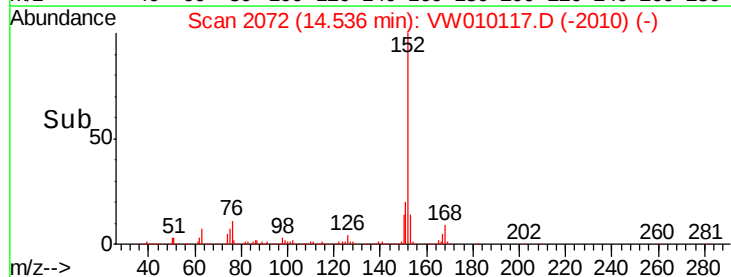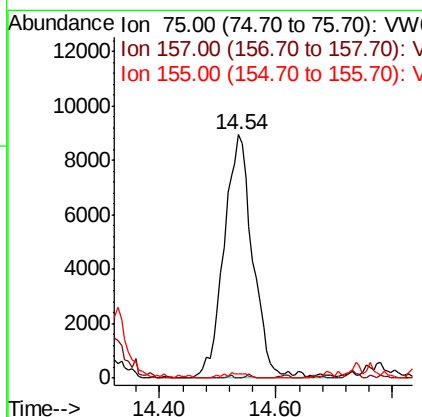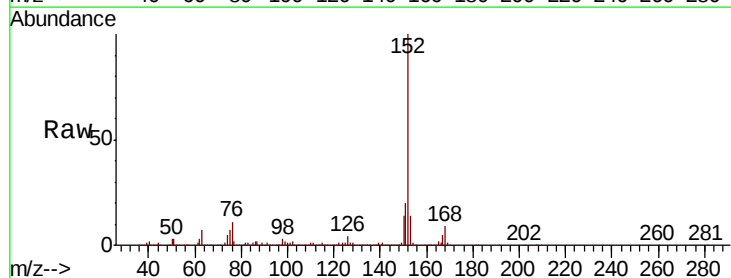

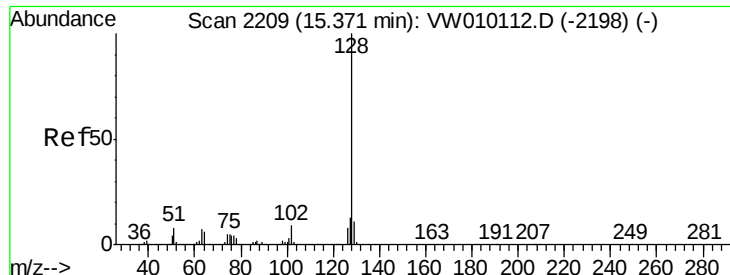

#69

Naphthalene

Concen: 13.881 ug/L

RT: 15.37 min Scan# 2209

Delta R.T. 0.00 min

Lab File: VW010117.D

Acq: 24 Apr 2019 18:41

Instrument :

MSVOA_W

ClientSampleId :

GAHW4

Tgt Ion:128 Resp: 398368

Ion Ratio Lower Upper

128 100

129 11.0 8.6 13.0

127 13.3 10.8 16.2

