

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042419\
 Data File : VW010132.D
 Acq On : 25 Apr 2019 08:05
 Operator : SY/VA
 Sample : K2497-05
 Misc : 5.10G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 GAHY1

Manual Integrations
APPROVED

MMDadoda
 4/30/2019 12:36:42 AM

Quant Time: Apr 25 09:11:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 09:08:51 2019
 Response via : Initial Calibration

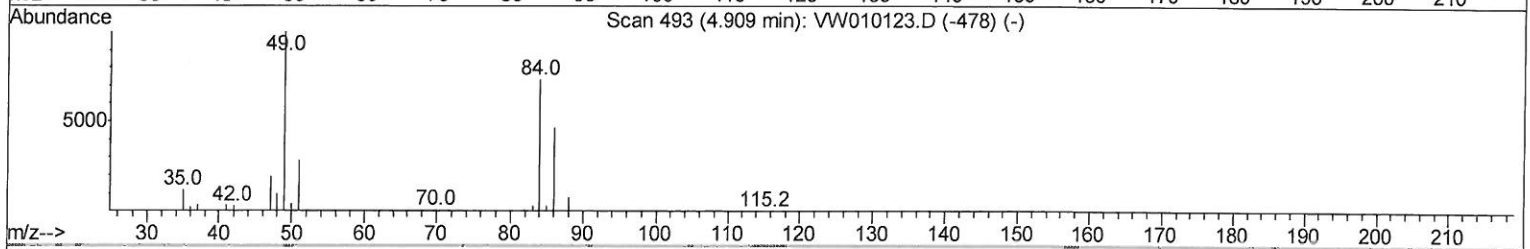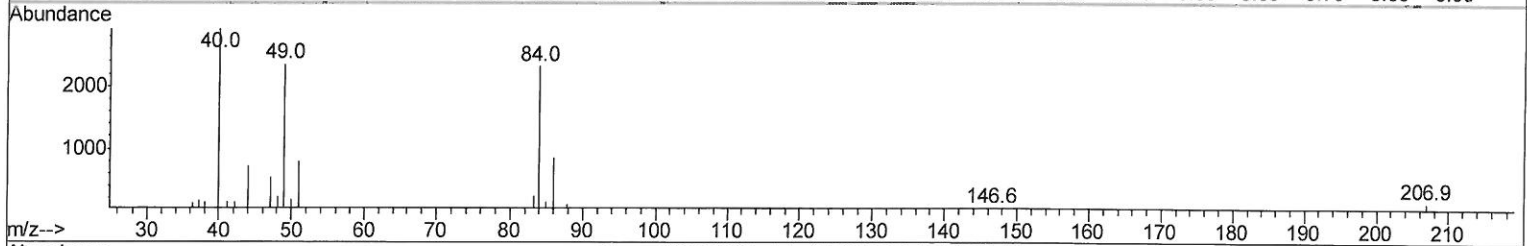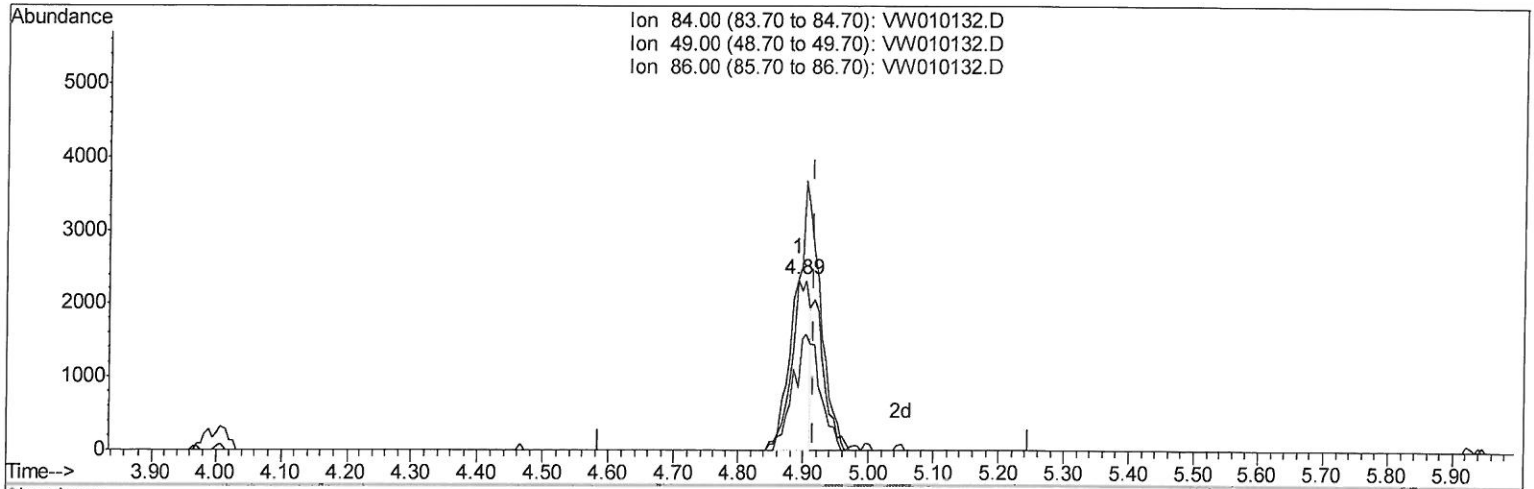

TIC: VW010132.D

(16) Methylene chloride (T)

4.891min (-0.024) 2.21ug/L

response 4541

Ion	Exp%	Act%
84.00	100	100
49.00	133.60	101.03
86.00	64.20	36.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042419\
 Data File : VW010132.D
 Acq On : 25 Apr 2019 08:05
 Operator : SY/VA
 Sample : K2497-05
 Misc : 5.10G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHY1

Manual Integrations
 APPROVED

MMDadoda
 4/30/2019 12:36:42 AM

Quant Time: Apr 25 09:11:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 09:08:51 2019
 Response via : Initial Calibration

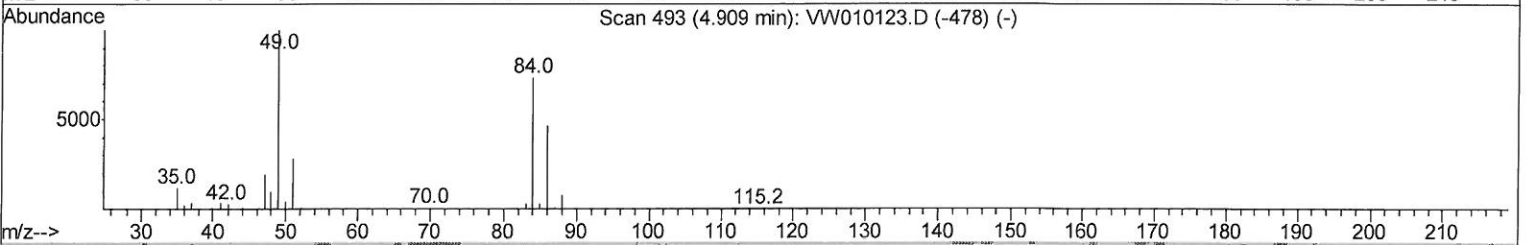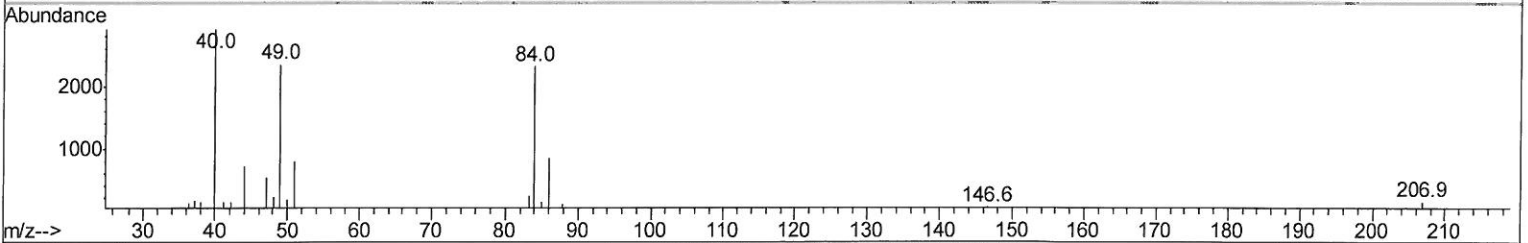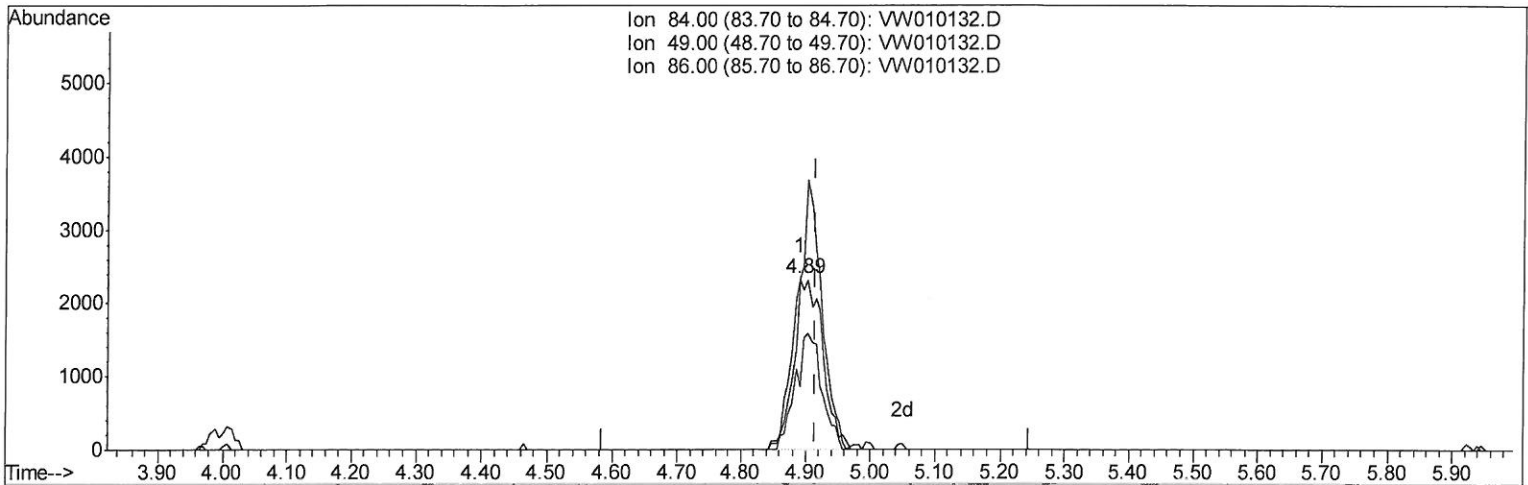

TIC: VW010132.D

(16) Methylene chloride (T)

4.891min (-0.024) 3.53ug/L m

04/28/19

response 7256

Ion	Exp%	Act%
84.00	100	100
49.00	133.60	101.03
86.00	64.20	36.65#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042419\
 Data File : VW010132.D
 Acq On : 25 Apr 2019 08:05
 Operator : SY/VA
 Sample : K2497-05
 Misc : 5.10G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAHY1

Manual Integrations
 APPROVED

MMDadoda
 4/30/2019 12:36:42 AM

Quant Time: Apr 25 09:13:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 09:08:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	146660	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	184581	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	77756	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	8030	5.73	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	22.92%#
7) Chloroethane-d5	2.89	69	15647	13.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.04%
10) 1,1-Dichloroethene-d2	4.00	63	24435	5.94	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	23.76%#
20) 2-Butanone-d5	7.09	46	52219	78.88	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	157.76%#
24) Chloroform-d	7.65	84	114484	29.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	117.28%
26) 1,2-Dichloroethane-d4	8.31	65	89442	39.17	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	156.68%#
29) Benzene-d6	8.27	84	186741	17.86	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.44%
33) 1,2-Dichloropropane-d6	9.27	67	87402	26.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.28%
37) Toluene-d8	10.32	98	150853	15.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	63.56%
38) trans-1,3-Dichloropropene-	10.58	79	31459	20.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.80%
39) 2-Hexanone-d5	10.93	63	33779	49.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.64%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	84385	31.19	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	124.76%#
61) 1,2-Dichlorobenzene-d4	13.86	152	76768	26.66	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.64%

Target Compounds

				Ovalue
13) Acetone	4.12	43	4632	9.271 ug/L 92
15) Methyl Acetate	4.67	43	5798	4.905 ug/L 98
16) Methylene chloride	4.89	84	7256m	3.530 ug/L
44) Toluene	10.39	91	28796	2.423 ug/L

04/28/19 SY

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042419\
Data File : VW010132.D
Acq On : 25 Apr 2019 08:05
Operator : SY/VA
Sample : K2497-05
Misc : 5.10G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAHY1

Manual Integrations
APPROVED

MMDadoda
4/30/2019 12:36:42 AM

Quant Time: Apr 25 09:13:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042419S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 25 09:08:51 2019
Response via : Initial Calibration

