


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW042420\
 Data File : VW015332.D
 Acq On : 24 Apr 2020 10:02
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W042020S.M
 Title : SW846 8260
 Last Update : Tue Apr 21 06:39:58 2020

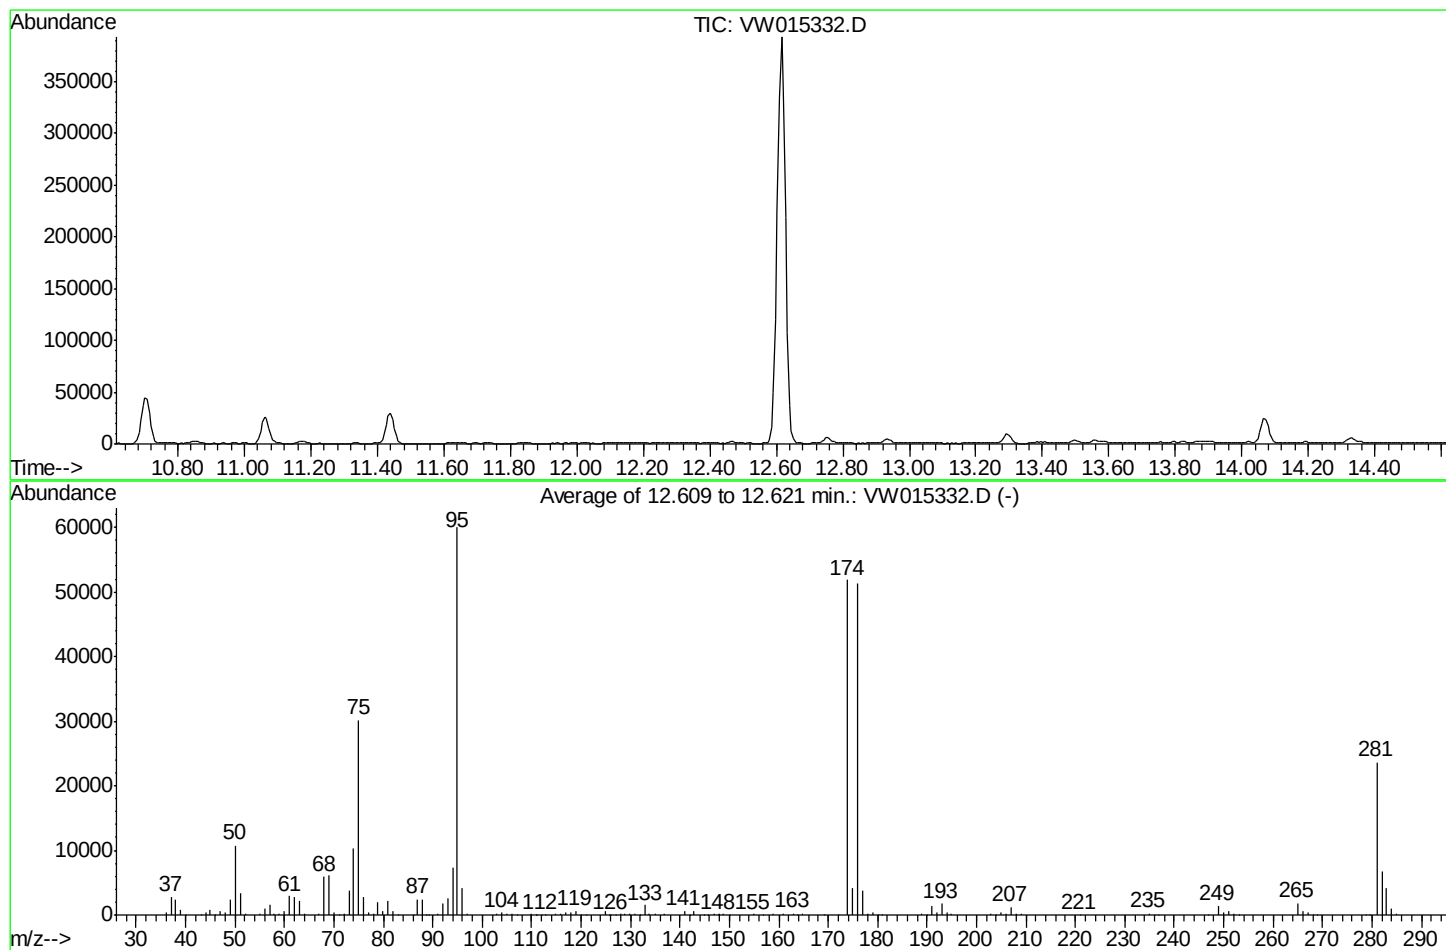

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	10765	PASS
75	95	30	60	50.2	30152	PASS
95	95	100	100	100.0	60008	PASS
96	95	5	9	7.0	4209	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.4	51829	PASS
175	174	5	9	7.9	4074	PASS
176	174	95	101	98.9	51282	PASS
177	176	5	9	7.4	3792	PASS