




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
 Data File : VW025660.D
 Acq On : 24 Apr 2023 15:40
 Operator : SY/MD
 Sample : 02479-01
 Misc : 2.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW942

Manual IntegrationsAPPROVED

Quant Time: Apr 25 01:12:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 25 01:06:51 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/25/2023
 Supervised By :Mahesh Dadoda 04/25/2023

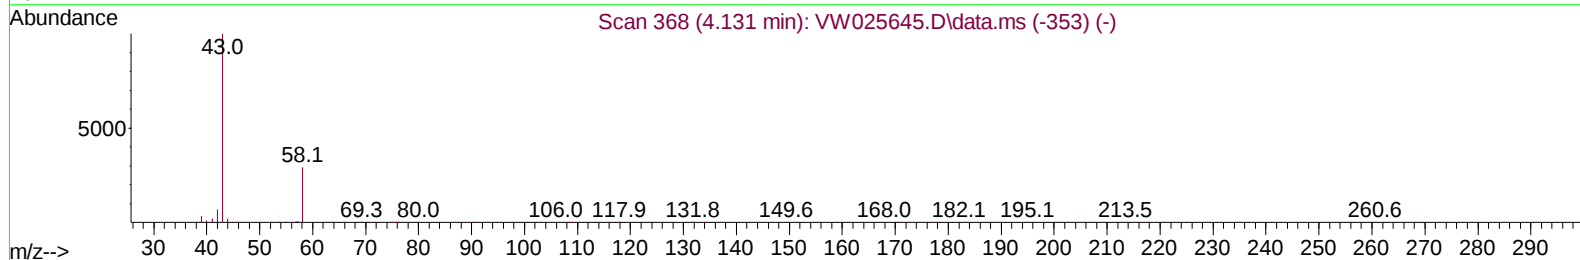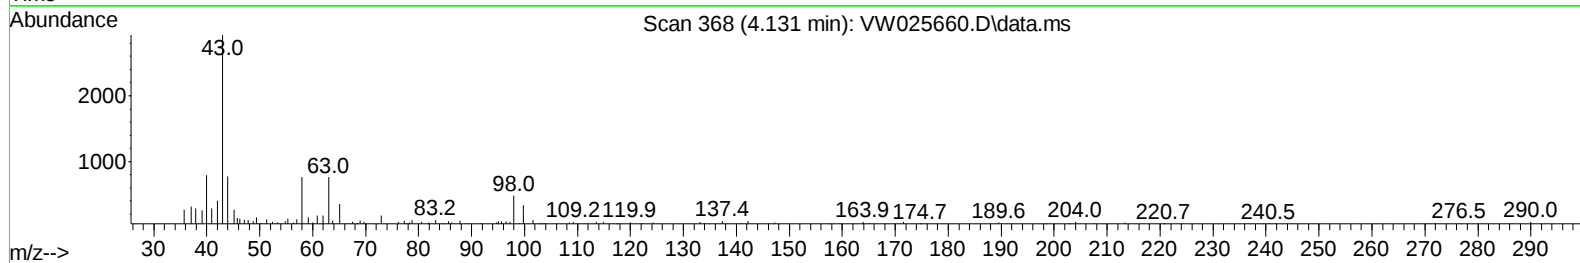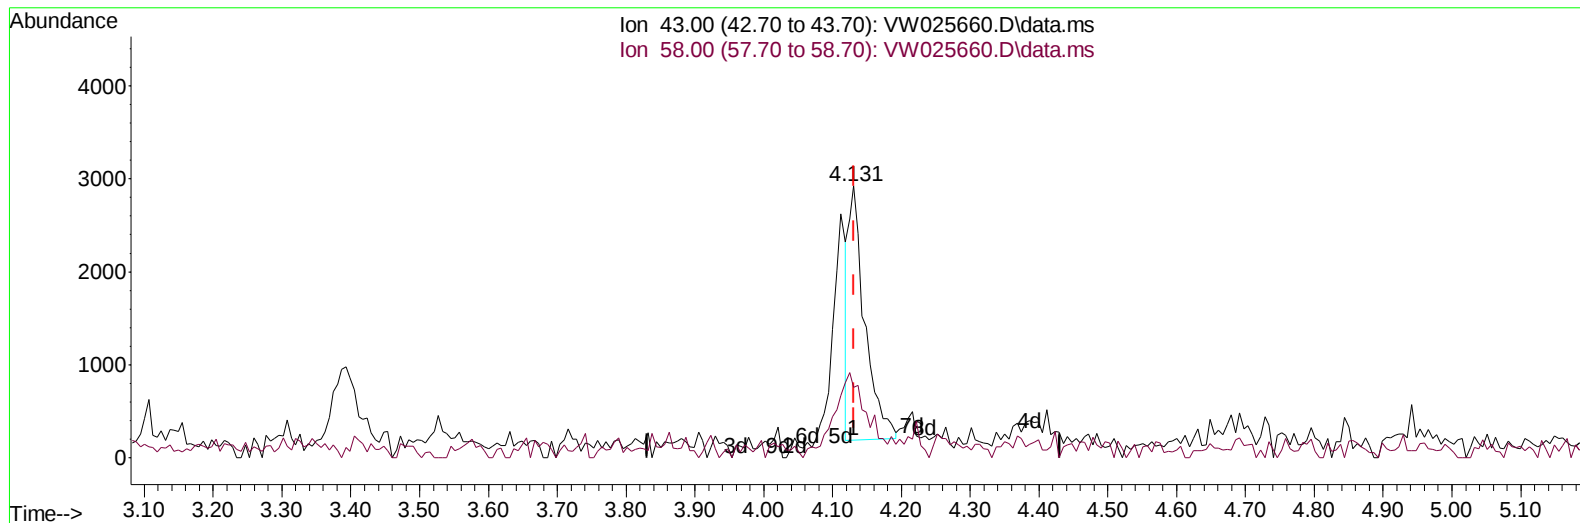

TIC: VW025660.D\data.ms

(13) Acetone (T)

4.131min (+ 0.000) 2.15 ug/L

response 4493

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.70	45.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
 Data File : VW025660.D
 Acq On : 24 Apr 2023 15:40
 Operator : SY/MD
 Sample : 02479-01
 Misc : 2.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW942

Manual IntegrationsAPPROVED

Quant Time: Apr 25 01:12:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 25 01:06:51 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/25/2023
 Supervised By :Mahesh Dadoda 04/25/2023

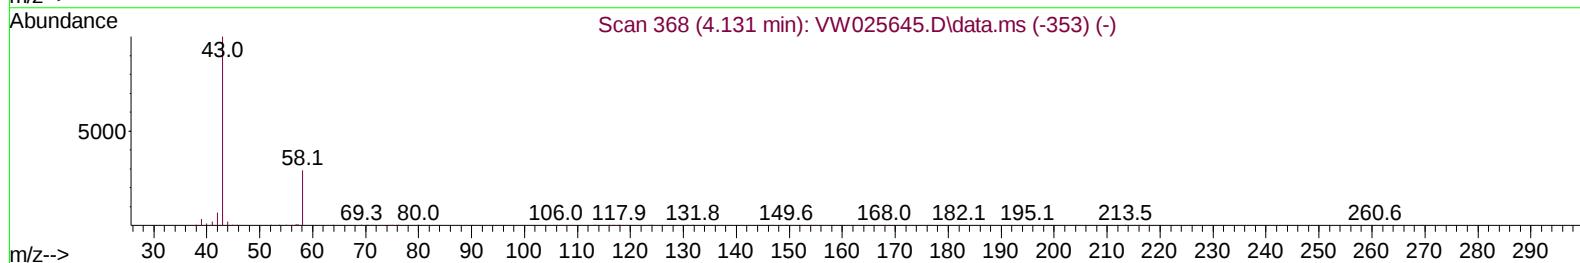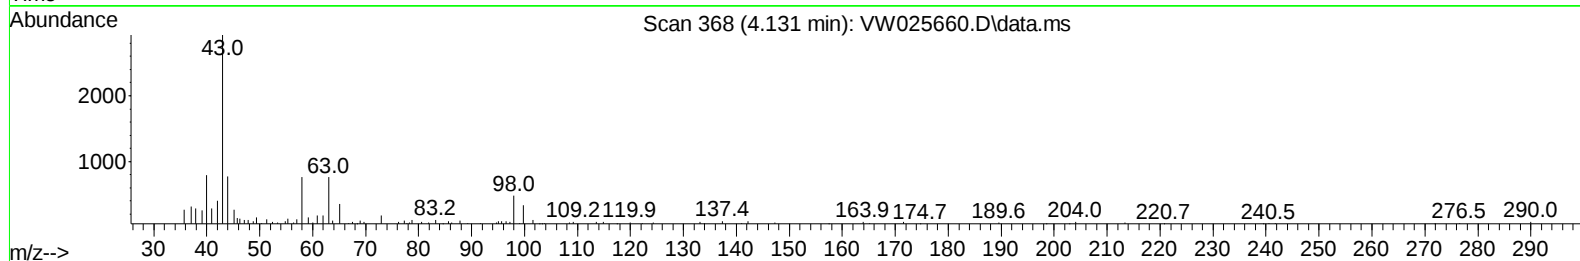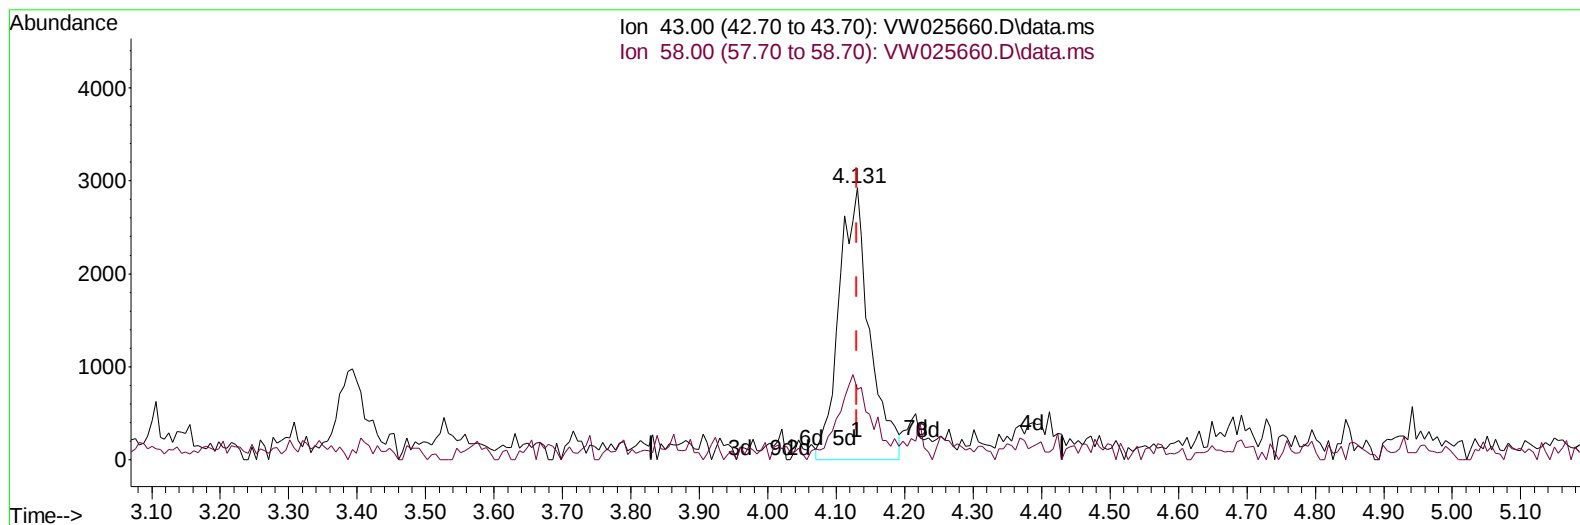

TIC: VW025660.D\data.ms

(13) Acetone (T)

4.131min (+ 0.000) 4.32 ug/L m

response 9029

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.70	22.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
 Data File : VW025660.D
 Acq On : 24 Apr 2023 15:40
 Operator : SY/MD
 Sample : 02479-01
 Misc : 2.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW942

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/25/2023
 Supervised By :Mahesh Dadoda 04/25/2023

Quant Time: Apr 25 01:12:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 25 01:06:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	680338	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	405613	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	79292	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	163060	14.729	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.920%	
7) Chloroethane-d5	2.899	69	146349	18.567	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.280%	
11) 1,1-Dichloroethene-d2	4.021	63	274791	12.273	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	49.080%	
21) 2-Butanone-d5	7.075	46	165222	66.897	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	133.800%	
24) Chloroform-d	7.642	84	418230	21.894	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	87.560%	
26) 1,2-Dichloroethane-d4	8.301	65	245958	24.750	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	99.000%	
32) Benzene-d6	8.270	84	775990	29.546	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	118.200%	
36) 1,2-Dichloropropane-d6	9.270	67	270707	33.057	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	132.240%#	
41) Toluene-d8	10.319	98	518301	22.592	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	90.360%	
43) trans-1,3-Dichloroprop...	10.575	79	85969	28.001	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	112.000%	
47) 2-Hexanone-d5	10.922	63	95952	85.722	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	171.440%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	150385	27.208	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.840%	
66) 1,2-Dichlorobenzene-d4	13.848	152	59173	21.722	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	86.880%	
Target Compounds					Qvalue	
13) Acetone	4.131	43	9029m	4.319	ug/L	
16) Methylene chloride	4.911	84	34690	3.208	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
Data File : VW025660.D
Acq On : 24 Apr 2023 15:40
Operator : SY/MD
Sample : 02479-01
Misc : 2.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW942

Manual IntegrationsAPPROVED

Quant Time: Apr 25 01:12:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 25 01:06:51 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/25/2023
Supervised By :Mahesh Dadoda 04/25/2023

