




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
 Data File : VW025663.D
 Acq On : 24 Apr 2023 16:51
 Operator : SY/MD
 Sample : 02479-07
 Misc : 4.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/25/2023
 Supervised By :Mahesh Dadoda 04/25/2023

Quant Time: Apr 25 01:13:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 25 01:06:51 2023
 Response via : Initial Calibration

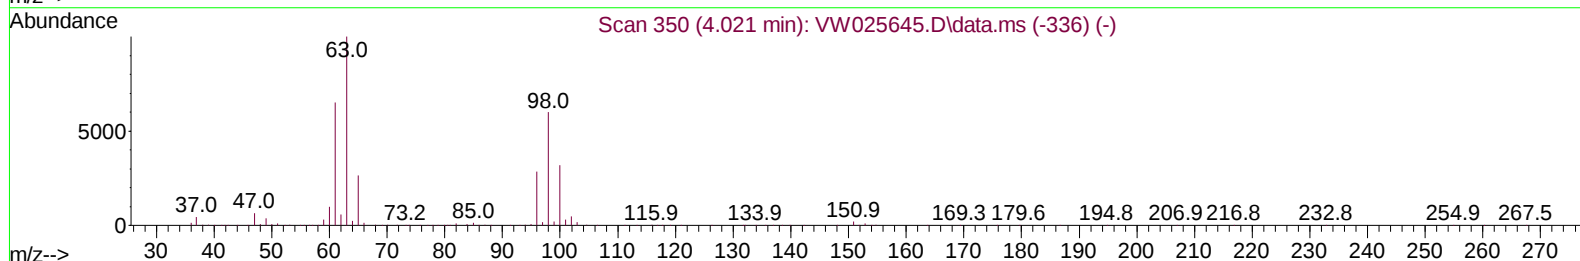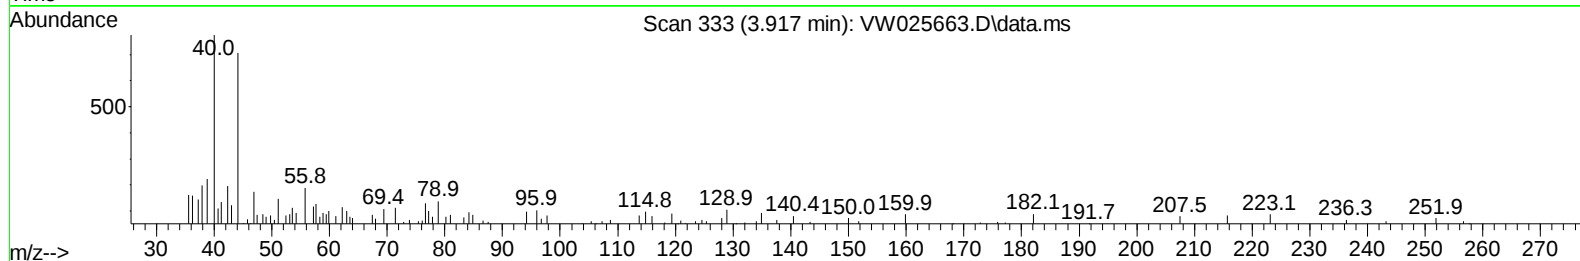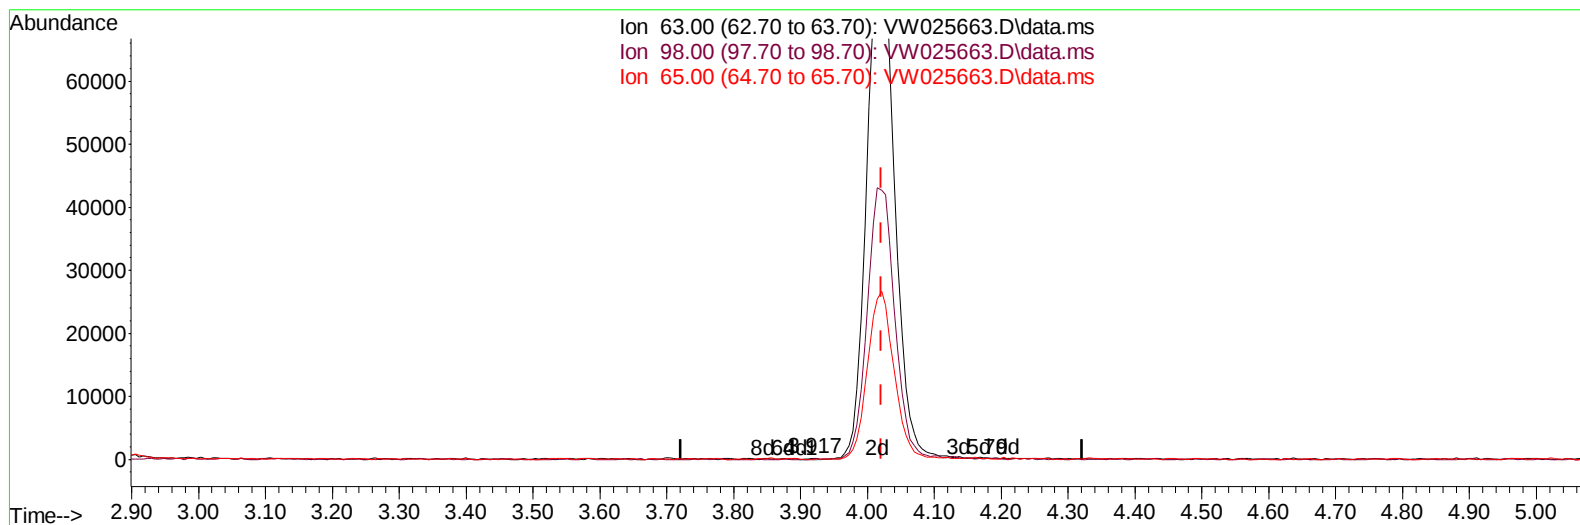

TIC: VW025663.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.917min (-0.104) 0.01 ug/L

response 201

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	68.16
65.00	23.30	25.37
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
 Data File : VW025663.D
 Acq On : 24 Apr 2023 16:51
 Operator : SY/MD
 Sample : 02479-07
 Misc : 4.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/25/2023
 Supervised By :Mahesh Dadoda 04/25/2023

Quant Time: Apr 25 01:13:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 25 01:06:51 2023
 Response via : Initial Calibration

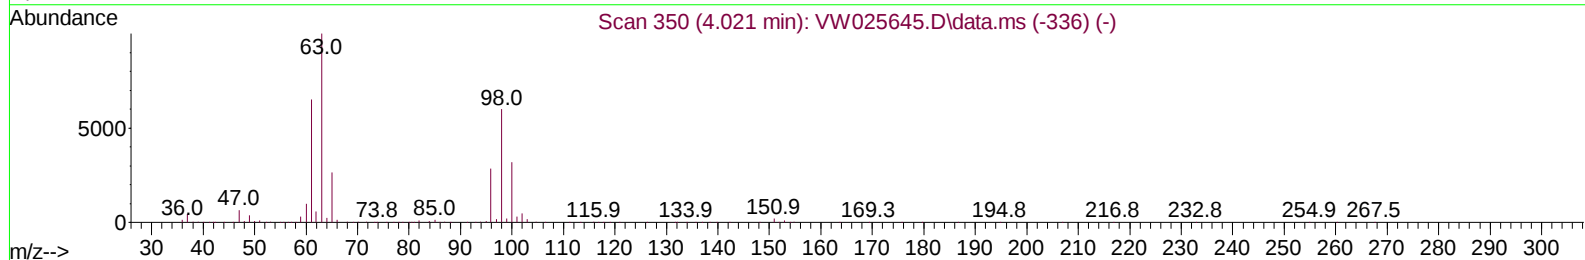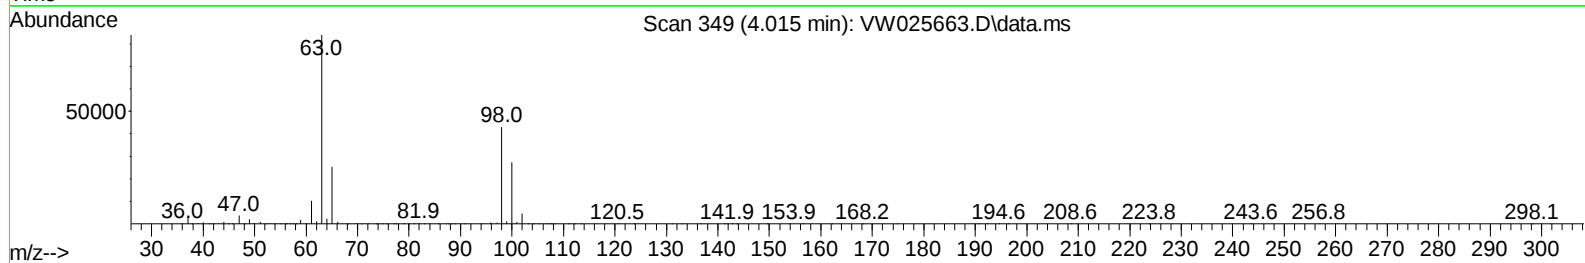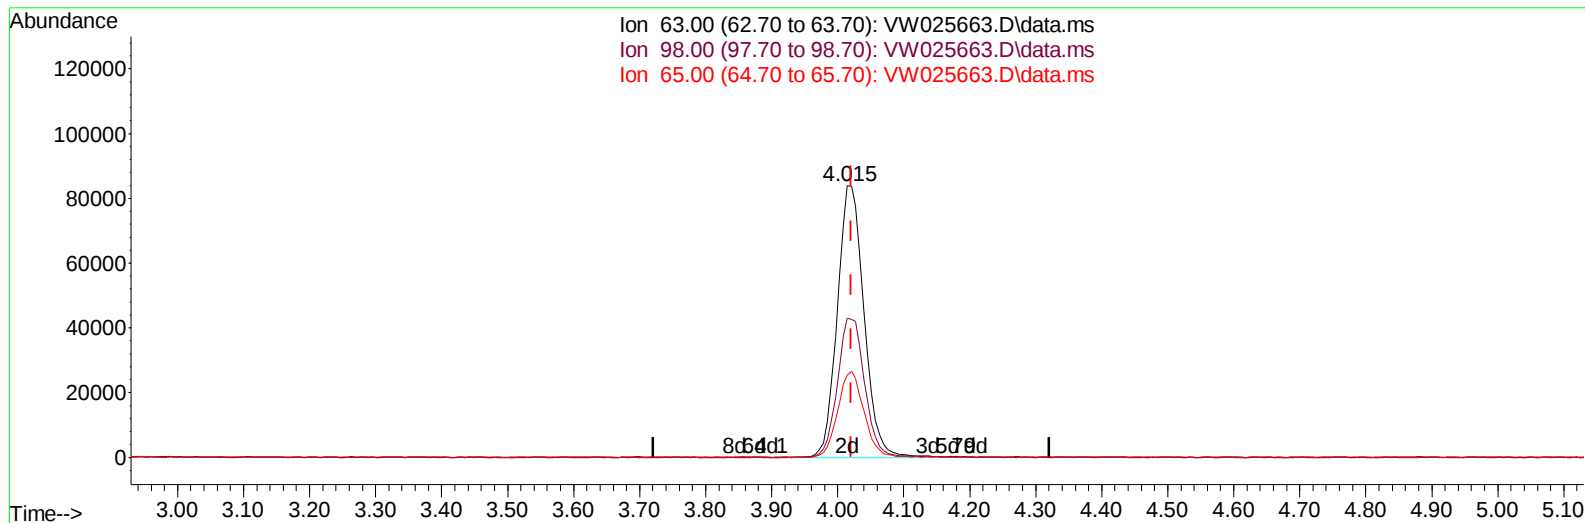

TIC: VW025663.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.015min (-0.006) 13.35 ug/L m

response 235747

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.70	0.06#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
 Data File : VW025663.D
 Acq On : 24 Apr 2023 16:51
 Operator : SY/MD
 Sample : 02479-07
 Misc : 4.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Quant Time: Apr 25 01:13:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 25 01:06:51 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/25/2023
 Supervised By :Mahesh Dadoda 04/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	536589	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	435958	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	144267	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	131329	15.040	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.160%	
7) Chloroethane-d5	2.899	69	116482	18.737	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.960%	
11) 1,1-Dichloroethene-d2	4.015	63	235747m	13.350	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.400%	
21) 2-Butanone-d5	7.075	46	105052	53.929	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.860%	
24) Chloroform-d	7.648	84	349843	23.220	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.880%	
26) 1,2-Dichloroethane-d4	8.307	65	194805	24.854	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	99.400%	
32) Benzene-d6	8.276	84	671564	23.790	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	95.160%	
36) 1,2-Dichloropropane-d6	9.276	67	232037	26.362	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	105.440%	
41) Toluene-d8	10.325	98	540944	21.937	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.760%	
43) trans-1,3-Dichloroprop...	10.575	79	75660	22.928	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.720%	
47) 2-Hexanone-d5	10.922	63	65212	54.204	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.400%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	159688	26.880	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	107.520%	
66) 1,2-Dichlorobenzene-d4	13.848	152	121229	24.460	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.840%	
Target Compounds						
					Qvalue	
13) Acetone	4.125	43	21630	13.120	ug/L	99
16) Methylene chloride	4.917	84	25472	2.986	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042423\
Data File : VW025663.D
Acq On : 24 Apr 2023 16:51
Operator : SY/MD
Sample : 02479-07
Misc : 4.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW948

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/25/2023
Supervised By :Mahesh Dadoda 04/25/2023

Quant Time: Apr 25 01:13:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 25 01:06:51 2023
Response via : Initial Calibration

