

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	322249	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	304633	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159625	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	137227	19.263	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.040%
7) Chloroethane-d5	2.892	69	90716	20.318	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.280%
11) 1,1-Dichloroethene-d2	4.019	63	156976	16.989	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.960%
21) 2-Butanone-d5	7.177	46	602	0.484	ug/L	0.10
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.960%#
24) Chloroform-d	7.653	84	225731	22.411	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.640%
26) 1,2-Dichloroethane-d4	8.305	65	122478	21.282	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.120%
32) Benzene-d6	8.275	84	454200	24.404	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	9.275	67	126527	23.492	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.960%
41) Toluene-d8	10.323	98	423506	23.233	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.920%
43) trans-1,3-Dichloroprop...	10.579	79	51491	20.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.040%
47) 2-Hexanone-d5	10.921	63	39608	39.525	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.060%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	99515	21.730	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.920%
66) 1,2-Dichlorobenzene-d4	13.847	152	134926	23.864	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.440%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.031	75	4995	0.635	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022608.D
Acq On : 25 Apr 2022 10:58
Operator : SY/VA
Sample : VW0425SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK485

Quant Time: Apr 26 01:35:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

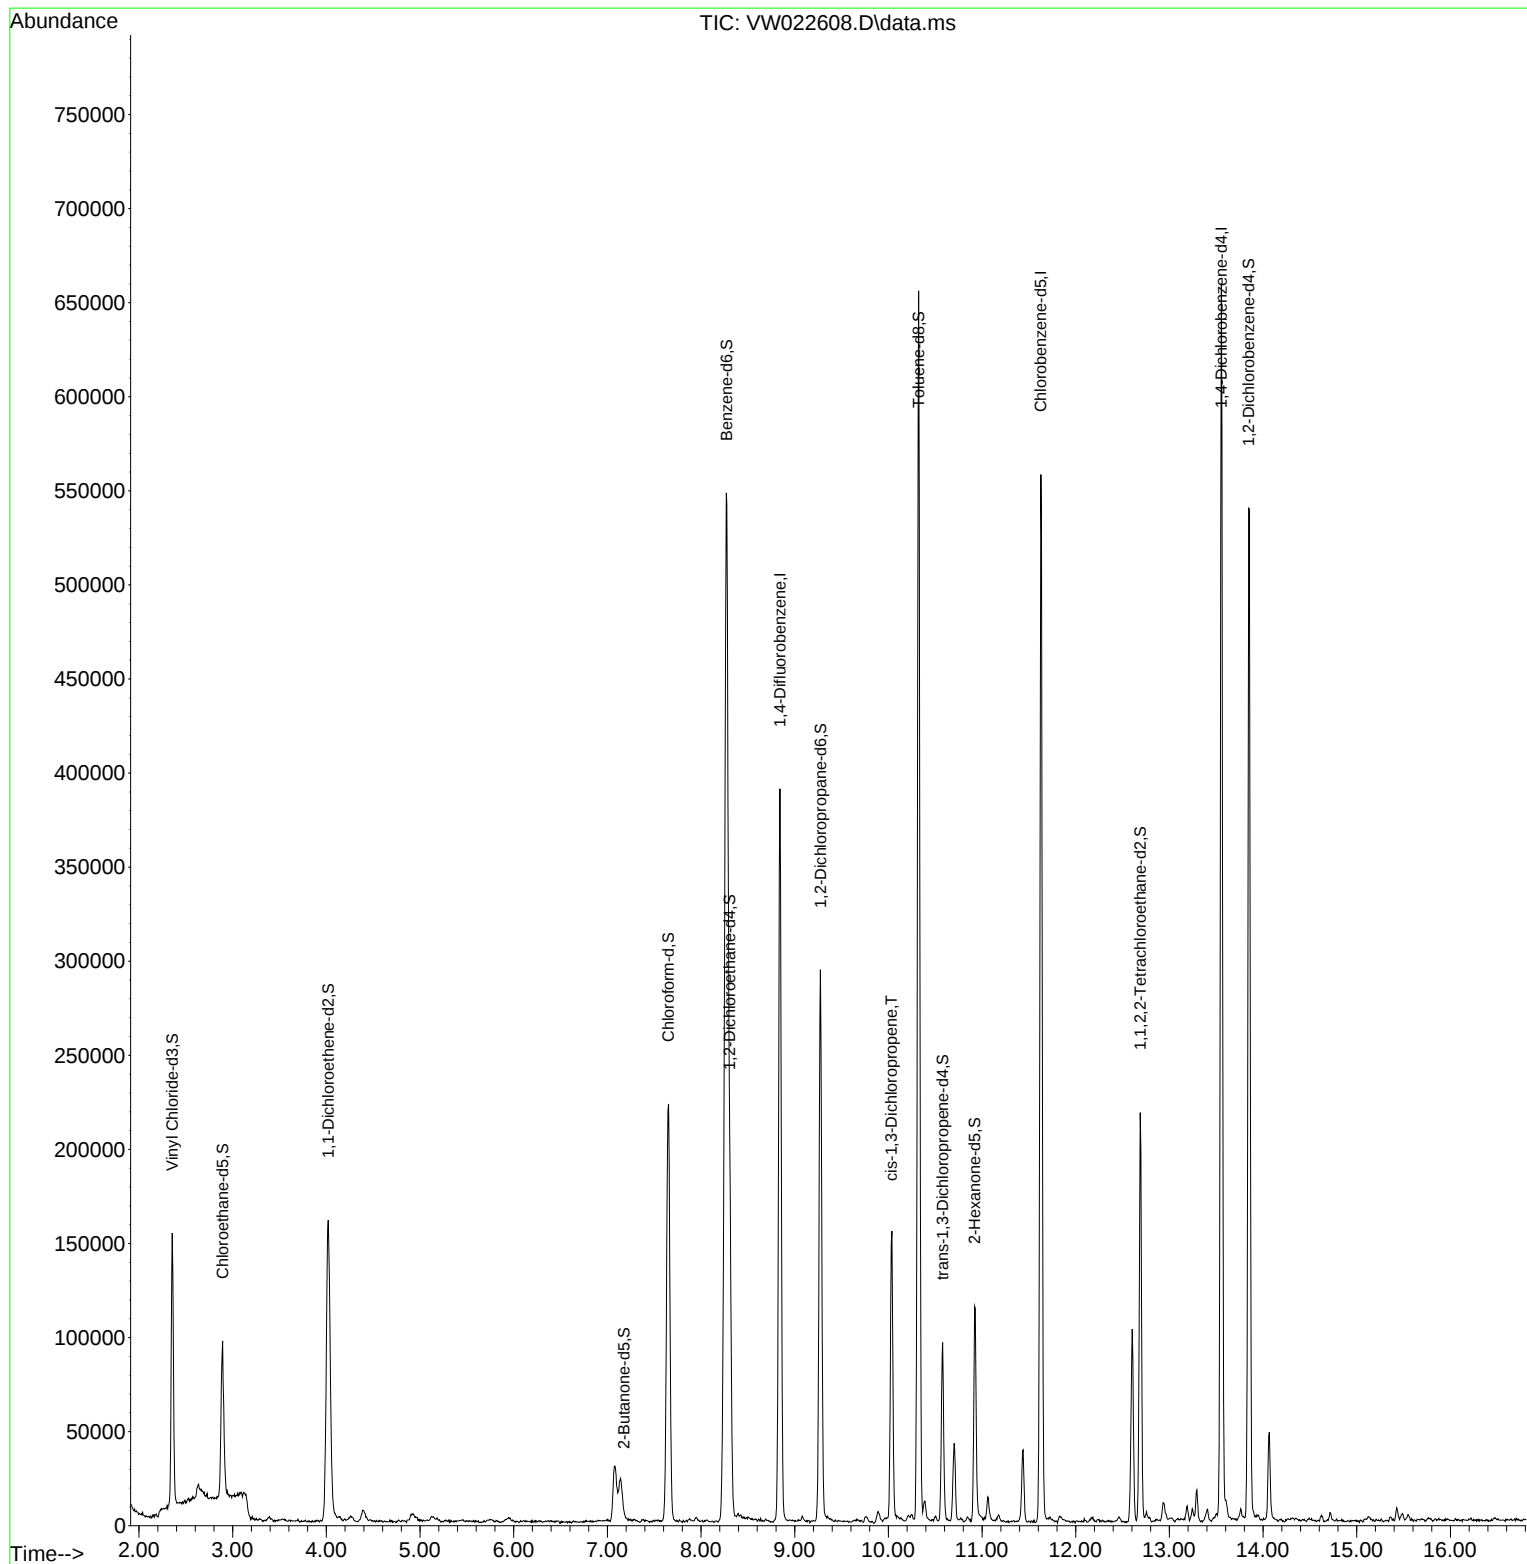

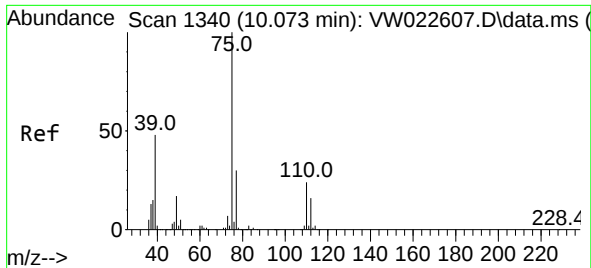

#39

cis-1,3-Dichloropropene

Concen: 0.635 ug/L

RT: 10.031 min Scan# 11

Delta R.T. -0.042 min

Lab File: VW022608.D


Acq: 25 Apr 2022 10:58

Instrument :

MSVOA_W

ClientSampleId :

VBLK485

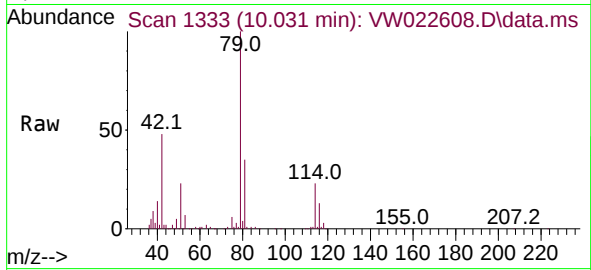

Tgt Ion: 75 Resp: 4995

Ion Ratio Lower Upper

75 100

77 43.5 22.6 42.0#

