

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022610.D
 Acq On : 25 Apr 2022 16:25
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK432

Quant Time: Apr 26 01:36:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	302971	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	295245	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	157466	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	143768	21.465	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.880%
7) Chloroethane-d5	2.885	69	88194	21.010	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.040%
11) 1,1-Dichloroethene-d2	4.019	63	152500	17.555	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.200%
21) 2-Butanone-d5	7.086	46	50916	43.542	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.080%
24) Chloroform-d	7.653	84	228493	24.128	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.520%
26) 1,2-Dichloroethane-d4	8.427	65	166	0.031	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.275	84	453766	25.156	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.640%
36) 1,2-Dichloropropane-d6	9.275	67	128140	24.547	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.200%
41) Toluene-d8	10.323	98	428190	24.237	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.960%
43) trans-1,3-Dichloroprop...	10.579	79	53575	21.747	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.000%
47) 2-Hexanone-d5	10.927	63	43281	44.564	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.120%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	102847	23.171	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.680%
66) 1,2-Dichlorobenzene-d4	13.853	152	139278	24.972	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	5297	0.695	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022610.D
Acq On : 25 Apr 2022 16:25
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK432

Quant Time: Apr 26 01:36:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

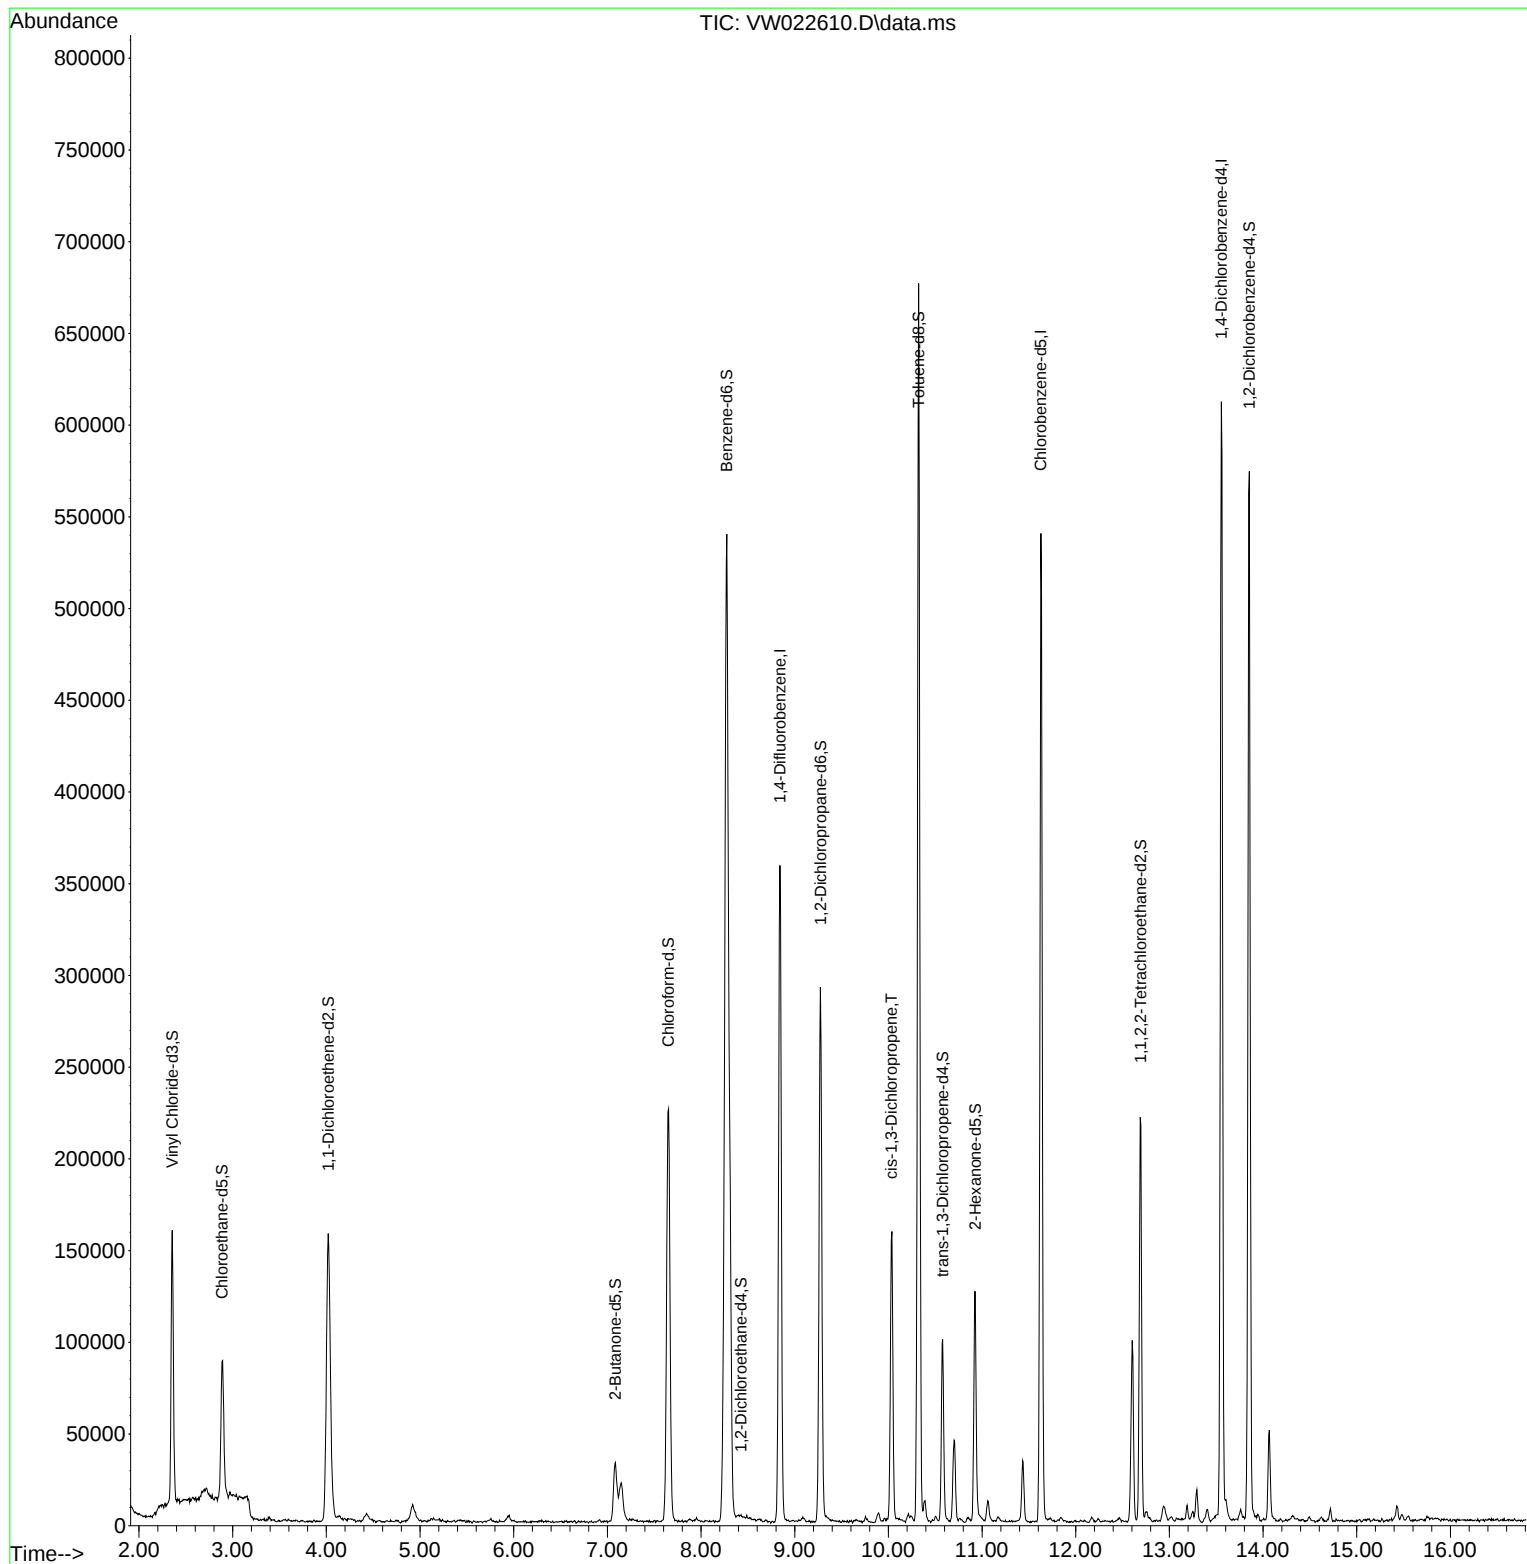

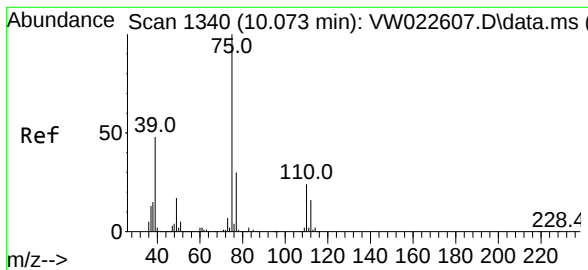

#39
 cis-1,3-Dichloropropene
 Concen: 0.695 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VW022610.D
 Acq: 25 Apr 2022 16:25

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK432

Tgt Ion: 75 Resp: 5297
 Ion Ratio Lower Upper
 75 100
 77 44.4 22.6 42.0#

