




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

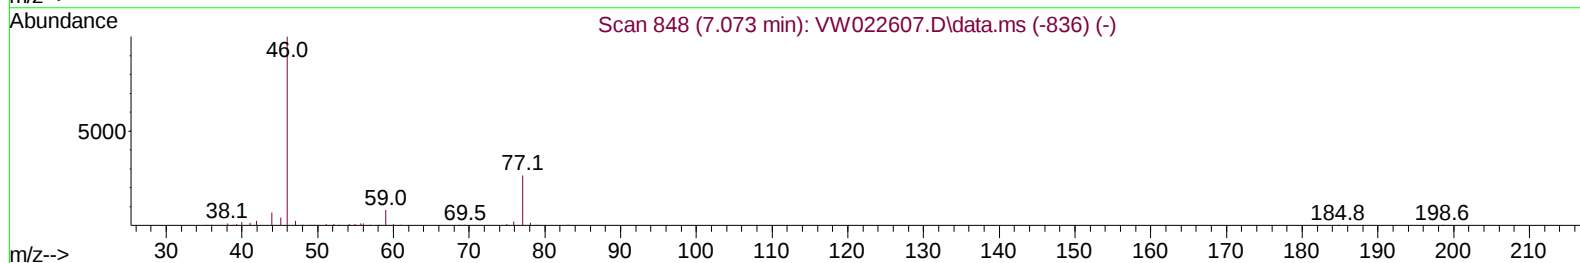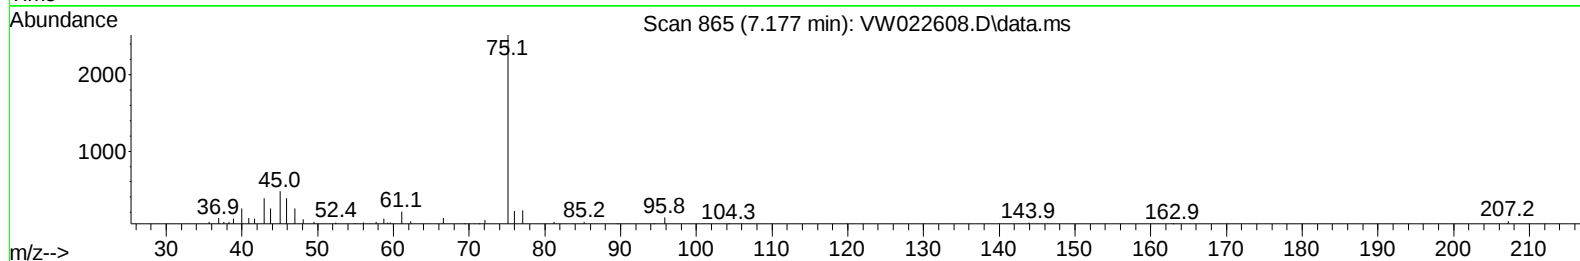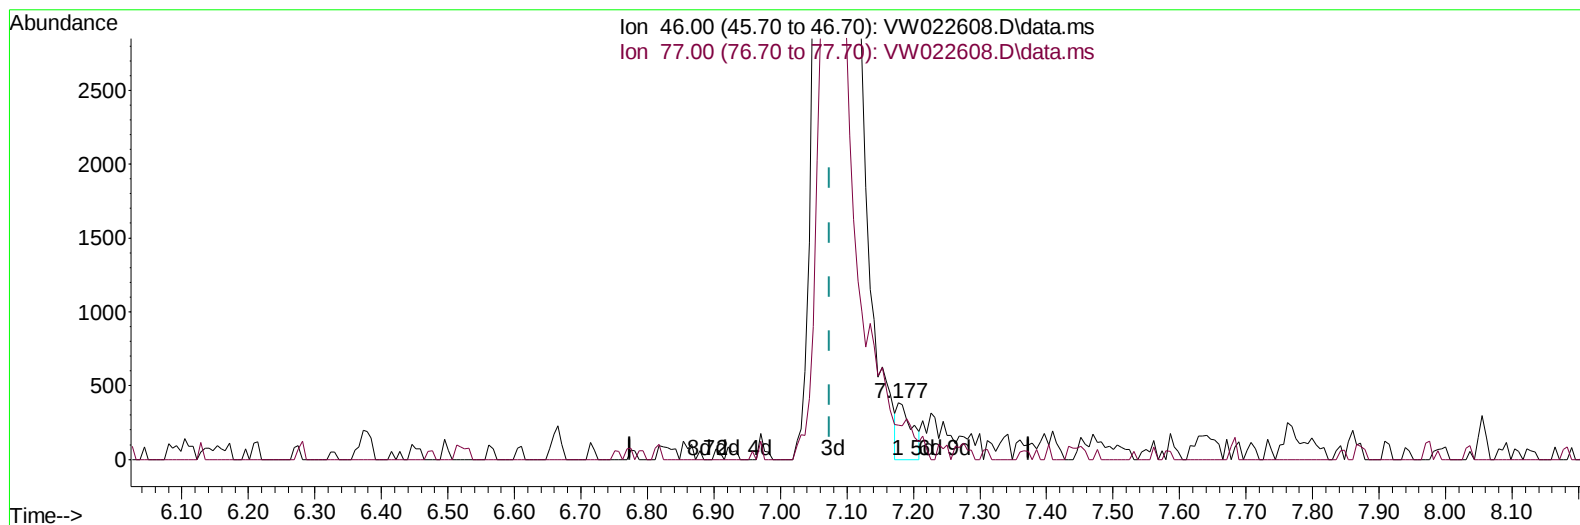

TIC: VW022608.D\data.ms

(21) 2-Butanone-d5 (S)

7.177min (+ 0.104) 0.48 ug/L

response 602

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	18.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

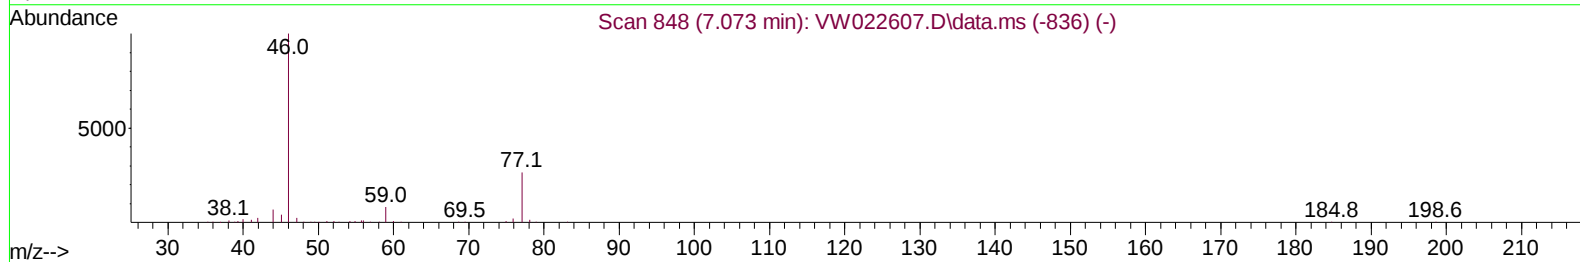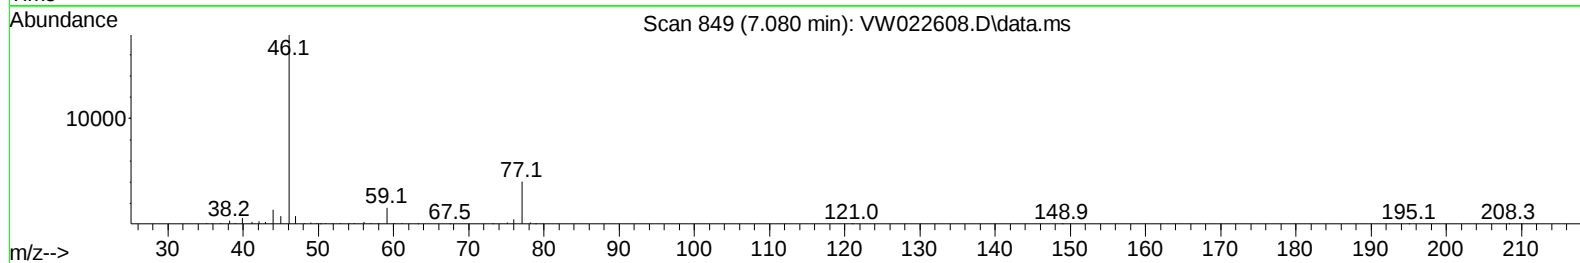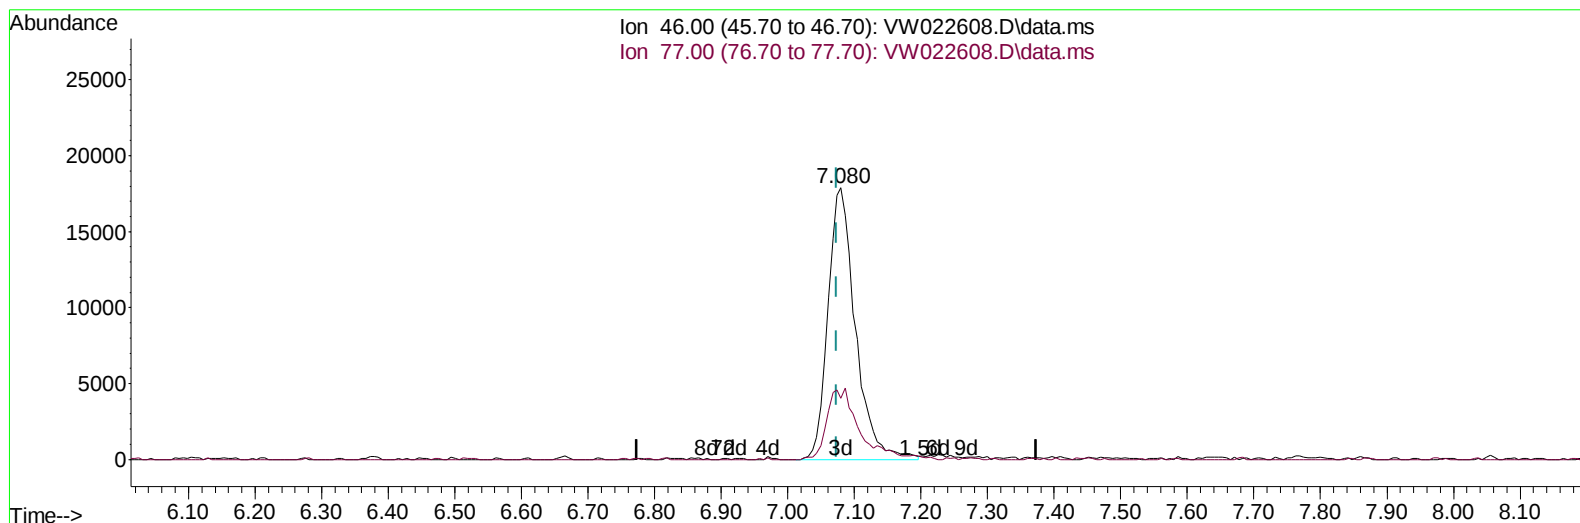

TIC: VW022608.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 41.01 ug/L m

response 51011

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	0.21#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

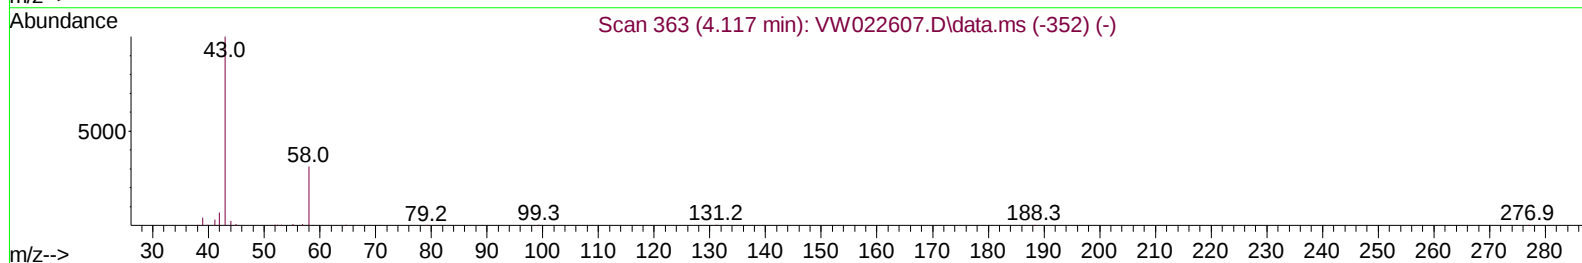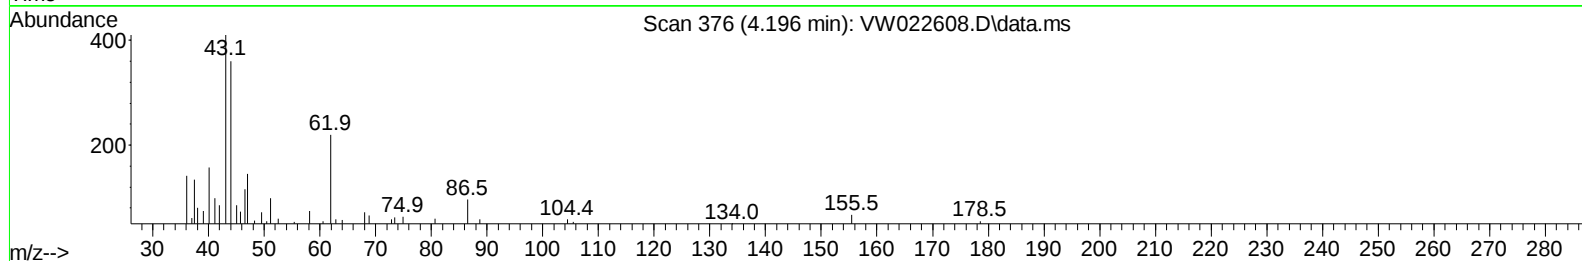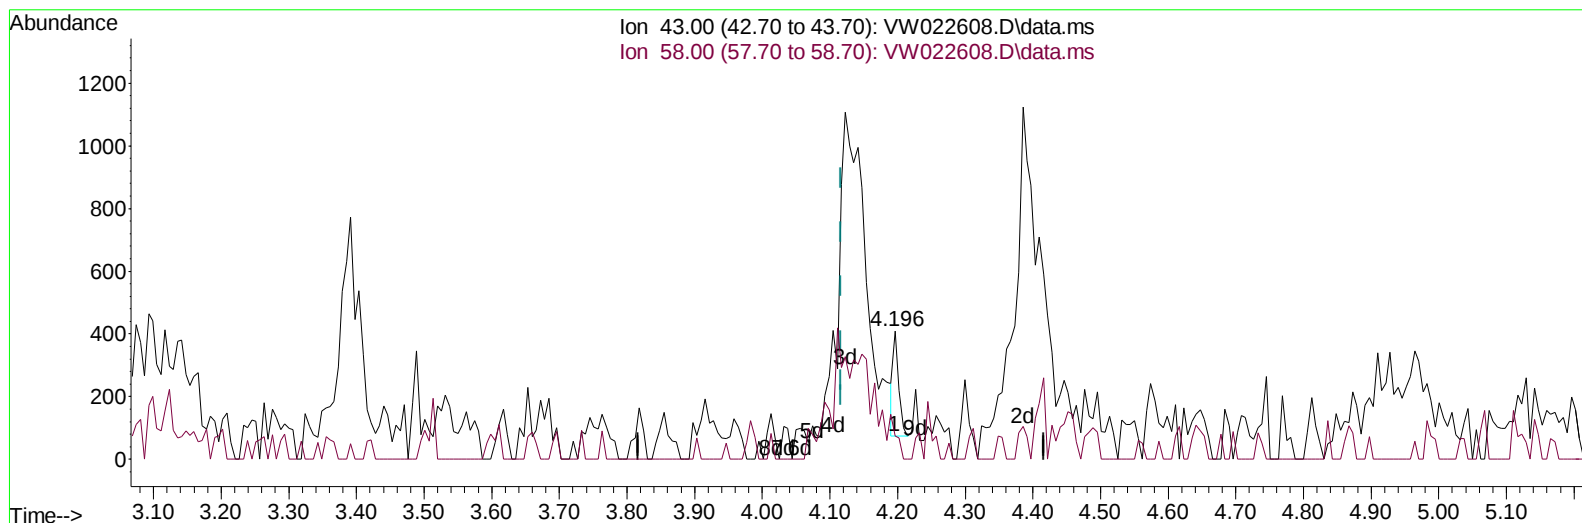

TIC: VW022608.D\data.ms

(13) Acetone (T)

4.196min (+ 0.079) 0.22 ug/L

response 185

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	56.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

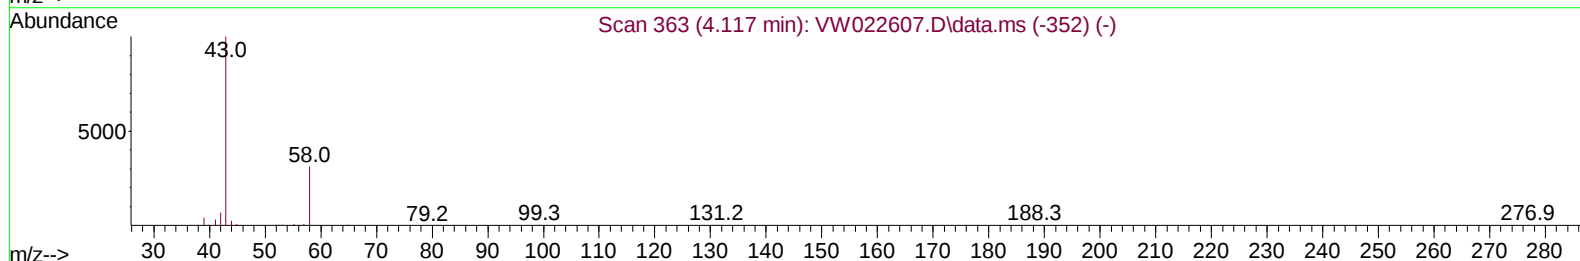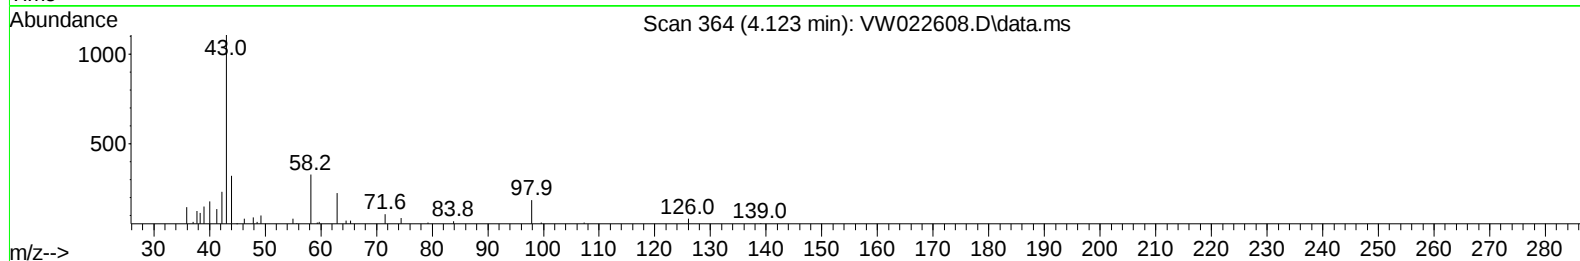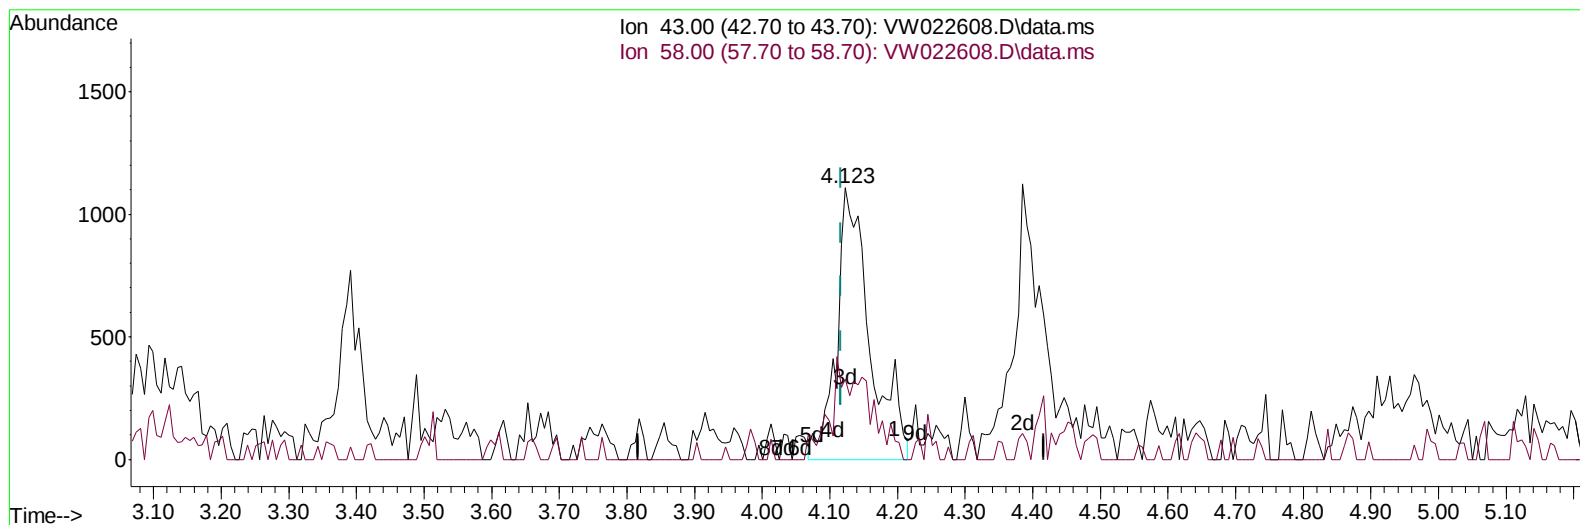

TIC: VW022608.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 4.43 ug/L m

response 3754

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	2.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		322249	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		304633	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		159625	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		137227	19.263	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	77.040%		
7) Chloroethane-d5	2.892	69		90716	20.318	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.280%		
11) 1,1-Dichloroethene-d2	4.019	63		156976	16.989	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	67.960%		
21) 2-Butanone-d5	7.080	46		51011m	41.014	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	82.020%		
24) Chloroform-d	7.653	84		225731	22.411	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	89.640%		
26) 1,2-Dichloroethane-d4	8.305	65		122478	21.282	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	85.120%		
32) Benzene-d6	8.275	84		454200	24.404	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	97.600%		
36) 1,2-Dichloropropane-d6	9.275	67		126527	23.492	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	93.960%		
41) Toluene-d8	10.323	98		423506	23.233	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	92.920%		
43) trans-1,3-Dichloroprop...	10.579	79		51491	20.257	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	81.040%		
47) 2-Hexanone-d5	10.921	63		39608	39.525	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	79.060%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		99515	21.730	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	86.920%		
66) 1,2-Dichlorobenzene-d4	13.847	152		134926	23.864	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	95.440%		
Target Compounds							Qvalue
13) Acetone	4.123	43		3754m	4.433	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022608.D
Acq On : 25 Apr 2022 10:58
Operator : SY/VA
Sample : VW0425SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK485

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:35:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

