




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022611.D
Acq On : 25 Apr 2022 16:59
Operator : SY/VA
Sample : N2316-15
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:36:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

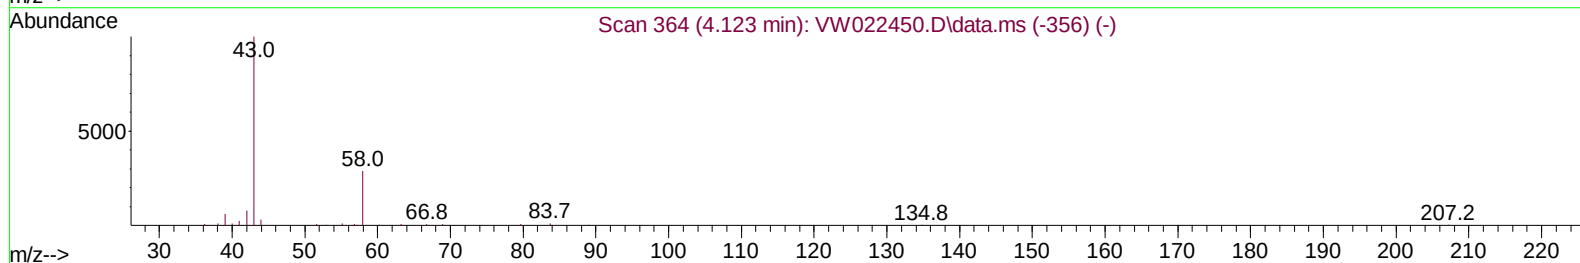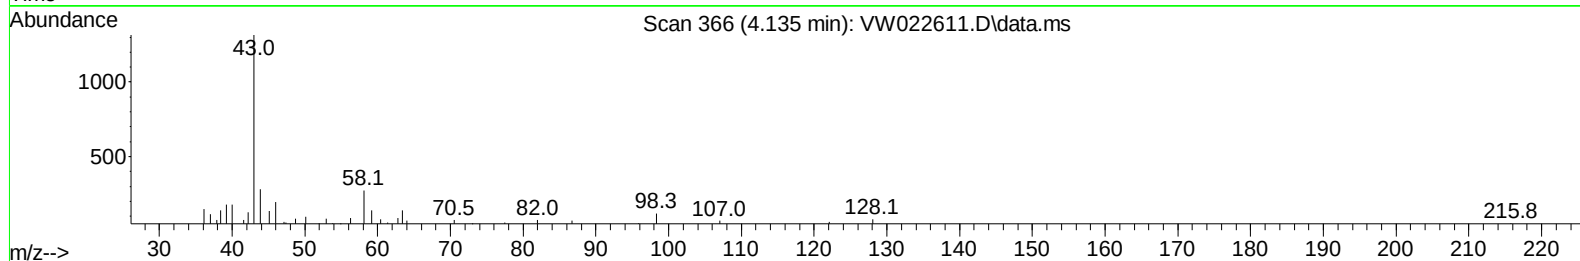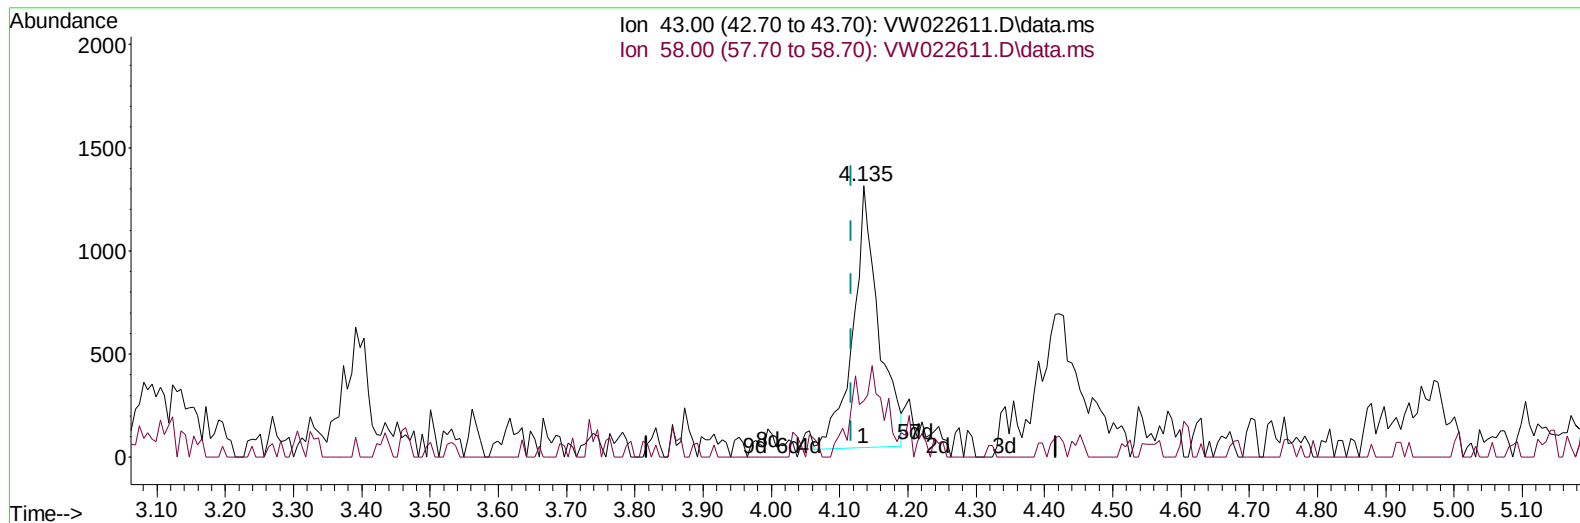

TIC: VW022611.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 4.05 ug/L

response 3292

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	9.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022611.D
 Acq On : 25 Apr 2022 16:59
 Operator : SY/VA
 Sample : N2316-15
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:36:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

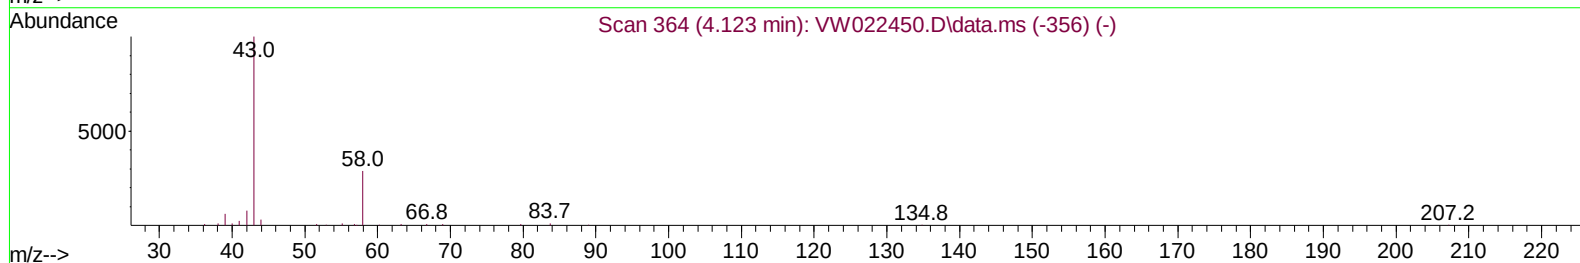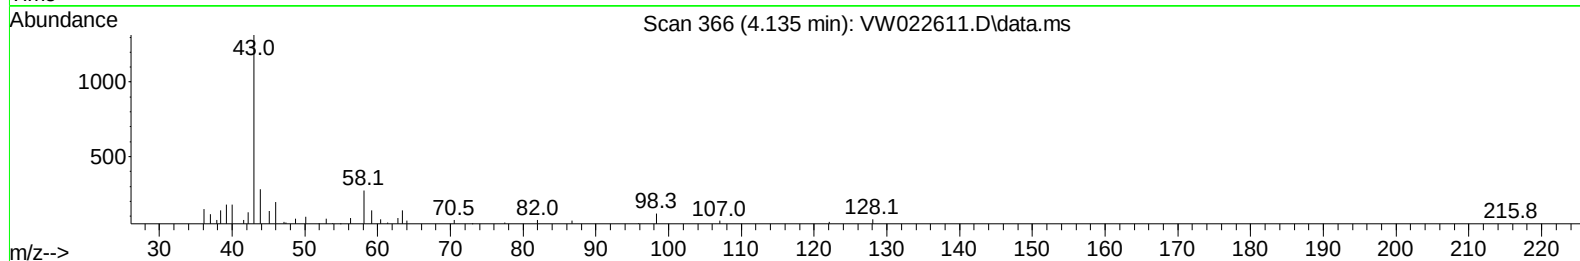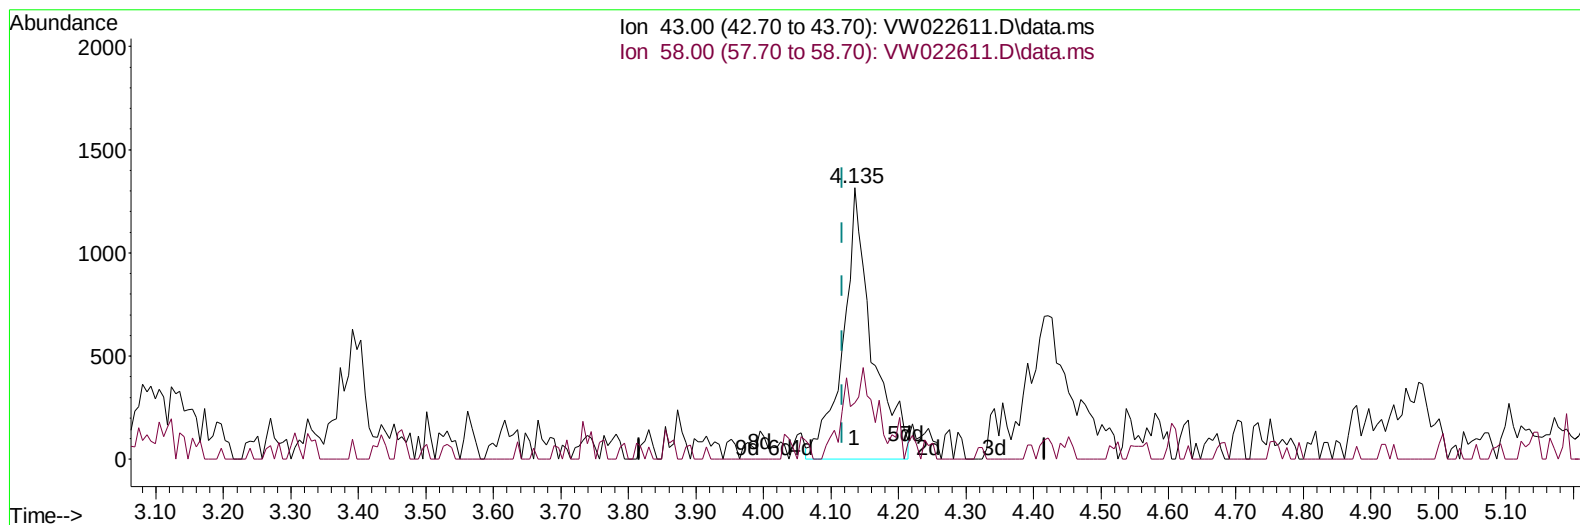

TIC: VW022611.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 4.83 ug/L m

response 3933

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	8.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022611.D
 Acq On : 25 Apr 2022 16:59
 Operator : SY/VA
 Sample : N2316-15
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:36:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		309662	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		301841	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		157945	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		142435	20.807	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.240%	
7) Chloroethane-d5	2.885	69		88626	20.657	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.640%	
11) 1,1-Dichloroethene-d2	4.019	63		157412	17.729	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	70.920%	
21) 2-Butanone-d5	7.080	46		56470	47.249	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	94.500%	
24) Chloroform-d	7.647	84		233351	24.109	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	96.440%	
26) 1,2-Dichloroethane-d4	8.305	65		131427	23.765	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	95.080%	
32) Benzene-d6	8.275	84		460913	24.994	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	99.960%	
36) 1,2-Dichloropropane-d6	9.274	67		131451	24.631	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	98.520%	
41) Toluene-d8	10.323	98		441556	24.448	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	97.800%	
43) trans-1,3-Dichloroprop...	10.579	79		53657	21.304	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	85.200%	
47) 2-Hexanone-d5	10.921	63		47377	47.715	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.440%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		112259	24.739	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	98.960%	
66) 1,2-Dichlorobenzene-d4	13.847	152		140955	25.196	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	100.800%	
Target Compounds							Qvalue
13) Acetone	4.135	43		3933m	4.833	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022611.D
Acq On : 25 Apr 2022 16:59
Operator : SY/VA
Sample : N2316-15
Misc : 5.08g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:36:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

