

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022608.D
 Acq On : 25 Apr 2022 10:58
 Operator : SY/VA
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:35:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	322249	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	304633	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159625	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	137227	19.263	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.040%		
7) Chloroethane-d5	2.892	69	90716	20.318	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.280%		
11) 1,1-Dichloroethene-d2	4.019	63	156976	16.989	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.960%		
21) 2-Butanone-d5	7.080	46	51011m	41.014	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.020%		
24) Chloroform-d	7.653	84	225731	22.411	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.640%		
26) 1,2-Dichloroethane-d4	8.305	65	122478	21.282	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.120%		
32) Benzene-d6	8.275	84	454200	24.404	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.600%		
36) 1,2-Dichloropropane-d6	9.275	67	126527	23.492	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.960%		
41) Toluene-d8	10.323	98	423506	23.233	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	92.920%		
43) trans-1,3-Dichloroprop...	10.579	79	51491	20.257	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.040%		
47) 2-Hexanone-d5	10.921	63	39608	39.525	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.060%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	99515	21.730	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	86.920%		
66) 1,2-Dichlorobenzene-d4	13.847	152	134926	23.864	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	95.440%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	3754m	4.433	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022608.D
Acq On : 25 Apr 2022 10:58
Operator : SY/VA
Sample : VW0425SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VBLK485

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022


Quant Time: Apr 26 01:35:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

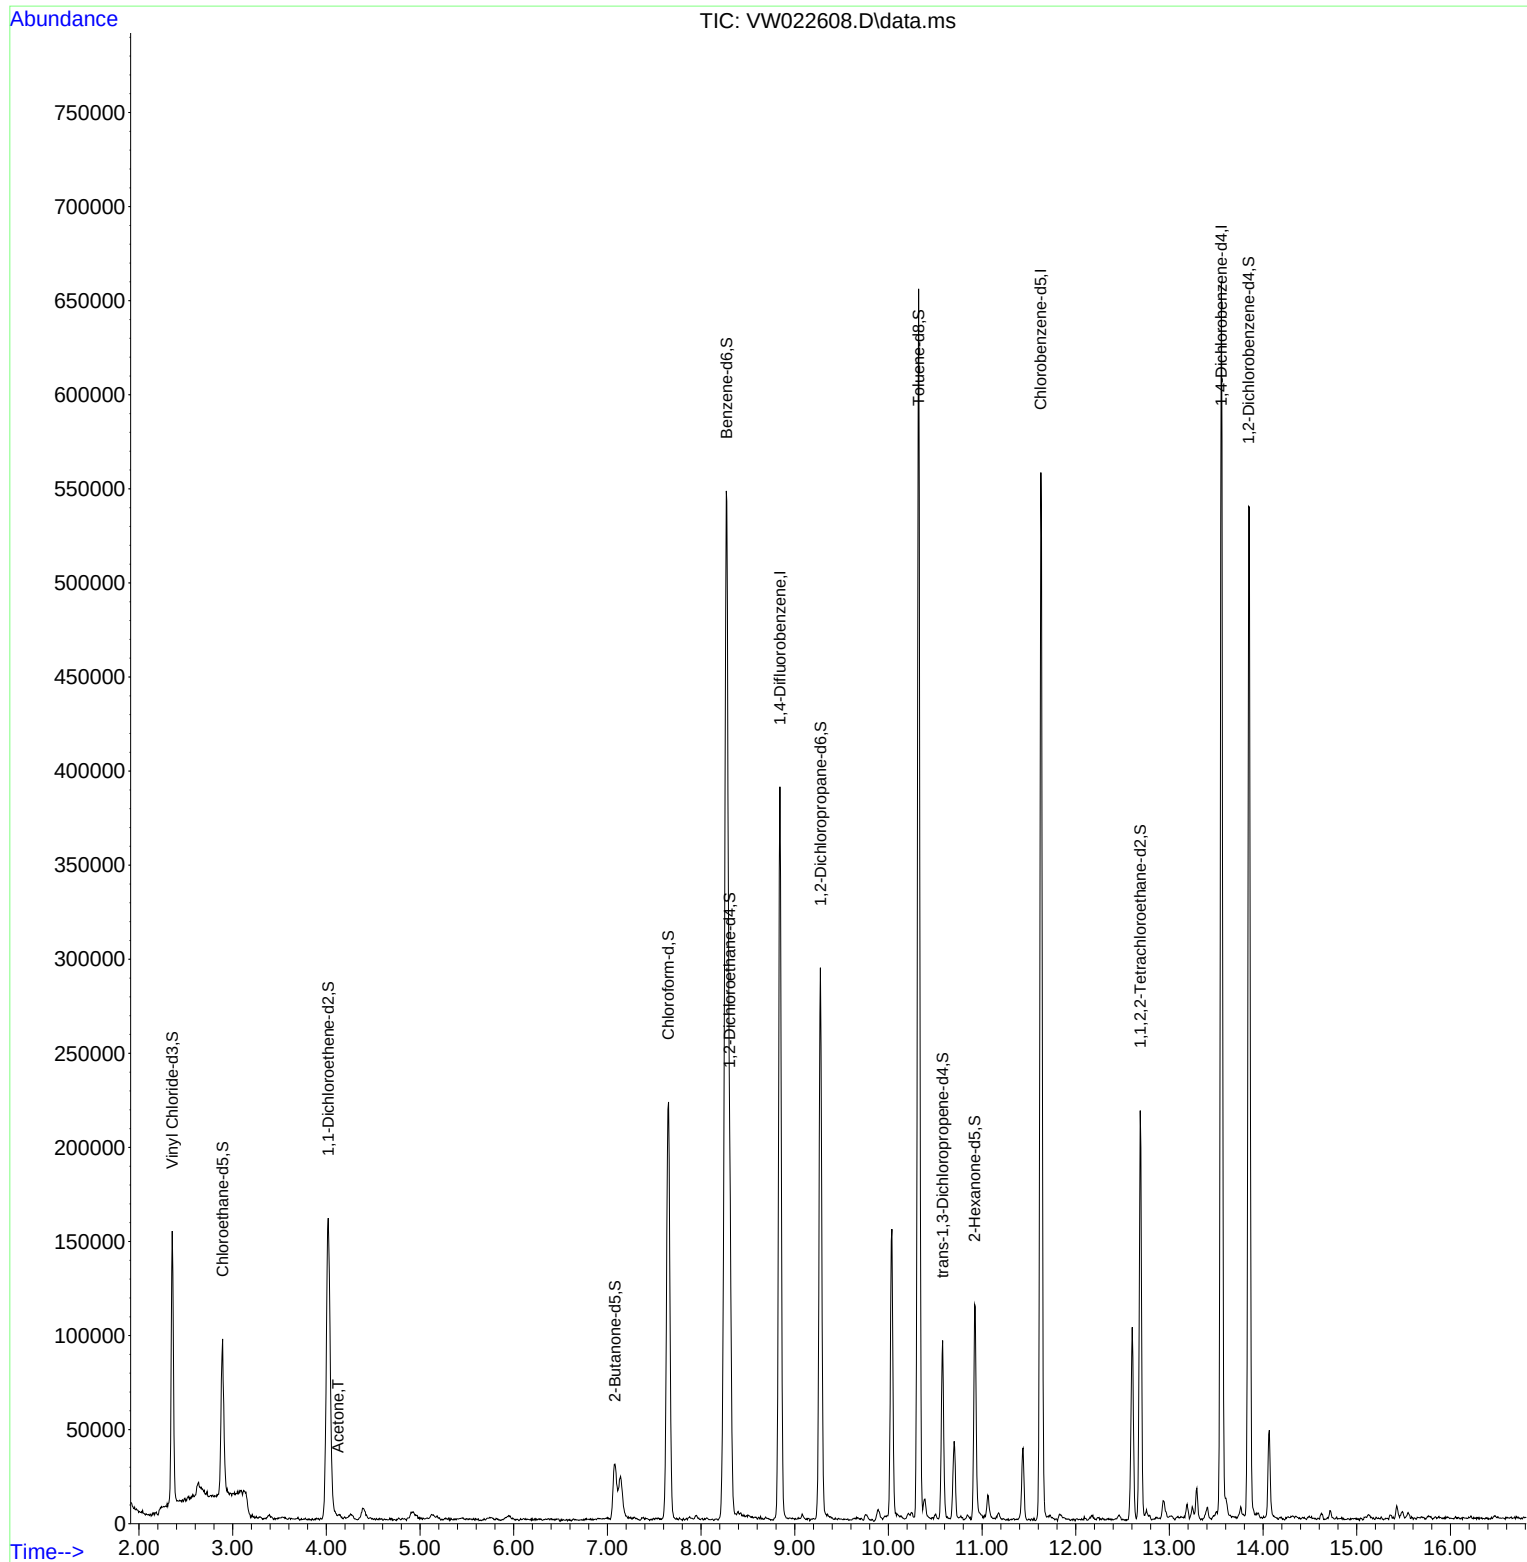

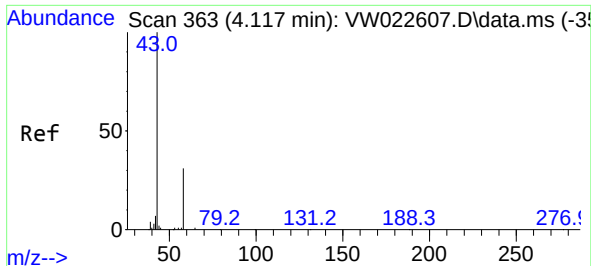

#13
 Acetone
 Concen: 4.433 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022608.D
 Acq: 25 Apr 2022 10:58

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK485

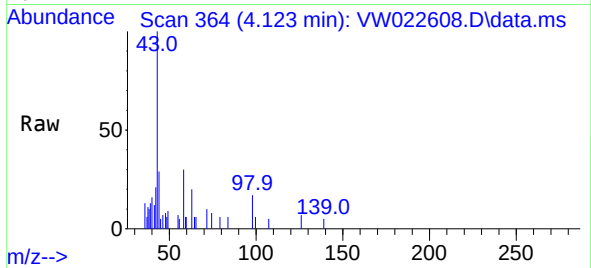

Tgt Ion: 43 Resp: 3754
 Ion Ratio Lower Upper
 43 100
 58 2.8 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

