

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022609.D
 Acq On : 25 Apr 2022 16:01
 Operator : SY/VA
 Sample : N2293-12
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/26/2022
 Supervised By : Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:35:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	327458	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	311059	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	161260	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	143541	19.829	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.320%		
7) Chloroethane-d5	2.891	69	93827m	20.681	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.720%		
11) 1,1-Dichloroethene-d2	4.019	63	168502	17.946	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.800%		
21) 2-Butanone-d5	7.074	46	51668	40.881	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.760%		
24) Chloroform-d	7.647	84	233014	22.766	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.080%		
26) 1,2-Dichloroethane-d4	8.305	65	126713	21.668	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.680%		
32) Benzene-d6	8.275	84	463984	24.414	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.640%		
36) 1,2-Dichloropropane-d6	9.274	67	129650	23.574	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.280%		
41) Toluene-d8	10.323	98	438654	23.567	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	94.280%		
43) trans-1,3-Dichloroprop...	10.573	79	52729	20.315	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.280%		
47) 2-Hexanone-d5	10.921	63	41167	40.232	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.460%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	99587	21.296	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.200%		
66) 1,2-Dichlorobenzene-d4	13.853	152	139086	24.350	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.400%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	3902	4.535	ug/L	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022609.D
Acq On : 25 Apr 2022 16:01
Operator : SY/VA
Sample : N2293-12
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Apr 26 01:35:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022

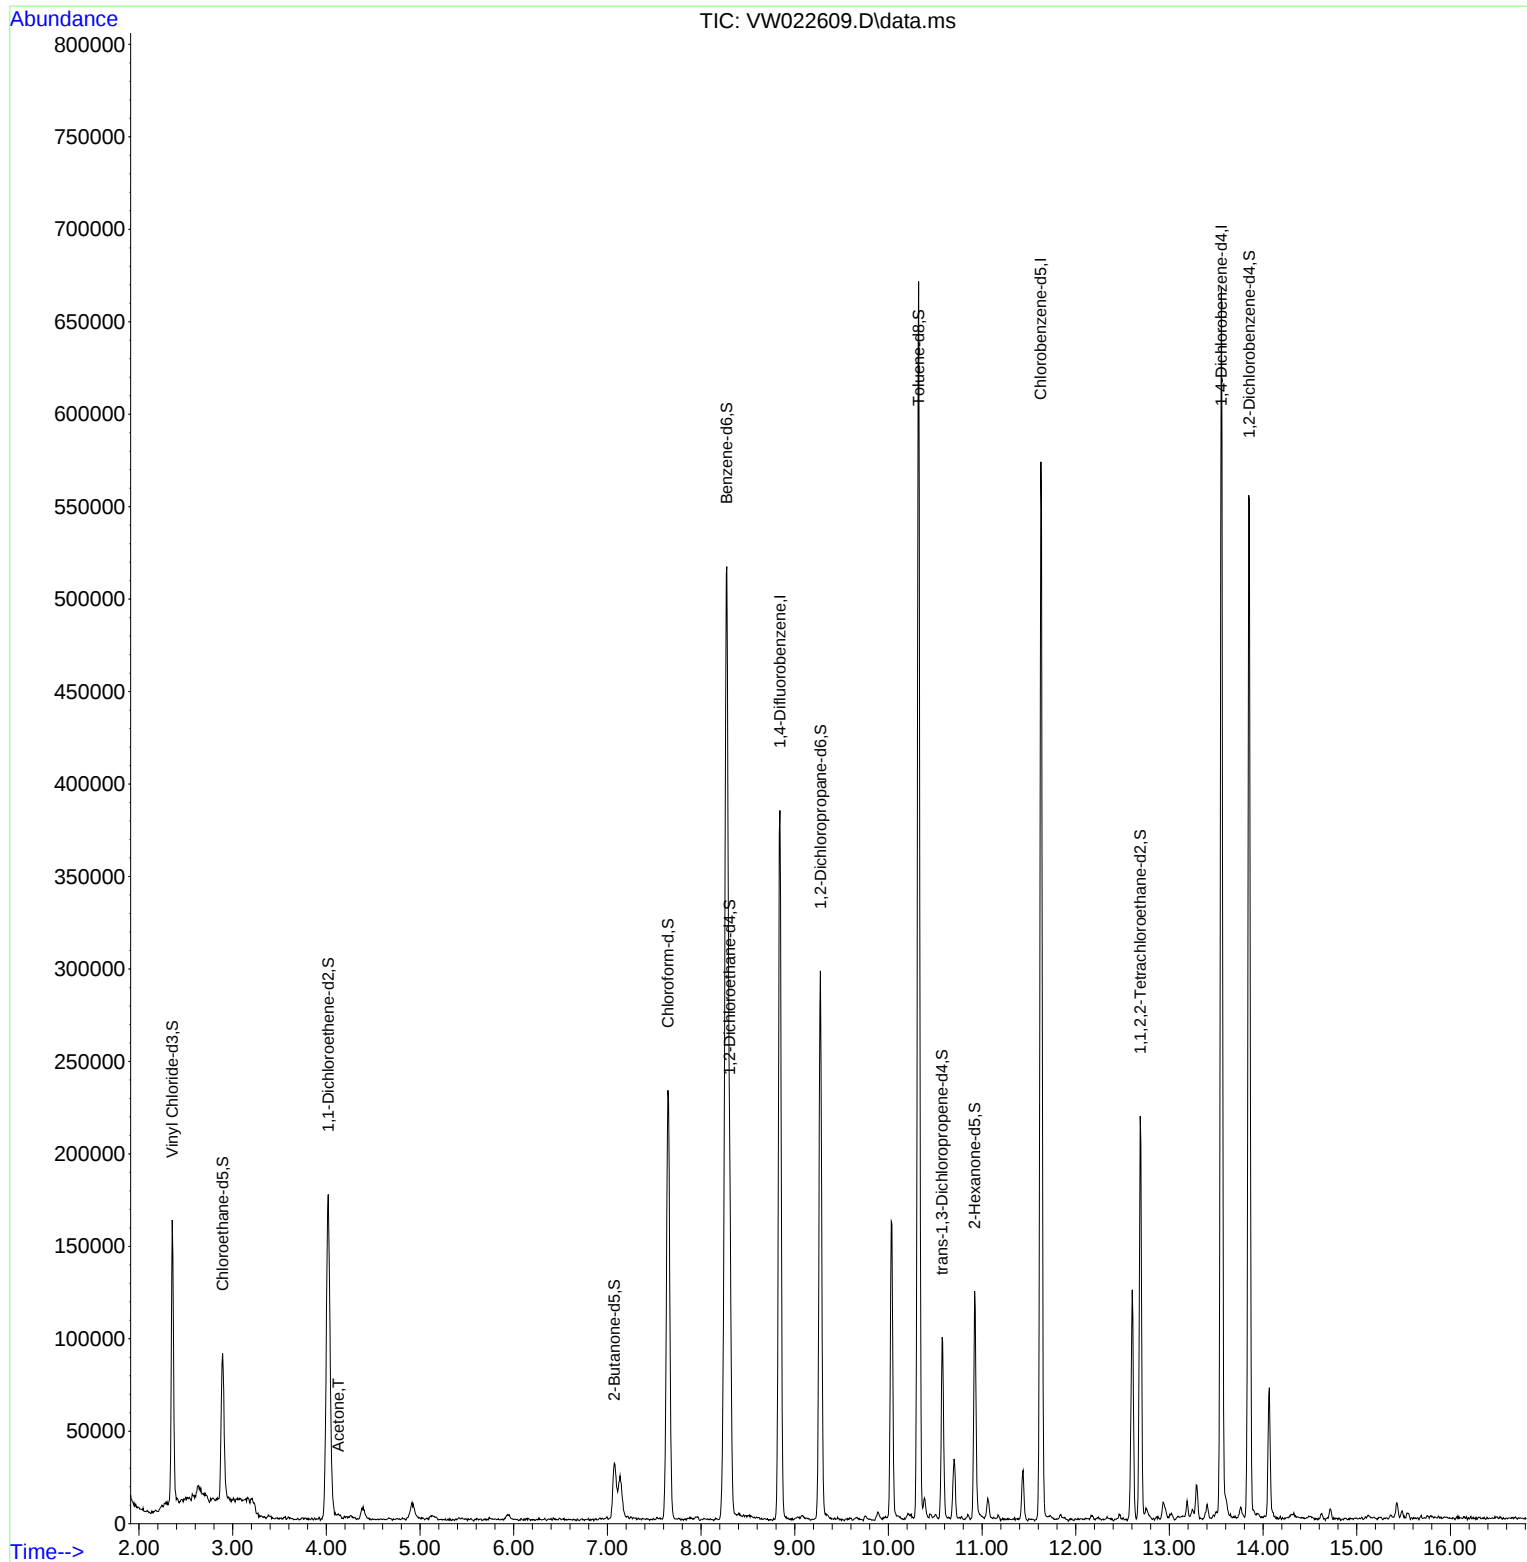

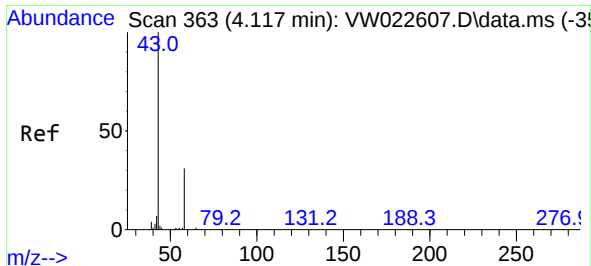

#13
Acetone
Concen: 4.535 ug/L
RT: 4.129 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW022609.D
Acq: 25 Apr 2022 16:01

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

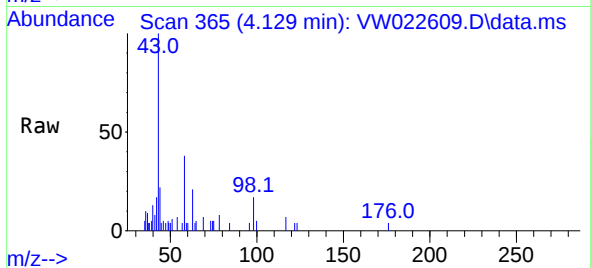

Tgt Ion: 43 Resp: 390
Ion Ratio Lower Upper
43 100
58 8.2 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022

