

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
 Data File : VW022611.D
 Acq On : 25 Apr 2022 16:59
 Operator : SY/VA
 Sample : N2316-15
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
 Supervised By :Mahesh Dadoda 04/26/2022

Quant Time: Apr 26 01:36:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 26 01:35:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	309662	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	301841	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	157945	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	142435	20.807	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.240%		
7) Chloroethane-d5	2.885	69	88626	20.657	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.640%		
11) 1,1-Dichloroethene-d2	4.019	63	157412	17.729	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	70.920%		
21) 2-Butanone-d5	7.080	46	56470	47.249	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.500%		
24) Chloroform-d	7.647	84	233351	24.109	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	96.440%		
26) 1,2-Dichloroethane-d4	8.305	65	131427	23.765	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.080%		
32) Benzene-d6	8.275	84	460913	24.994	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.960%		
36) 1,2-Dichloropropane-d6	9.274	67	131451	24.631	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.520%		
41) Toluene-d8	10.323	98	441556	24.448	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	97.800%		
43) trans-1,3-Dichloroprop...	10.579	79	53657	21.304	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.200%		
47) 2-Hexanone-d5	10.921	63	47377	47.715	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.440%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	112259	24.739	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.960%		
66) 1,2-Dichlorobenzene-d4	13.847	152	140955	25.196	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	100.800%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	3933m	4.833	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042522\
Data File : VW022611.D
Acq On : 25 Apr 2022 16:59
Operator : SY/VA
Sample : N2316-15
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Apr 26 01:36:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 26 01:35:04 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/26/2022
Supervised By : Mahesh Dadoda 04/26/2022

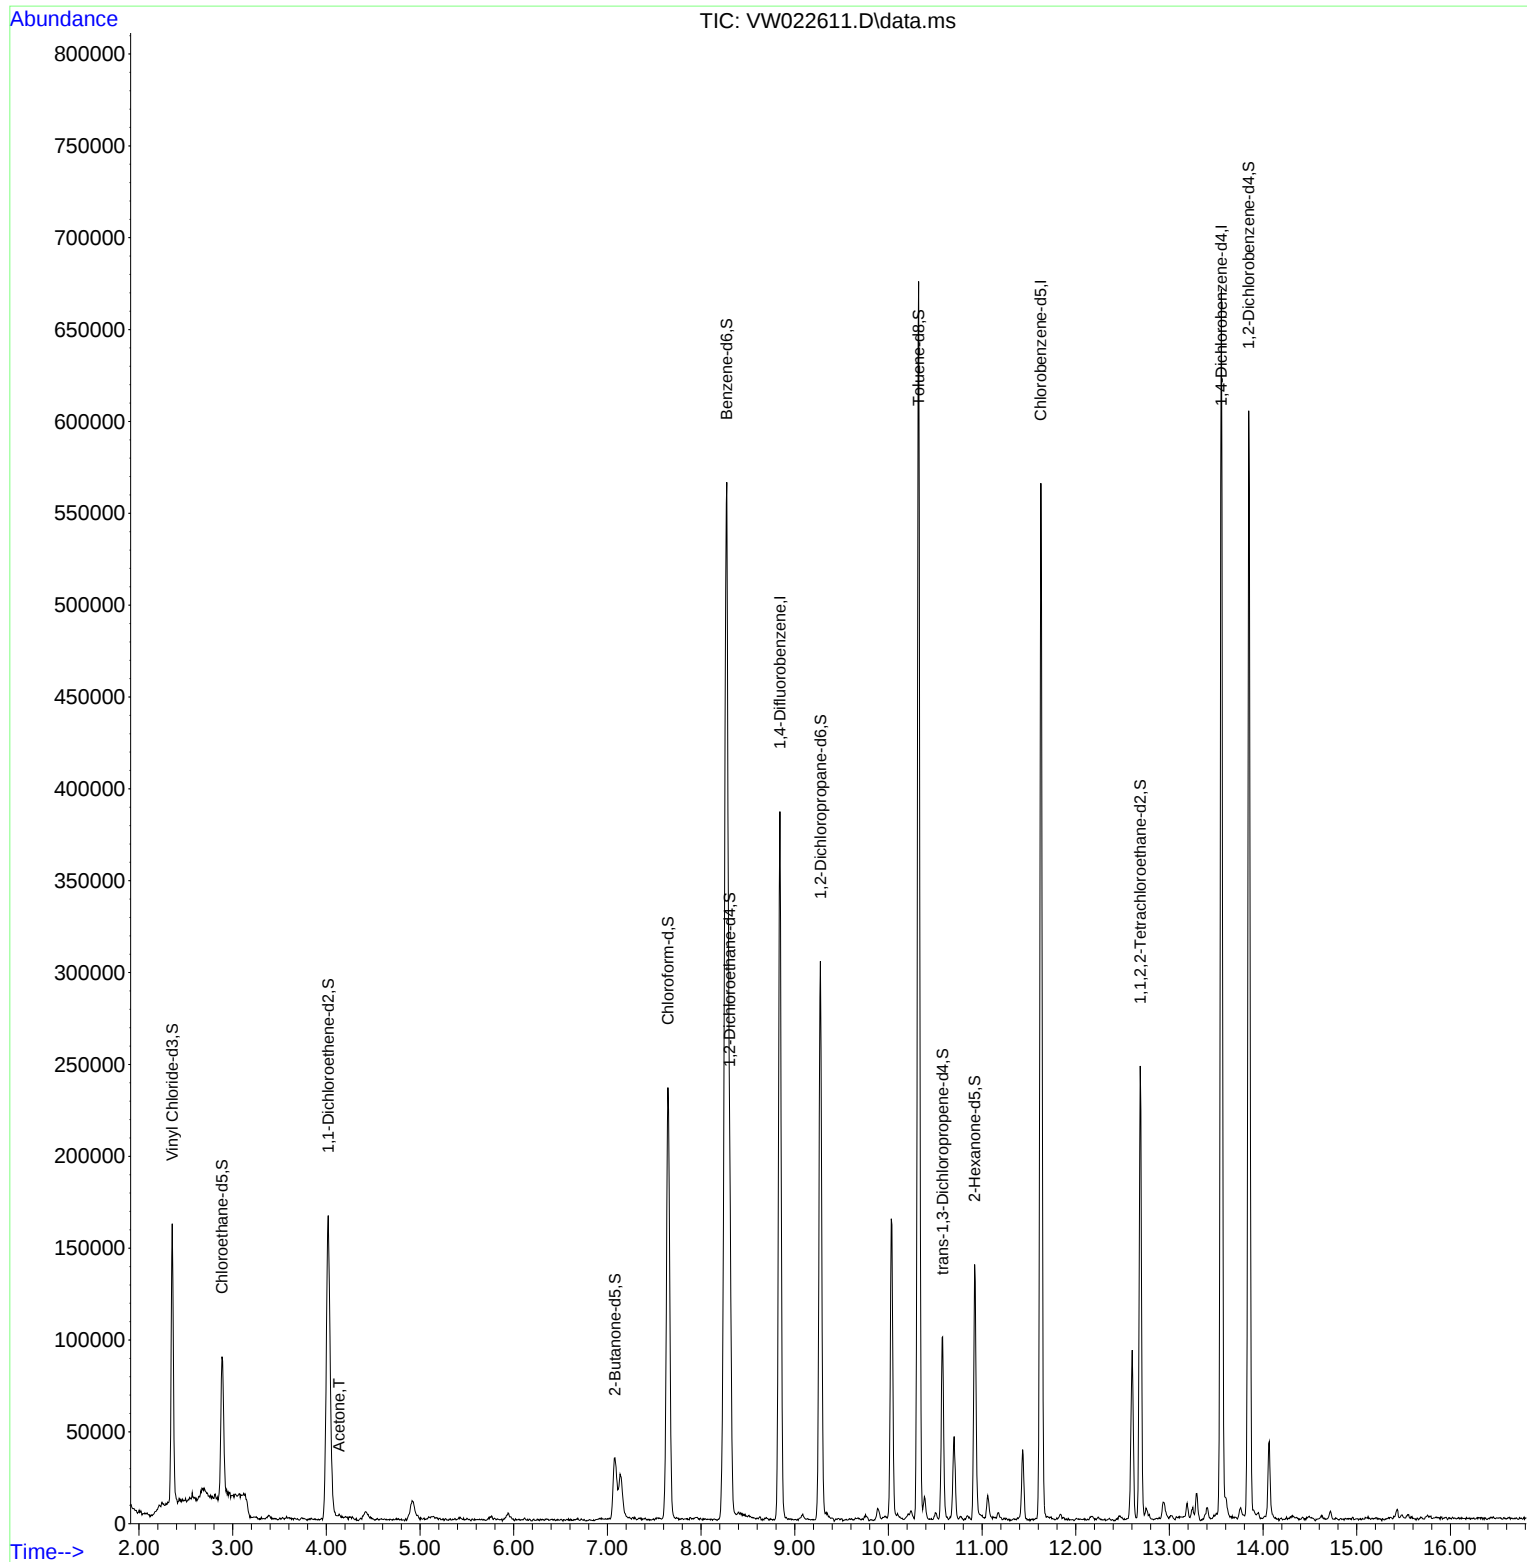

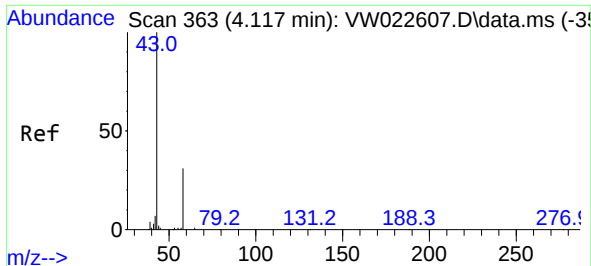

#13
Acetone
Concen: 4.833 ug/L m
RT: 4.135 min Scan# 30
Delta R.T. 0.018 min
Lab File: VW022611.D
Acq: 25 Apr 2022 16:59

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion: 43 Resp: 393
Ion Ratio Lower Upper
43 100
58 8.2 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/26/2022
Supervised By :Mahesh Dadoda 04/26/2022

