

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042524\
 Data File : VW028547.D
 Acq On : 25 Apr 2024 11:21
 Operator : SY/MD
 Sample : VW0425SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 26 01:10:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 26 01:10:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	311699	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	287057	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	132801	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	74795	14.968	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.880%
7) Chloroethane-d5	2.905	69	65147	17.201	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.800%
11) 1,1-Dichloroethene-d2	4.021	65	35103	16.588	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.360%
21) 2-Butanone-d5	7.081	46	41581	44.468	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.940%
24) Chloroform-d	7.648	84	164772	20.258	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.040%
26) 1,2-Dichloroethane-d4	8.307	65	89890	21.266	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.080%
32) Benzene-d6	8.276	84	312736	19.943	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.760%
36) 1,2-Dichloropropane-d6	9.270	67	97485	20.914	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.640%
41) Toluene-d8	10.325	98	272891	19.137	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.560%
43) trans-1,3-Dichloroprop...	10.575	79	35060	18.916	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.680%
47) 2-Hexanone-d5	10.922	63	27371	42.391	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.780%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	73679	22.403	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	91249	21.727	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3315	0.483	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042524\
Data File : VW028547.D
Acq On : 25 Apr 2024 11:21
Operator : SY/MD
Sample : VW0425SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 26 01:10:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 26 01:10:19 2024
Response via : Initial Calibration

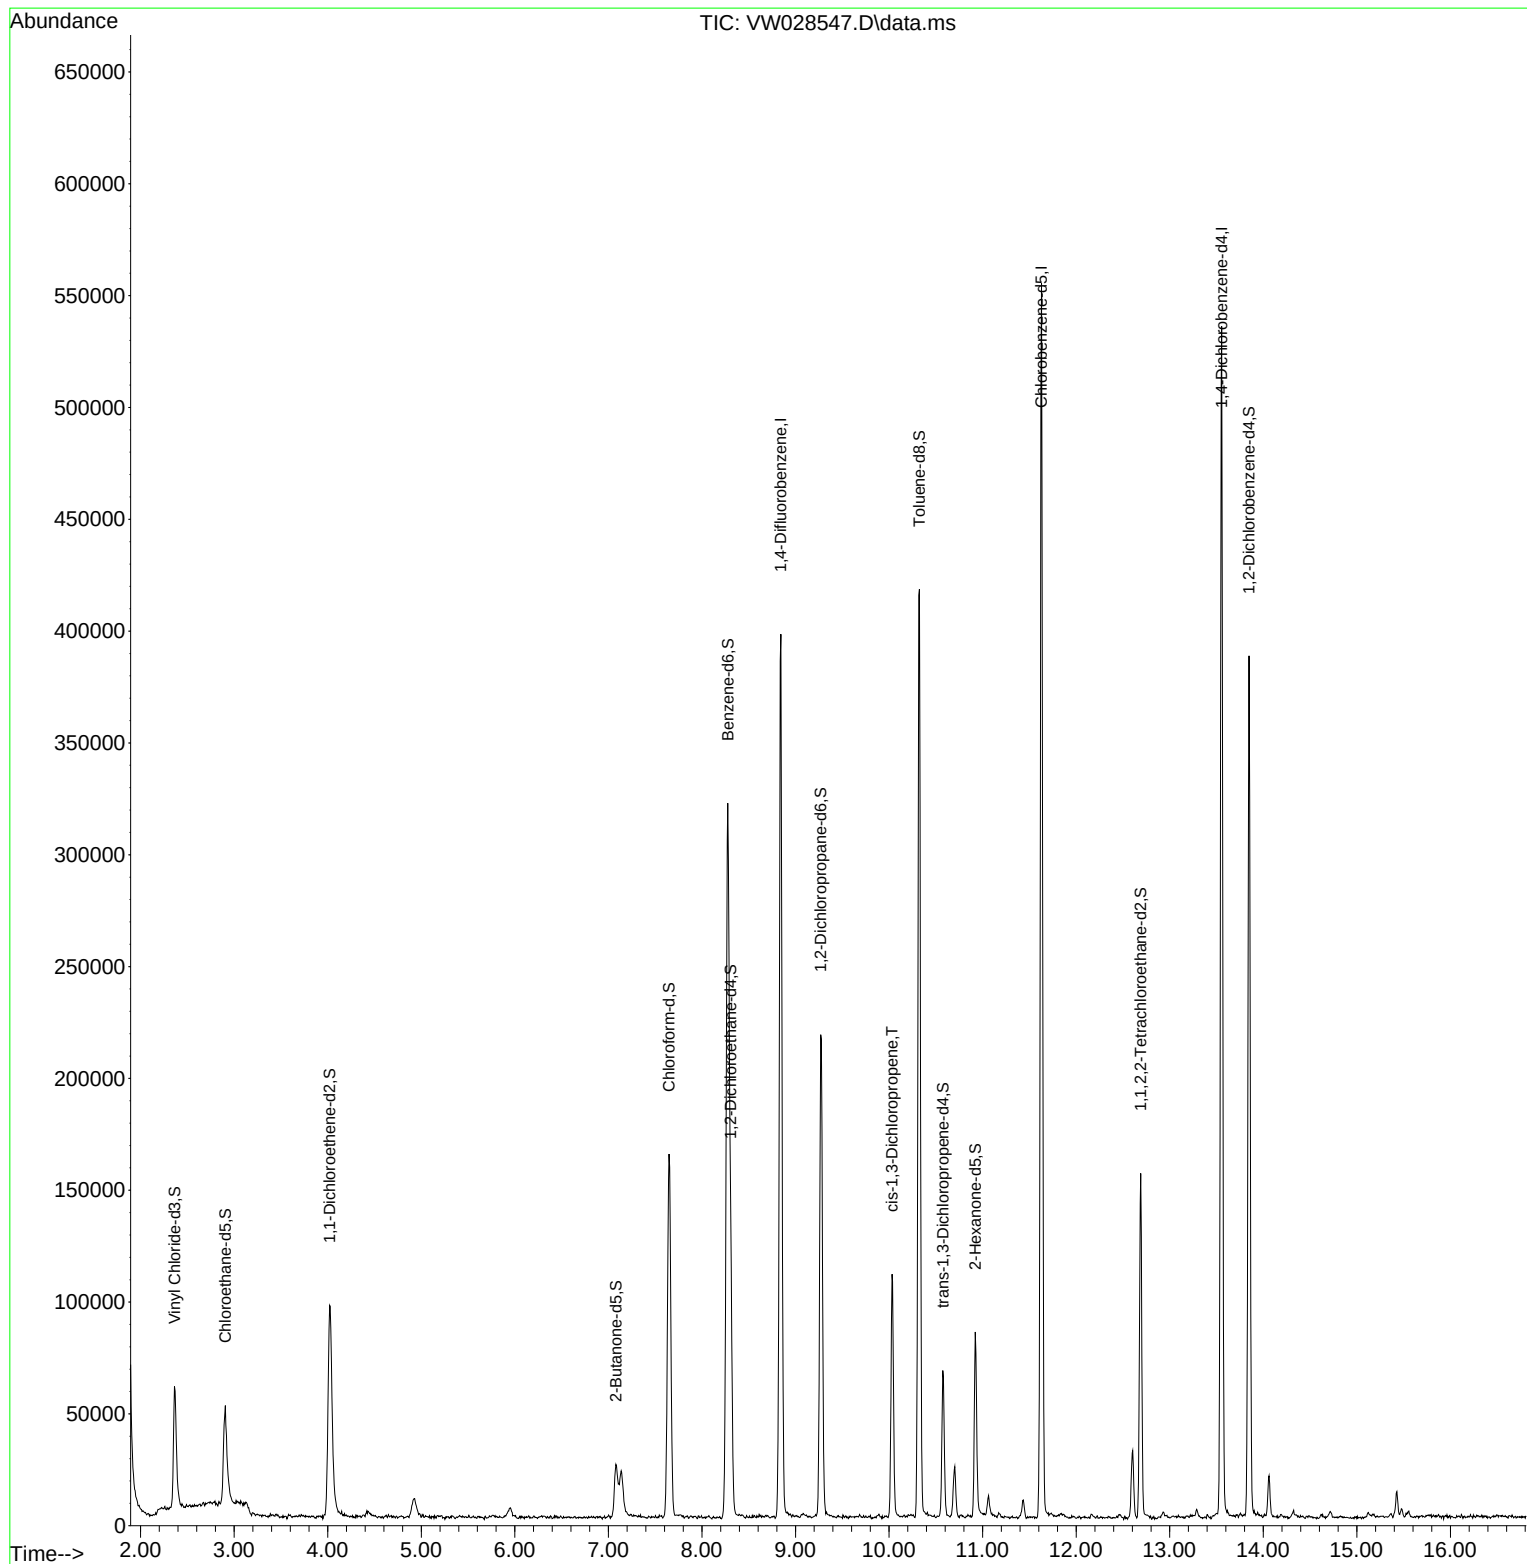

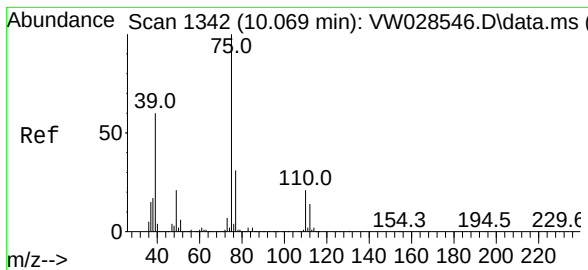

#39
 cis-1,3-Dichloropropene
 Concen: 0.483 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW028547.D
 Acq: 25 Apr 2024 11:21

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3315
 Ion Ratio Lower Upper
 75 100
 77 50.6 21.3 39.5#

