


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042720\
 Data File : VW015347.D
 Acq On : 27 Apr 2020 08:35
 Operator : SY/VA
 Sample : BFB01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB24

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042720S.M
 Title : VOC Analysis
 Last Update : Mon Apr 27 09:28:28 2020

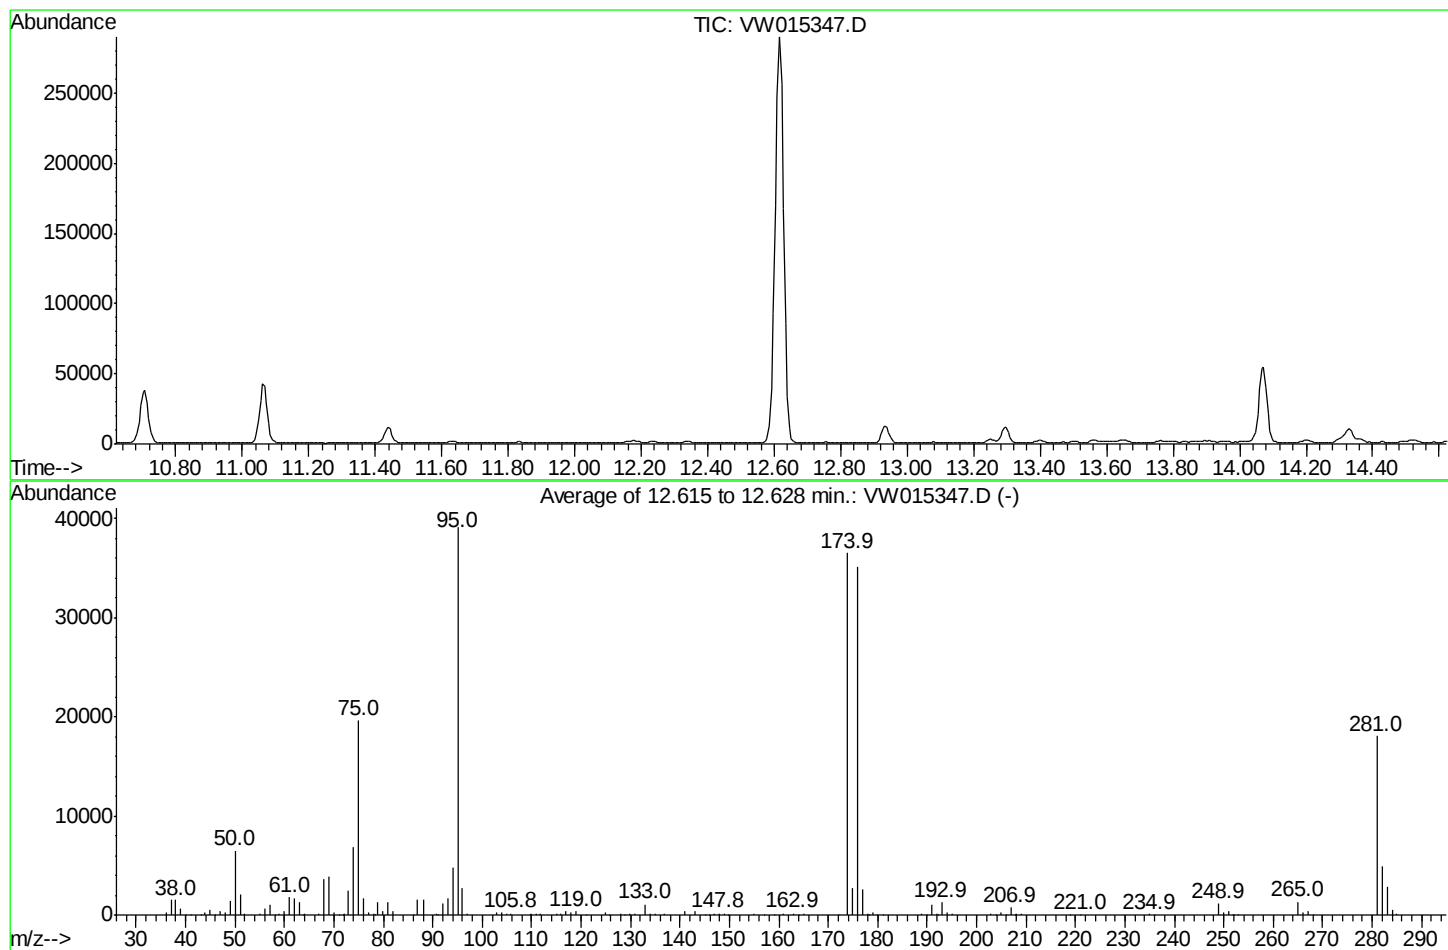

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	6492	PASS
75	95	30	80	50.1	19600	PASS
95	95	100	100	100.0	39125	PASS
96	95	5	9	7.1	2759	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	93.4	36533	PASS
175	174	5	9	7.6	2760	PASS
176	174	95	101	96.3	35186	PASS
177	176	5	9	7.4	2620	PASS

m/z	Abundance
36.00	417.0
37.00	1893.0
38.00	1819.0
39.00	758.0
40.00	147.0
41.00	152.0
43.00	154.0
44.00	470.0
45.00	610.0
46.00	59.0
47.00	529.0
48.00	304.0
49.00	1708.0
50.00	8025.0
51.00	2368.0
51.90	156.0
55.00	183.0
56.00	712.0
57.00	1372.0
58.10	72.0
59.00	278.0
60.00	408.0
61.00	2159.0
62.00	2076.0
63.00	1586.0
63.80	150.0
67.10	191.0
68.00	4257.0
69.00	4643.0
69.90	375.0
71.00	78.0
71.80	163.0
72.10	180.0
73.00	3204.0
74.00	8083.0
75.00	23144.0
76.00	2091.0
77.00	251.0
78.00	172.0
78.90	1438.0
79.90	473.0
80.90	1426.0
81.90	413.0
85.90	57.0
87.00	1755.0
88.00	1798.0
90.80	183.0
92.00	1341.0
93.00	1817.0
94.00	5558.0
95.00	43248.0
96.00	3282.0
96.90	153.0
102.90	331.0
103.90	365.0
104.80	161.0
105.90	200.0
109.70	106.0
110.10	119.0
110.90	126.0
111.80	132.0
115.10	154.0
115.90	182.0
116.90	446.0
117.90	326.0
119.00	555.0
121.00	79.0
125.00	505.0
127.90	160.0
128.90	110.0
129.90	144.0
130.80	101.0
133.00	1871.0
133.80	328.0
134.90	190.0
136.80	102.0
140.90	473.0
142.90	440.0
145.10	63.0
145.80	82.0
146.90	235.0
147.90	172.0
148.90	146.0
149.80	57.0
154.80	110.0
157.00	78.0
159.00	74.0
161.00	130.0
162.90	270.0
164.00	55.0
165.00	207.0
173.90	38992.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24

174.90	2988.0
175.90	37656.0
176.90	2951.0
177.90	175.0
178.90	462.0
179.80	56.0
181.00	62.0
188.90	204.0
189.90	58.0
190.90	1725.0
191.90	478.0
192.90	2052.0
194.00	365.0
195.00	216.0
202.90	115.0
203.90	59.0
205.00	387.0
206.00	76.0
207.00	1260.0
208.10	299.0
209.00	212.0
219.00	66.0
221.00	108.0
234.90	249.0
236.00	71.0
249.00	1897.0
250.00	529.0
251.00	677.0
251.80	182.0
252.90	116.0
265.00	2259.0
266.00	475.0
267.00	438.0
268.10	107.0
281.00	29592.0
282.00	8601.0
283.00	4759.0
284.10	913.0
285.00	302.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24

m/z	Abundance
36.00	294.0
37.00	1644.0
38.00	1661.0
39.00	704.0
40.10	118.0
41.10	126.0
43.00	118.0
44.00	455.0
45.00	521.0
45.90	52.0
47.10	313.0
47.90	212.0
49.00	1570.0
50.00	6969.0
51.00	2341.0
52.00	107.0
54.90	235.0
56.00	631.0
57.00	1104.0
58.90	149.0
60.00	382.0
61.00	2002.0
62.00	1880.0
63.10	1354.0
64.00	201.0
66.90	140.0
68.00	3917.0
69.00	4294.0
70.00	315.0
71.10	64.0
72.00	197.0
73.00	2796.0
74.00	7586.0
75.00	21096.0
76.00	1725.0
77.00	230.0
78.20	156.0
78.90	1389.0
79.90	379.0
80.90	1556.0
81.90	354.0
86.00	55.0
86.90	1483.0
88.00	1645.0
90.80	177.0
92.00	1267.0
93.00	1800.0
94.00	5244.0
95.00	44048.0
96.00	3004.0
97.00	207.0
103.00	178.0
103.70	210.0
104.90	94.0
105.80	209.0
109.90	73.0
111.00	103.0
111.70	97.0
115.00	160.0
115.90	221.0
116.90	353.0
117.90	199.0
119.00	349.0
121.00	57.0
125.00	265.0
125.70	80.0
127.90	85.0
128.90	99.0
129.90	230.0
130.90	69.0
133.00	1000.0
133.90	220.0
134.90	175.0
136.90	113.0
140.90	394.0
142.90	453.0
146.90	113.0
147.70	121.0
148.90	89.0
154.80	133.0
159.10	63.0
160.90	110.0
162.80	127.0
163.00	122.0
164.90	123.0
172.10	75.0
173.90	40480.0
174.90	2897.0
175.90	39680.0
176.90	2816.0
177.90	136.0
178.90	229.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24

189.00	86.0
190.90	920.0
192.10	183.0
193.00	1286.0
193.90	191.0
194.90	168.0
202.90	112.0
205.00	264.0
206.10	86.0
207.00	741.0
208.10	151.0
208.90	88.0
235.00	124.0
248.90	1086.0
250.00	264.0
250.90	440.0
252.10	105.0
265.00	1260.0
266.00	341.0
267.00	337.0
268.00	77.0
281.00	17216.0
282.00	4432.0
283.00	2558.0
284.00	579.0
285.00	173.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24

m/z	Abundance
36.00	260.0
37.00	1061.0
38.00	1148.0
39.00	423.0
40.00	68.0
41.00	117.0
43.00	112.0
43.90	255.0
45.10	248.0
47.10	193.0
47.90	136.0
49.00	1141.0
50.00	4484.0
51.00	1405.0
51.90	68.0
54.90	150.0
56.00	427.0
57.00	695.0
58.90	54.0
59.90	227.0
61.00	1259.0
62.00	1216.0
63.00	1074.0
64.00	94.0
66.90	124.0
68.00	2851.0
69.00	2923.0
69.90	289.0
72.00	163.0
73.00	1418.0
74.00	4794.0
75.00	14561.0
76.00	1209.0
76.80	309.0
77.90	94.0
78.90	957.0
80.00	235.0
80.90	1054.0
81.90	227.0
87.00	1232.0
88.00	1185.0
91.00	165.0
92.00	879.0
93.00	1321.0
94.00	3420.0
95.00	30080.0
96.00	1993.0
97.00	69.0
103.00	94.0
103.90	172.0
104.90	137.0
105.90	166.0
110.00	55.0
114.90	93.0
115.90	140.0
117.00	247.0
117.80	94.0
118.90	252.0
124.80	103.0
127.90	92.0
129.90	104.0
130.80	57.0
132.80	259.0
134.80	78.0
136.90	72.0
141.00	240.0
142.90	328.0
146.90	64.0
147.90	121.0
154.80	73.0
159.00	67.0
160.90	77.0
162.80	68.0
169.00	51.0
173.90	30128.0
174.90	2397.0
175.90	28224.0
177.00	2095.0
178.10	70.0
190.90	364.0
191.80	62.0
192.90	402.0
193.90	67.0
195.10	55.0
202.80	73.0
205.00	122.0
207.00	356.0
207.80	62.0
248.90	439.0
250.00	115.0
250.90	148.0
265.00	500.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24

266.10	97.0
266.90	113.0
267.10	114.0
281.10	7382.0
282.00	1786.0
283.00	1251.0
284.00	232.0
285.00	107.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24

Scan 1749 (12.567 min): VW015347.D
BFB24

m/z	Abundance
40.00	88.0
41.00	112.0
43.00	82.0
43.90	182.0
55.10	99.0
69.10	86.0
72.80	57.0
168.90	51.0
206.80	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB24