

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042721\
 Data File : VW018799.D
 Acq On : 27 Apr 2021 13:23
 Operator : SY/VA
 Sample : VIBLK125
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK125

Manual Integrations
 APPROVED

MMDadoda

4/29/2021 10:03:33 AM

Quant Time: Apr 28 00:42:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 28 00:41:12 2021
 Response via : Initial Calibration

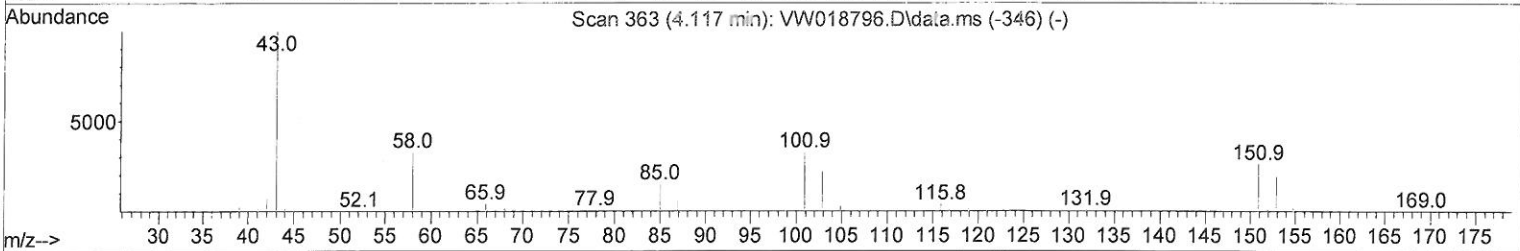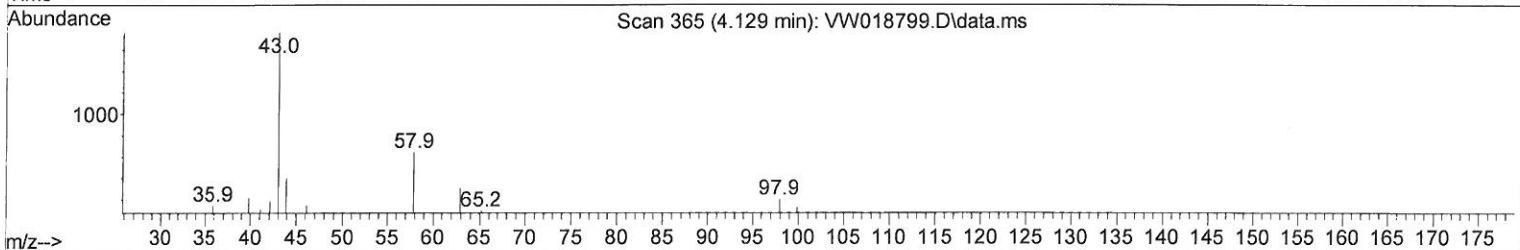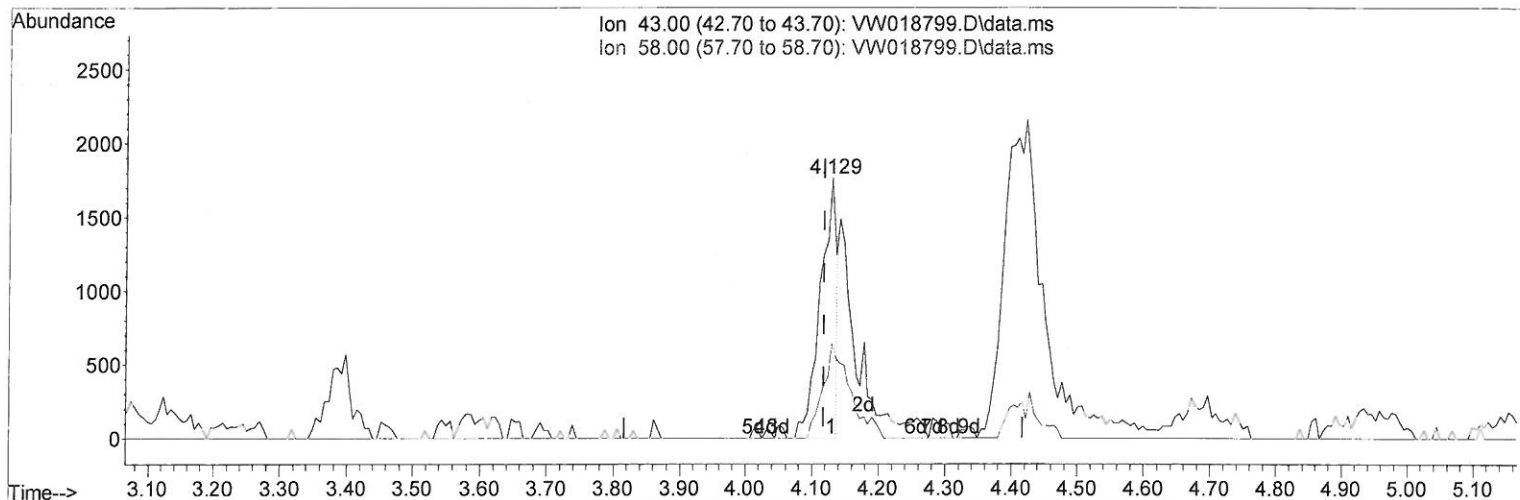

TIC: VW018799.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 2.17 ug/L

response 2921

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	58.78#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042721\
 Data File : VW018799.D
 Acq On : 27 Apr 2021 13:23
 Operator : SY/VA
 Sample : VIBLK125
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK125

Manual Integrations
 APPROVED

MMDadoda

4/29/2021 10:03:33 AM

Quant Time: Apr 28 00:42:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 28 00:41:12 2021
 Response via : Initial Calibration

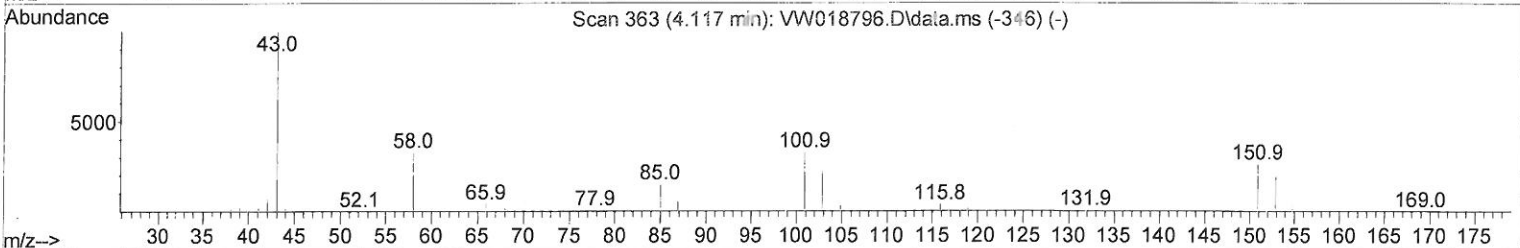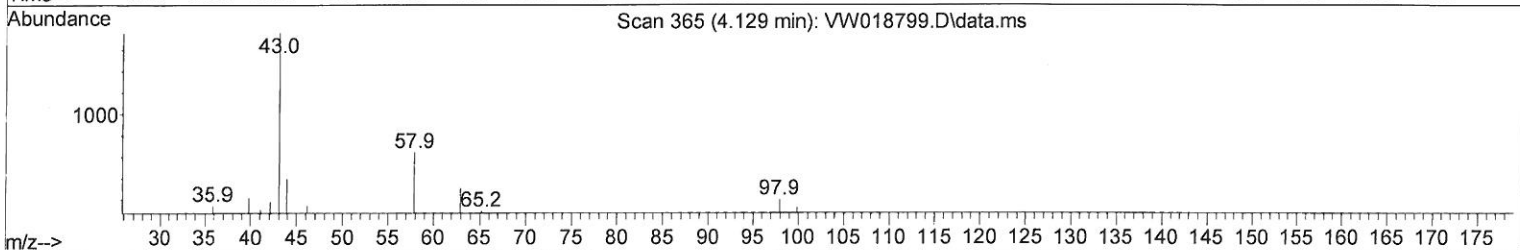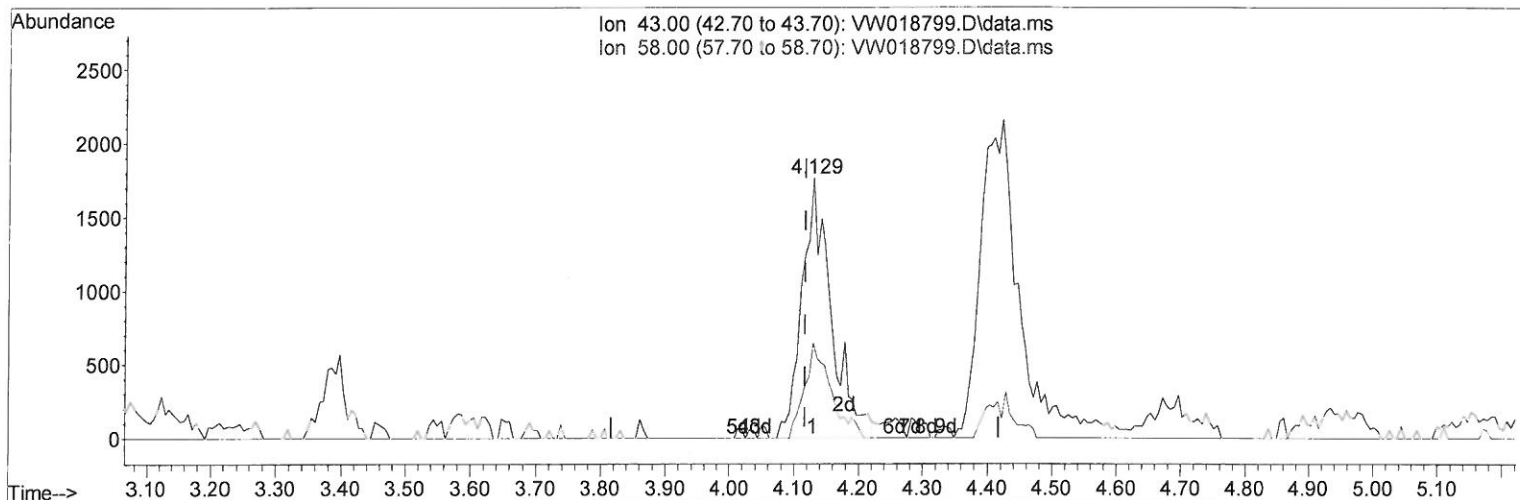

TIC: VW018799.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 4.12 ug/L m

response 5542

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	30.98
0.00	0.00	0.00
0.00	0.00	0.00

204/30/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042721\
 Data File : VW018799.D
 Acq On : 27 Apr 2021 13:23
 Operator : SY/VA
 Sample : VIBLK125
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK125

Manual Integrations
 APPROVED

MMDadoda

4/29/2021 10:03:33 AM

Quant Time: Apr 28 00:42:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 28 00:41:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	535113	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	485528	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	232202	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	113085	13.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.64%
7) Chloroethane-d5	2.891	69	101647	14.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.40%
11) 1,1-Dichloroethene-d2	4.019	63	179156	12.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.76%
21) 2-Butanone-d5	7.074	46	82617	44.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.26%
24) Chloroform-d	7.647	84	301678	20.54	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.16%
26) 1,2-Dichloroethane-d4	8.305	65	177159	21.46	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.84%
32) Benzene-d6	8.275	84	584361	20.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.08%
36) 1,2-Dichloropropane-d6	9.274	67	182598	21.27	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.08%
41) Toluene-d8	10.323	98	515698	19.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.20%
43) trans-1,3-Dichloroprop...	10.579	79	74857	20.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.96%
47) 2-Hexanone-d5	10.927	63	69845	46.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.60%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	155991	21.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.04%
66) 1,2-Dichlorobenzene-d4	13.853	152	179472	22.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.00%
Target Compounds						
13) Acetone	4.129	43	5542m	4.12	ug/L	Qvalue 86
16) Methylene chloride	4.909	84	14311	1.63	ug/L	86
42) Toluene	10.390	91	11606	0.35	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042721\
Data File : VW018799.D
Acq On : 27 Apr 2021 13:23
Operator : SY/VA
Sample : VIBLK125
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK125

Manual Integrations
APPROVED

MMDadoda

4/29/2021 10:03:33 AM

Quant Time: Apr 28 00:42:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM041421SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 28 00:41:12 2021
Response via : Initial Calibration

