




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022645.D
 Acq On : 27 Apr 2022 16:20
 Operator : SY/VA
 Sample : N2562-14
 Misc : 6.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW475

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

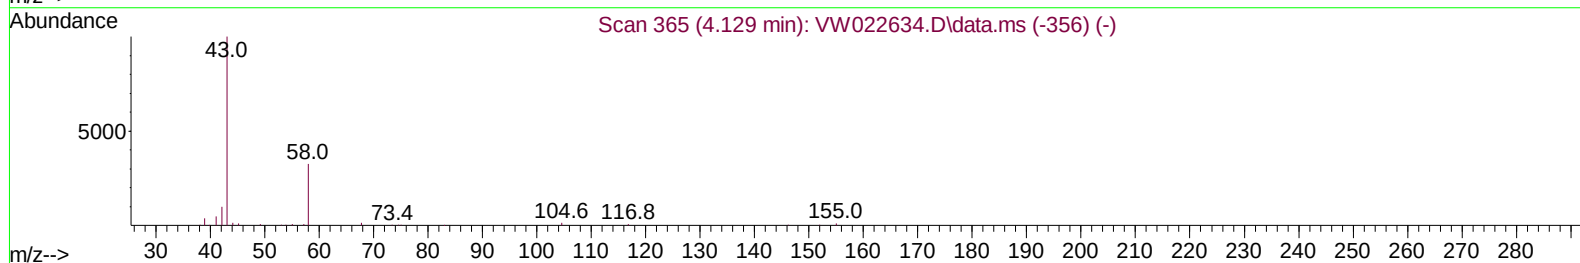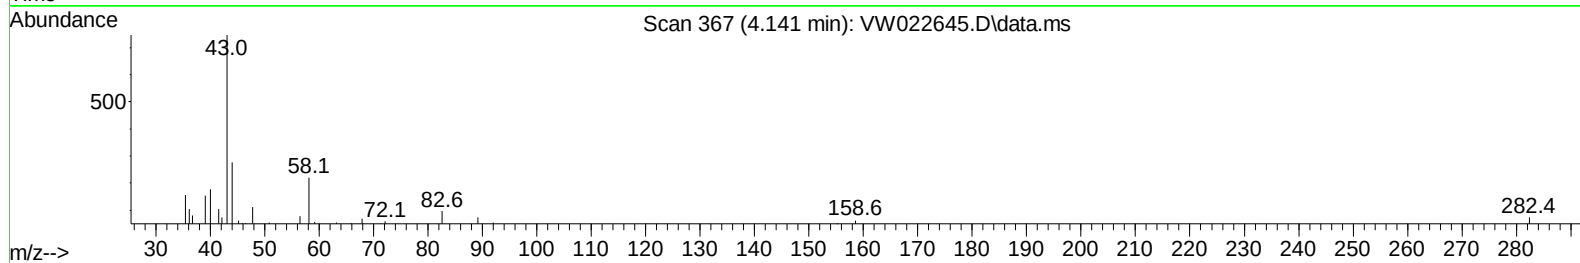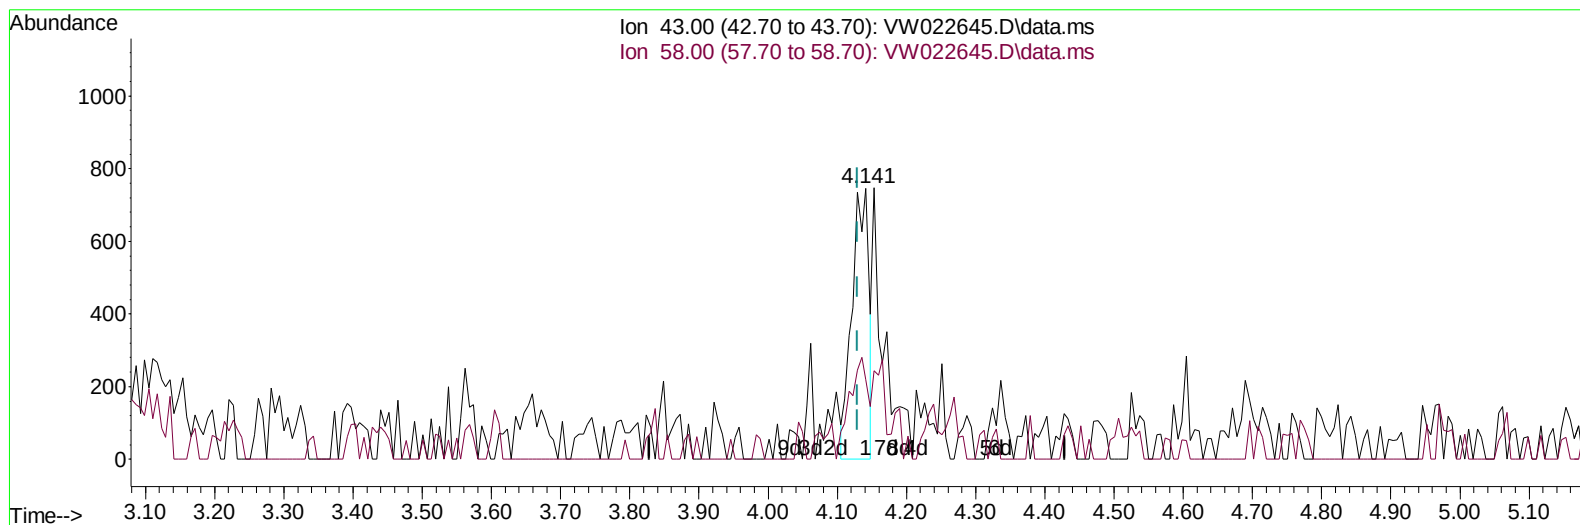

TIC: VW022645.D\data.ms

(13) Acetone (T)

4.141min (+ 0.012) 4.73 ug/L

response 1255

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	41.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022645.D
 Acq On : 27 Apr 2022 16:20
 Operator : SY/VA
 Sample : N2562-14
 Misc : 6.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW475

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

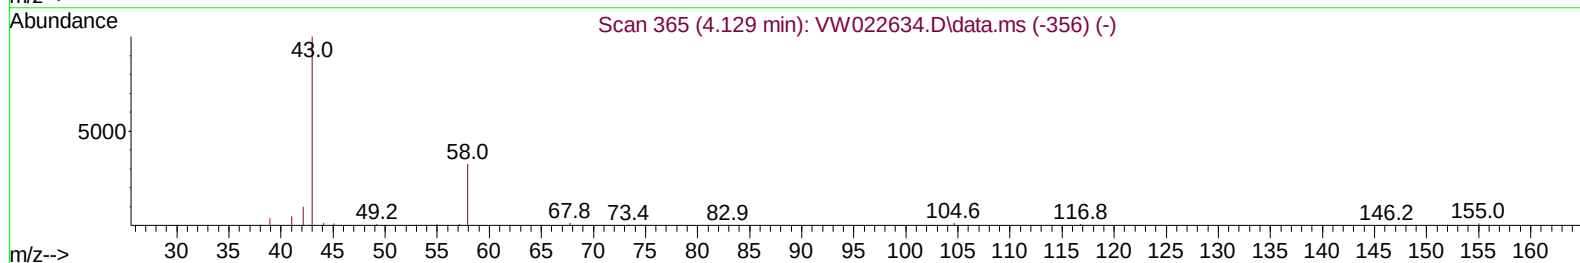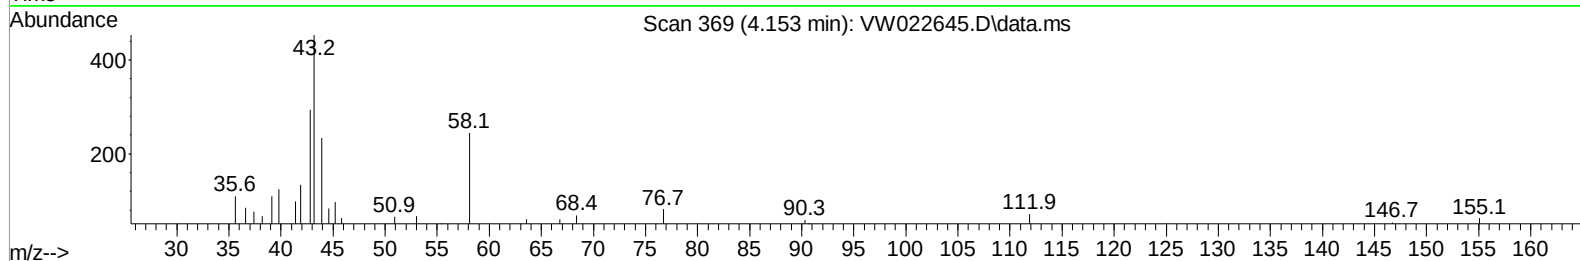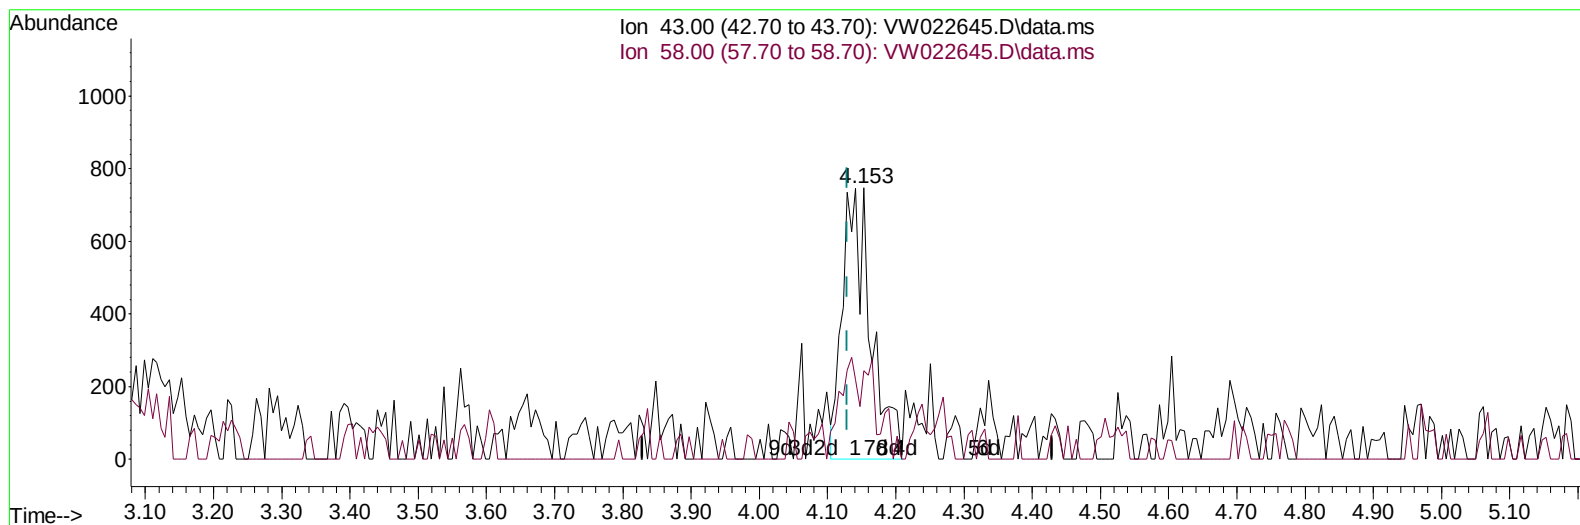

TIC: VW022645.D\data.ms

(13) Acetone (T)

4.153min (+ 0.024) 8.01 ug/L m

response 2127

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	24.59
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
Data File : VW022645.D
Acq On : 27 Apr 2022 16:20
Operator : SY/VA
Sample : N2562-14
Misc : 6.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW475

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/28/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 28 01:13:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 28 01:10:03 2022
Response via : Initial Calibration

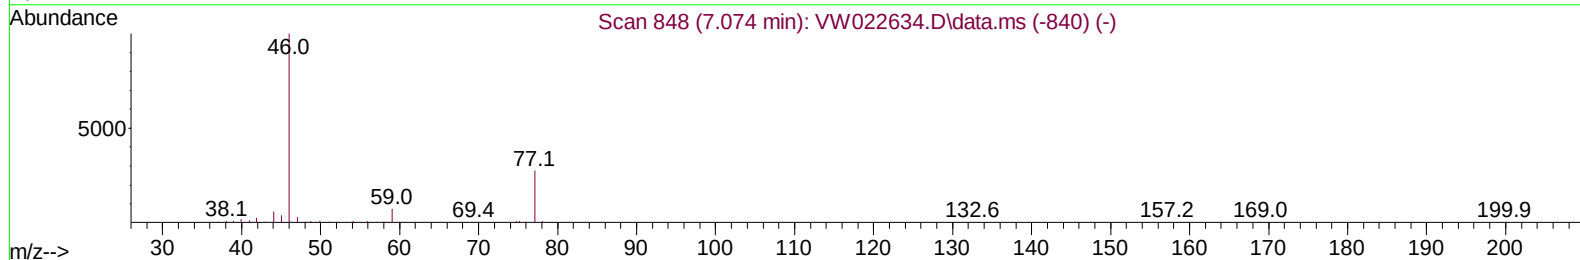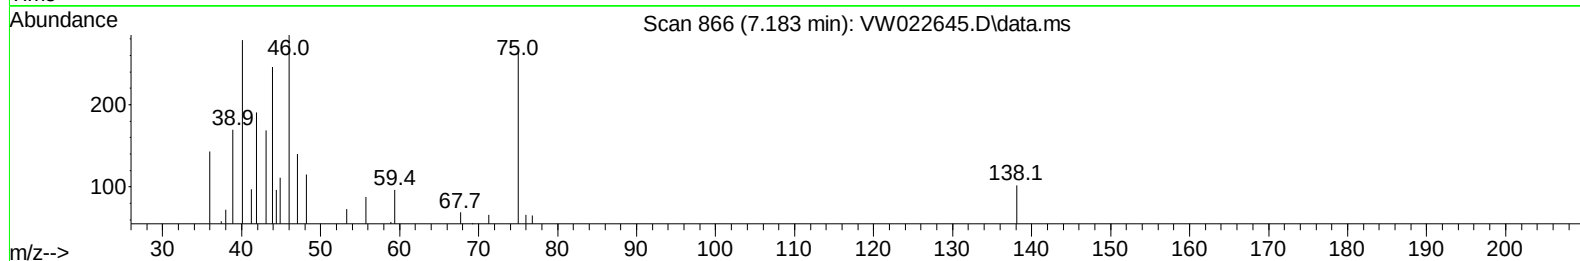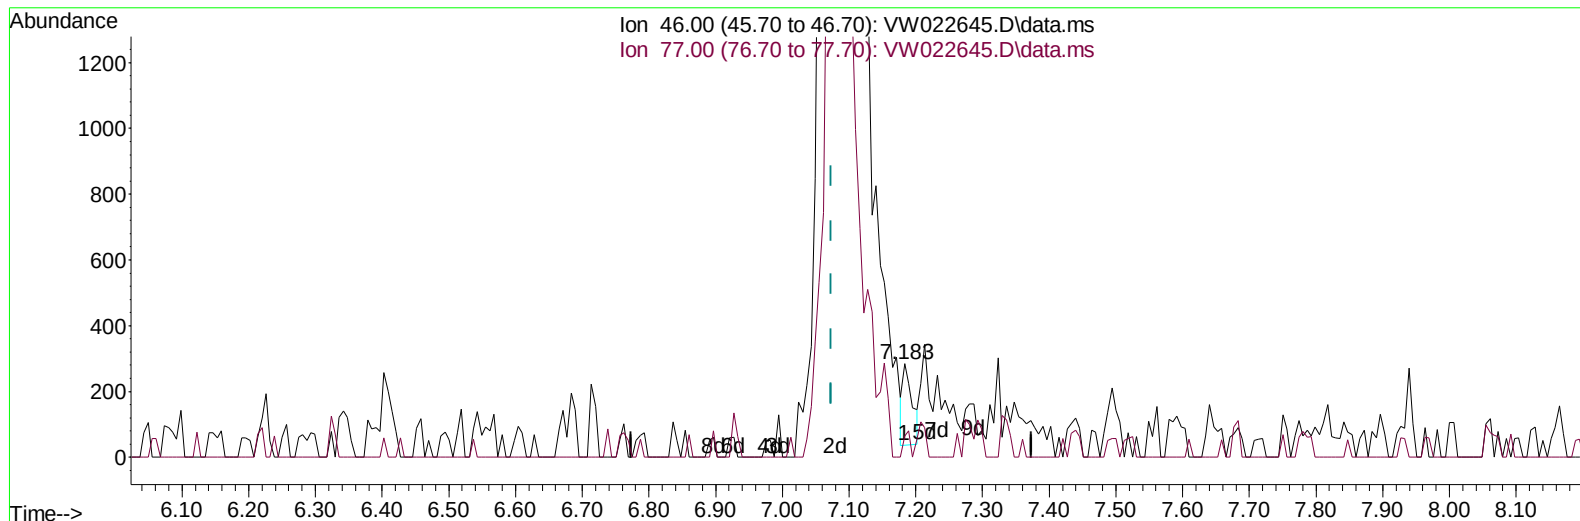

TIC: VW022645.D\data.ms

(21) 2-Butanone-d5 (S)

7.183min (+ 0.110) 0.61 ug/L

response 238

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	22.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022645.D
 Acq On : 27 Apr 2022 16:20
 Operator : SY/VA
 Sample : N2562-14
 Misc : 6.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW475

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

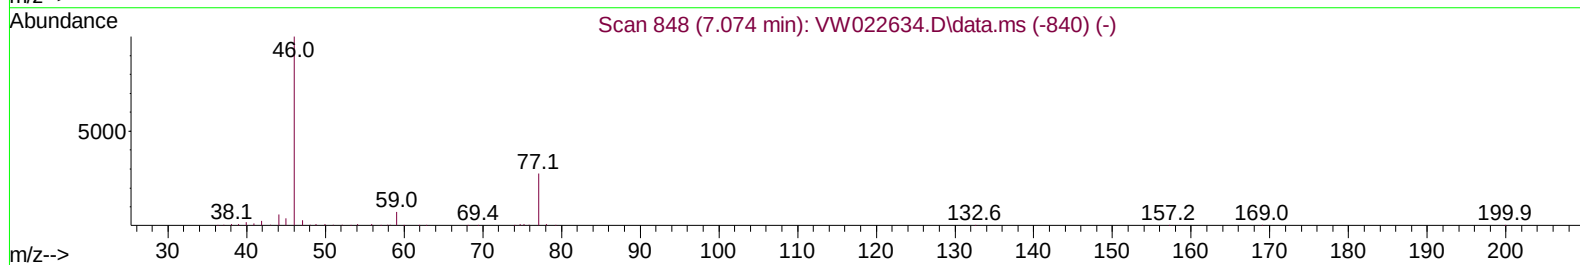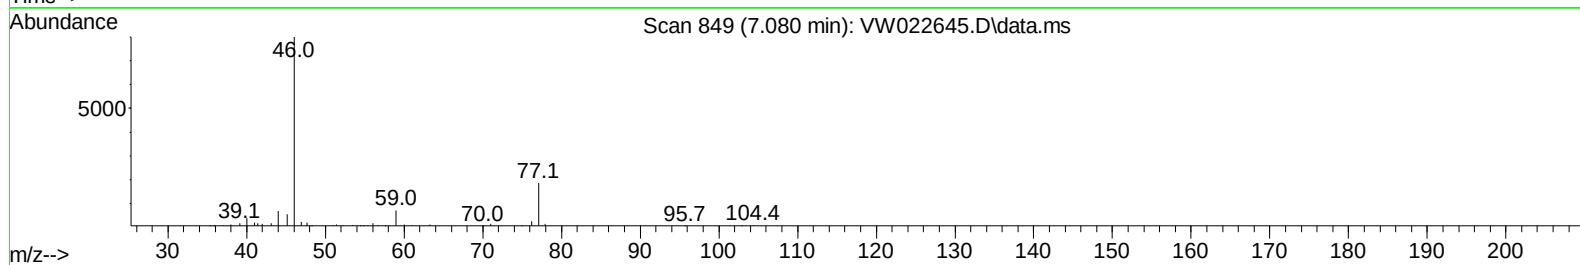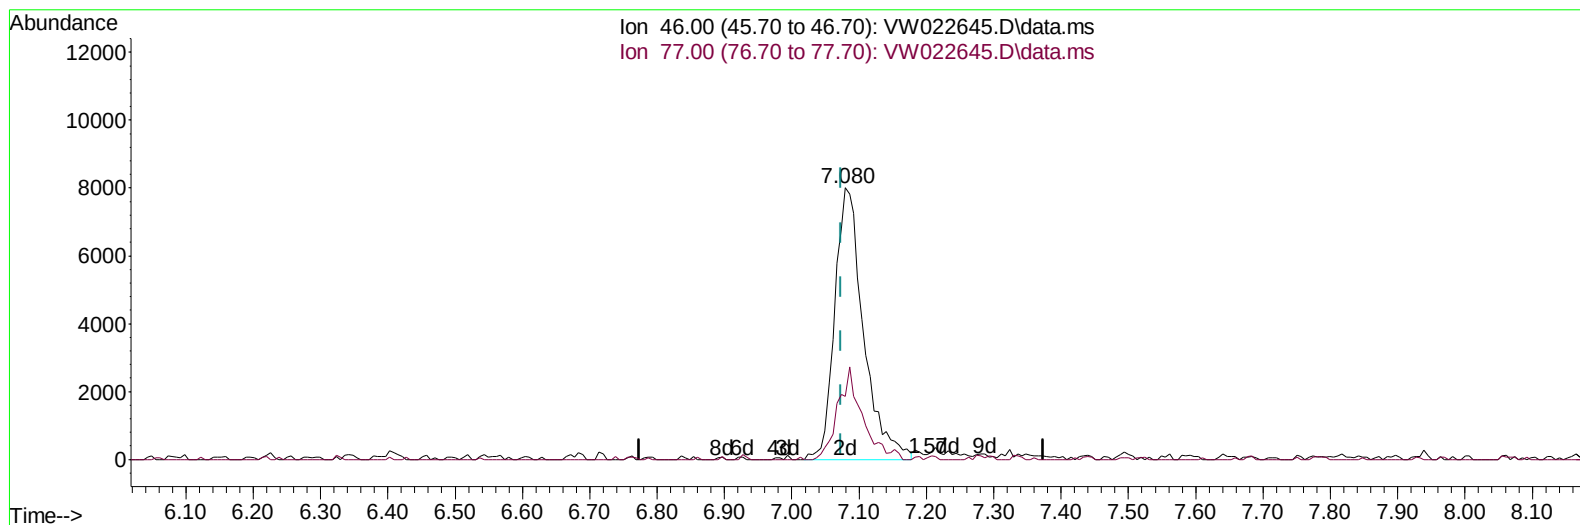

TIC: VW022645.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 60.83 ug/L m

response 23730

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	0.22#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022645.D
 Acq On : 27 Apr 2022 16:20
 Operator : SY/VA
 Sample : N2562-14
 Misc : 6.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW475

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 28 01:13:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		101069	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		88295	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		28362	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		30703	13.741	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.960%		
7) Chloroethane-d5	2.891	69		32993	23.561	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	94.240%		
11) 1,1-Dichloroethene-d2	4.019	63		36195	12.490	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	49.960%		
21) 2-Butanone-d5	7.080	46		23730m	60.833	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	121.660%		
24) Chloroform-d	7.653	84		71979	22.785	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	91.120%		
26) 1,2-Dichloroethane-d4	8.311	65		41210	22.831	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.320%		
32) Benzene-d6	8.281	84		117915	21.858	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.440%		
36) 1,2-Dichloropropane-d6	9.274	67		39804	25.497	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	102.000%		
41) Toluene-d8	10.323	98		96011	18.172	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	72.680%		
43) trans-1,3-Dichloroprop...	10.579	79		12603	17.106	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	68.440%		
47) 2-Hexanone-d5	10.926	63		17071	58.775	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	117.540%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		37884	28.540	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	114.160%		
66) 1,2-Dichlorobenzene-d4	13.853	152		24540	24.428	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	97.720%		
Target Compounds							
13) Acetone	4.153	43		2127m	8.008	ug/L	
16) Methylene chloride	4.928	84		7964	5.237	ug/L	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
Data File : VW022645.D
Acq On : 27 Apr 2022 16:20
Operator : SY/VA
Sample : N2562-14
Misc : 6.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW475

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/28/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 28 01:13:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 28 01:10:03 2022
Response via : Initial Calibration

