




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022647.D
 Acq On : 27 Apr 2022 17:08
 Operator : SY/VA
 Sample : N2562-21
 Misc : 8.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW480

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

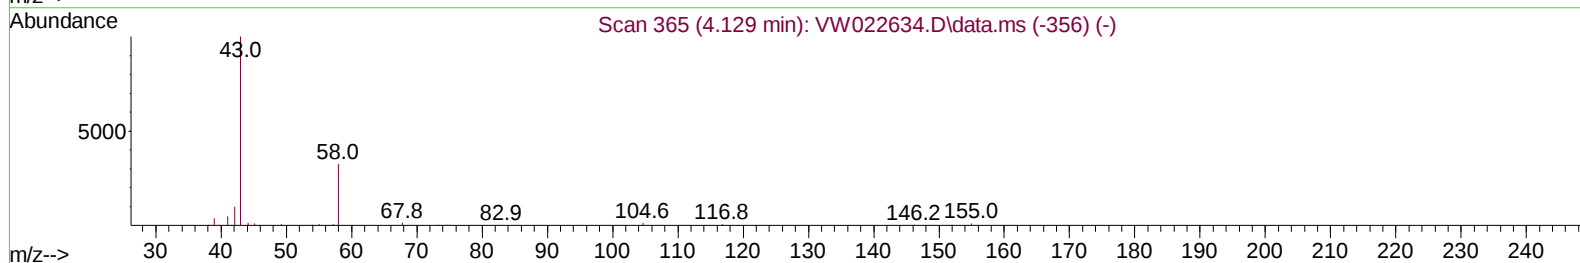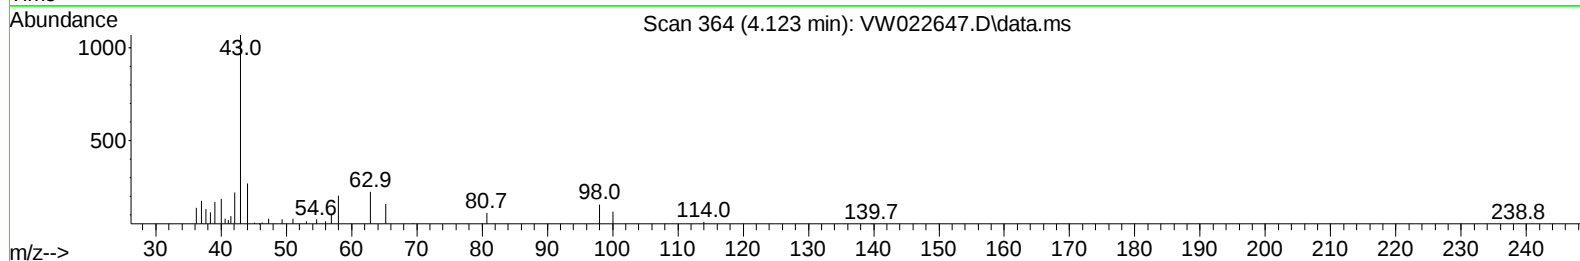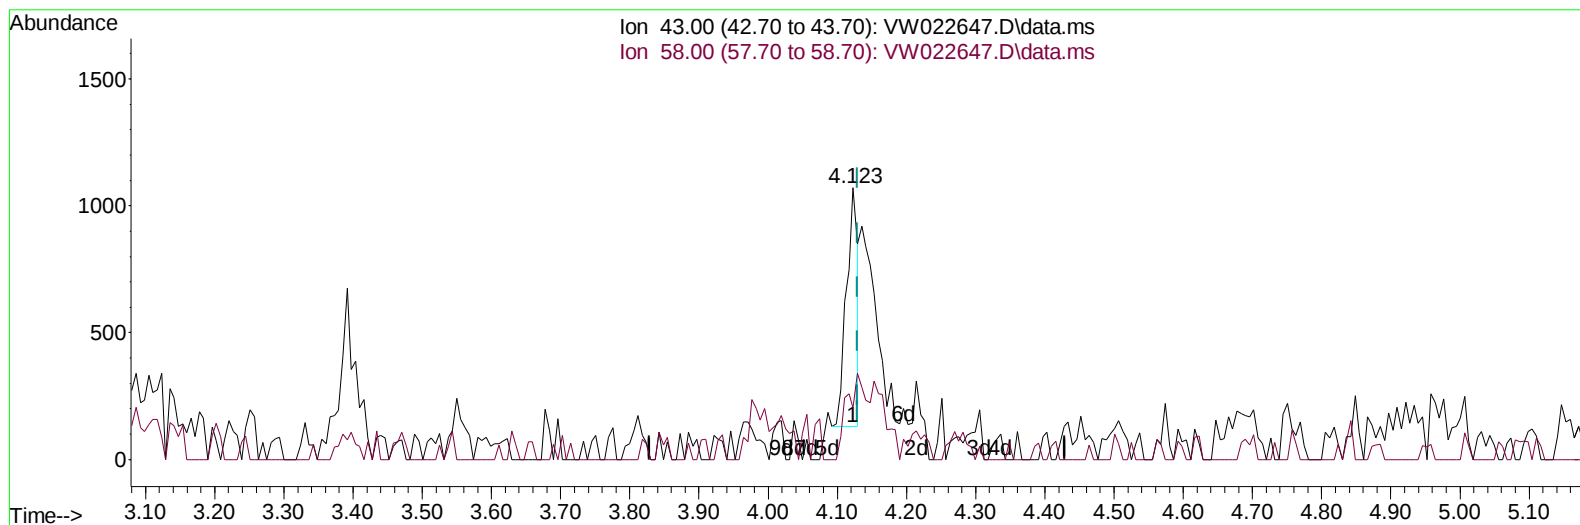

TIC: VW022647.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 1.64 ug/L

response 1069

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	37.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022647.D
 Acq On : 27 Apr 2022 17:08
 Operator : SY/VA
 Sample : N2562-21
 Misc : 8.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW480

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

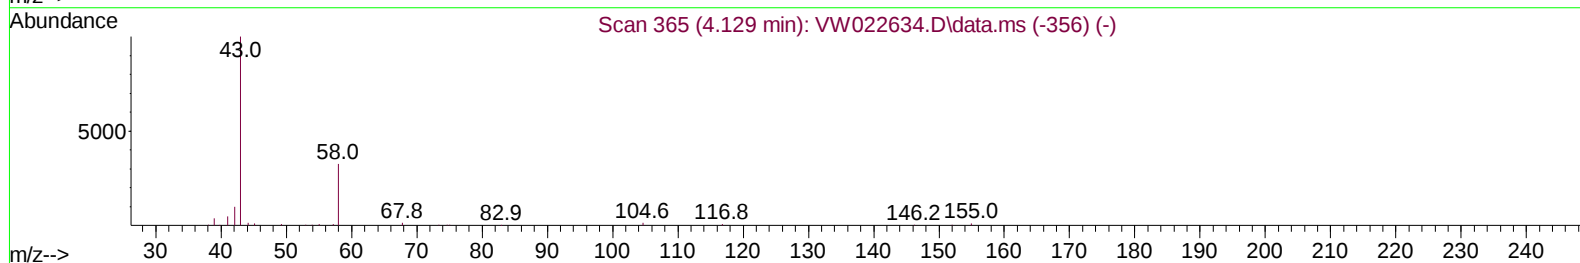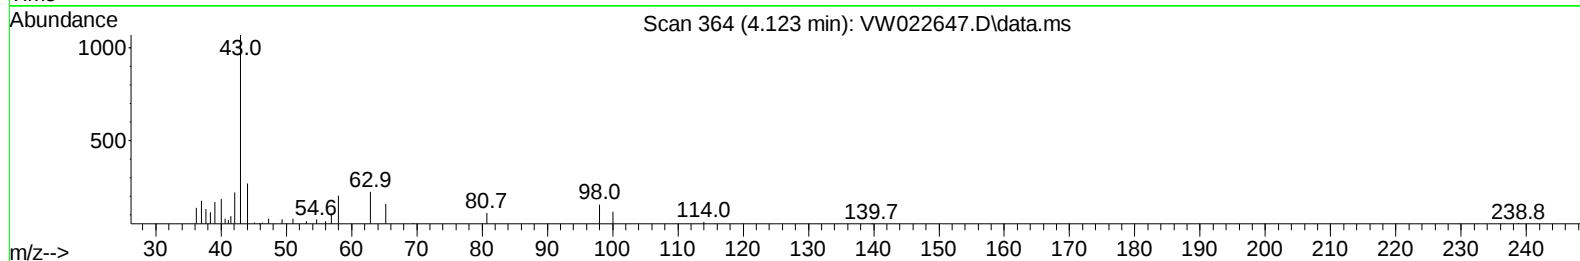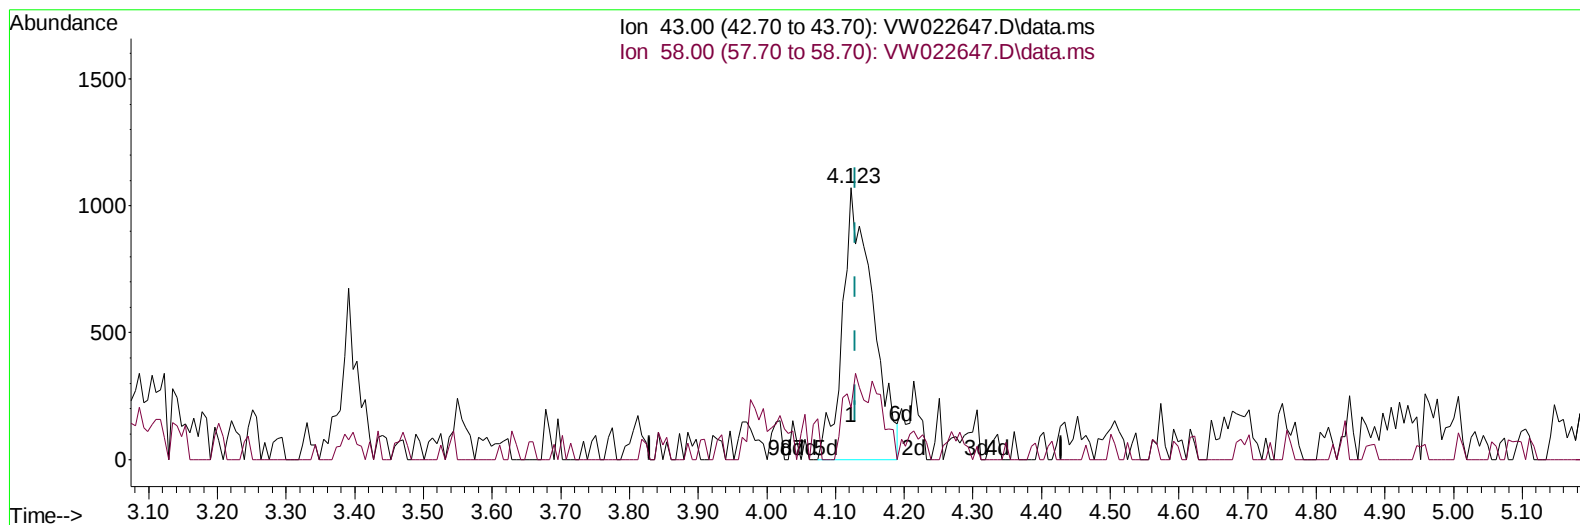

TIC: VW022647.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 5.02 ug/L m

response 3272

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	12.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022647.D
 Acq On : 27 Apr 2022 17:08
 Operator : SY/VA
 Sample : N2562-21
 Misc : 8.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW480

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		247942	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		153129	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		31513	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		77068	14.060	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	56.240%		
7) Chloroethane-d5	2.891	69		68301	19.883	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.520%		
11) 1,1-Dichloroethene-d2	4.019	63		80345	11.301	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	45.200%		
21) 2-Butanone-d5	7.080	46		73357	76.657	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	153.320%#		
24) Chloroform-d	7.653	84		171166	22.086	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	88.360%		
26) 1,2-Dichloroethane-d4	8.311	65		101100	22.832	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.320%		
32) Benzene-d6	8.275	84		275689	29.468	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	117.880%		
36) 1,2-Dichloropropane-d6	9.274	67		94111	34.761	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	139.040%#		
41) Toluene-d8	10.323	98		185706	20.267	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	81.080%		
43) trans-1,3-Dichloroprop...	10.579	79		25941	20.302	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	81.200%		
47) 2-Hexanone-d5	10.926	63		48662	96.605	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	193.220%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		99060	43.031	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	172.120%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		32748	29.339	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	117.360%		
Target Compounds							
13) Acetone	4.123	43		3272m	5.022	ug/L	
16) Methylene chloride	4.928	84		31208	8.365	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
Data File : VW022647.D
Acq On : 27 Apr 2022 17:08
Operator : SY/VA
Sample : N2562-21
Misc : 8.10g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW480

Manual IntegrationsAPPROVED

Quant Time: Apr 28 01:13:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 28 01:10:03 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/28/2022
Supervised By :Mahesh Dadoda 05/04/2022

