

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022637.D
 Acq On : 27 Apr 2022 11:19
 Operator : SY/VA
 Sample : N2562-04RE
 Misc : 7.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW464RE

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/28/2022
 Supervised By : Mahesh Dadoda 05/04/2022

Quant Time: Apr 28 01:11:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	81762	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	50019	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	11983	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	26697	14.770	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.080%		
7) Chloroethane-d5	2.885	69	26527	23.417	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.680%		
11) 1,1-Dichloroethene-d2	4.019	63	27508	11.734	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.920%		
21) 2-Butanone-d5	7.080	46	28093	89.024	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	178.040%#		
24) Chloroform-d	7.647	84	59552	23.303	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.200%		
26) 1,2-Dichloroethane-d4	8.305	65	37793	25.882	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.520%		
32) Benzene-d6	8.275	84	93664	30.650	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	122.600%		
36) 1,2-Dichloropropane-d6	9.275	67	34332	38.821	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	155.280%#		
41) Toluene-d8	10.323	98	60583	20.242	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.960%		
43) trans-1,3-Dichloroprop...	10.579	79	8886	21.291	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.160%		
47) 2-Hexanone-d5	10.921	63	19100	116.083	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	232.160%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	40392	53.716	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	214.880%#		
66) 1,2-Dichlorobenzene-d4	13.847	152	12618	29.729	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	118.920%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	2411m	11.221	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
Data File : VW022637.D
Acq On : 27 Apr 2022 11:19
Operator : SY/VA
Sample : N2562-04RE
Misc : 7.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW464RE

Quant Time: Apr 28 01:11:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 28 01:10:03 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/28/2022
Supervised By :Mahesh Dadoda 05/04/2022

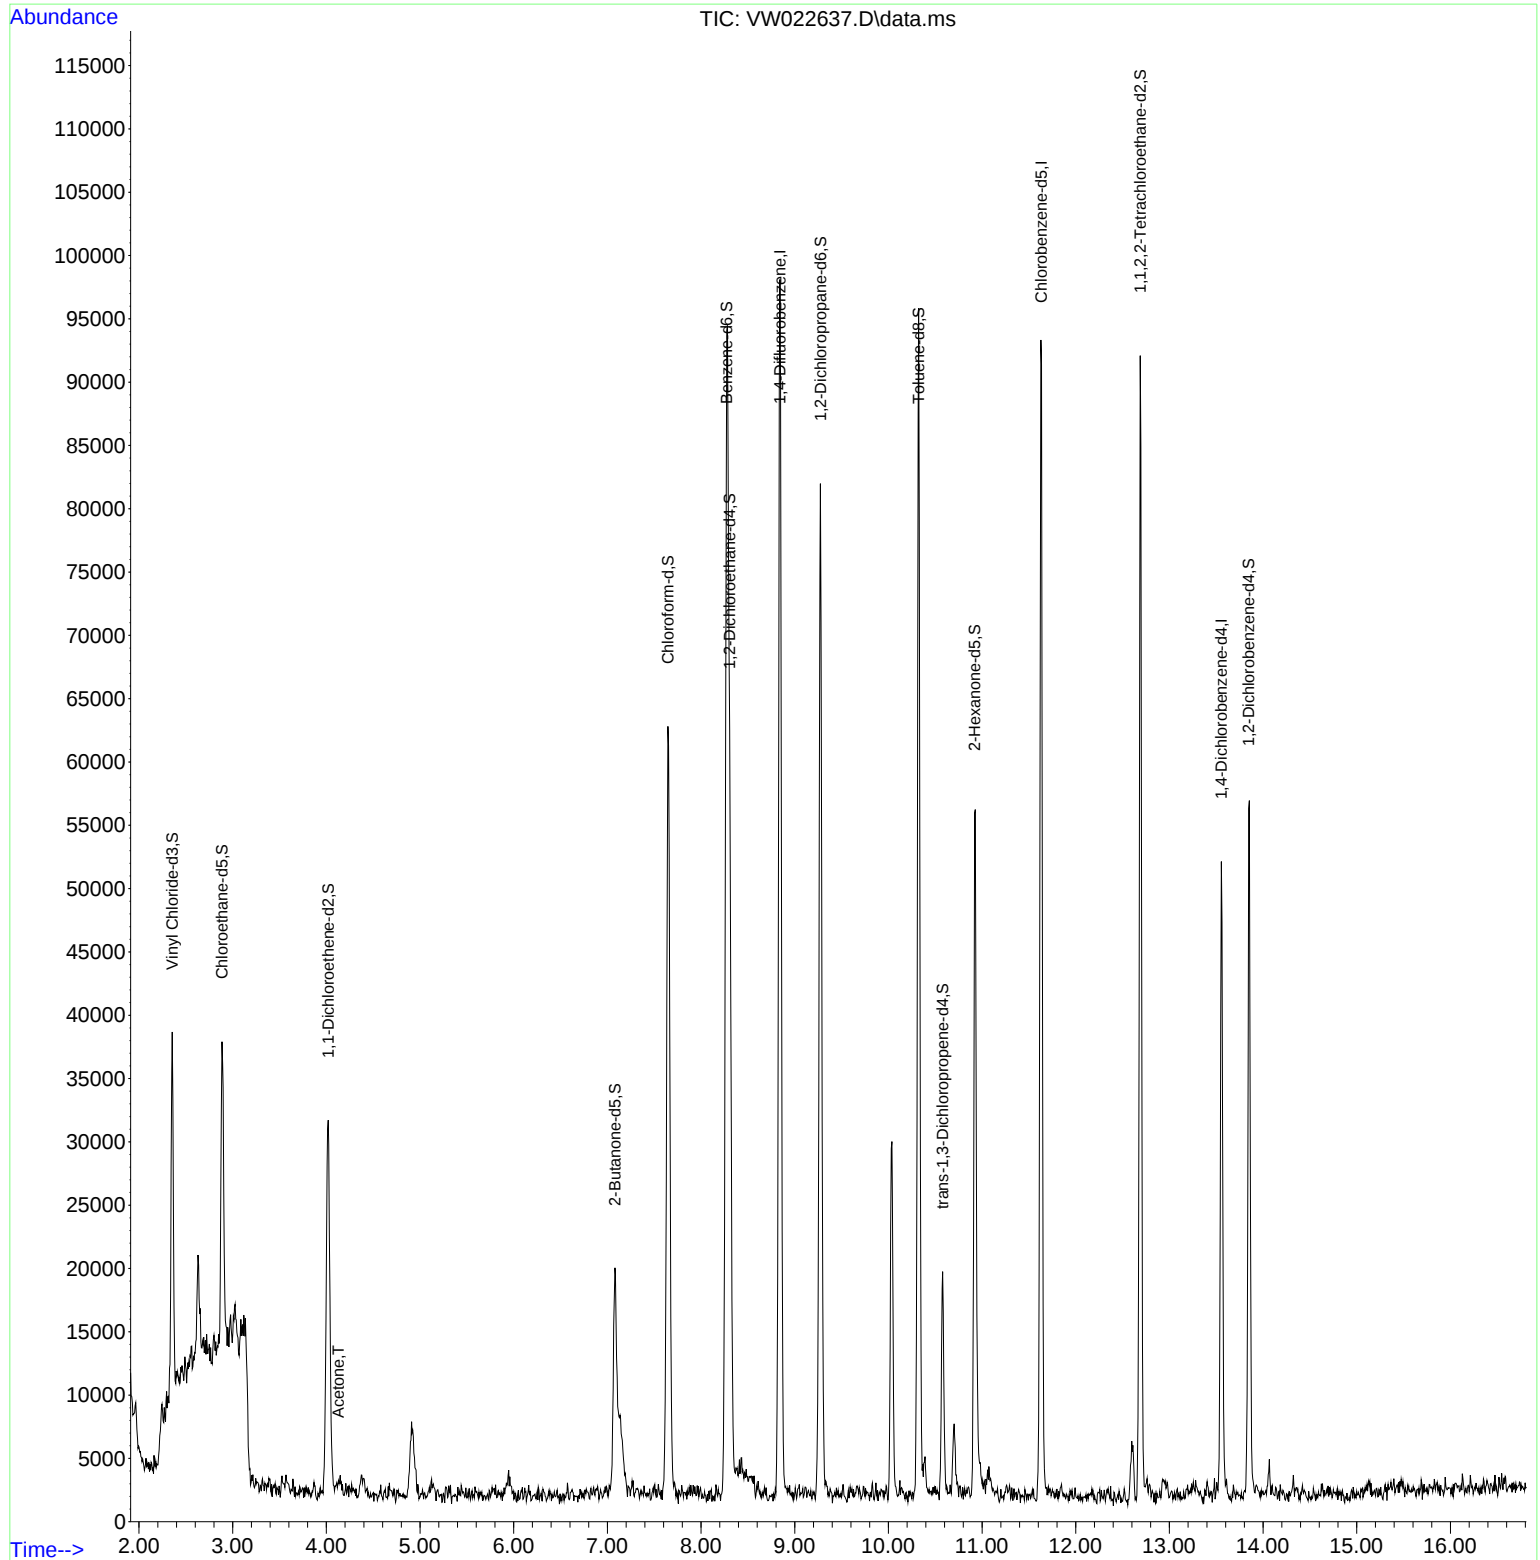

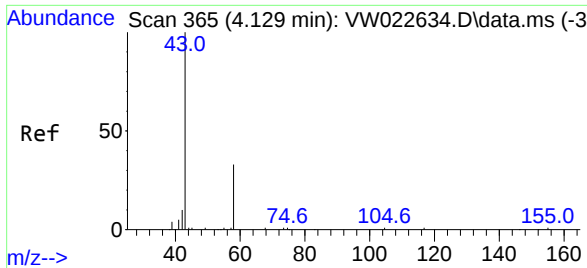

#13
Acetone
Concen: 11.221 ug/L m
RT: 4.129 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW022637.D
Acq: 27 Apr 2022 11:19

Instrument :
MSVOA_W
ClientSampleId :
EW464RE

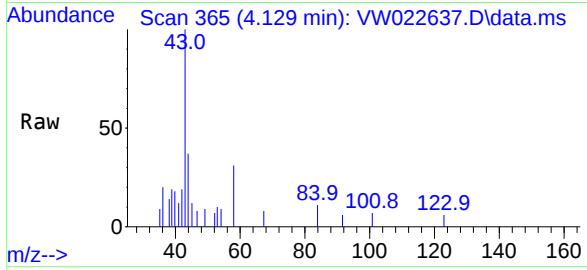

Tgt Ion: 43 Resp: 241
Ion Ratio Lower Upper
43 100
58 13.6 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/28/2022
Supervised By :Mahesh Dadoda 05/04/2022

