

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
 Data File : VW022643.D
 Acq On : 27 Apr 2022 15:32
 Operator : SY/VA
 Sample : N2562-10
 Misc : 3.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW470

Quant Time: Apr 28 01:12:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 28 01:10:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	412489	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	383497	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	168463	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	99455	10.906	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	43.640%
7) Chloroethane-d5	2.891	69	82418	14.421	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.680%
11) 1,1-Dichloroethene-d2	4.019	63	122308	10.341	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.360%#
21) 2-Butanone-d5	7.073	46	80342	50.465	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.920%
24) Chloroform-d	7.646	84	248580	19.280	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.120%
26) 1,2-Dichloroethane-d4	8.305	65	140231	19.036	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.160%
32) Benzene-d6	8.274	84	428529	18.290	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.160%
36) 1,2-Dichloropropane-d6	9.274	67	140435	20.712	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.840%
41) Toluene-d8	10.323	98	378415	16.491	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.960%
43) trans-1,3-Dichloroprop...	10.579	79	52109	16.284	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.120%
47) 2-Hexanone-d5	10.920	63	64273	50.949	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.900%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	135639	23.527	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.120%
66) 1,2-Dichlorobenzene-d4	13.852	152	129324	21.673	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.680%
Target Compounds					Qvalue	
13) Acetone	4.123	43	7028	6.484	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042722\
Data File : VW022643.D
Acq On : 27 Apr 2022 15:32
Operator : SY/VA
Sample : N2562-10
Misc : 3.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW470

Quant Time: Apr 28 01:12:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 28 01:10:03 2022
Response via : Initial Calibration

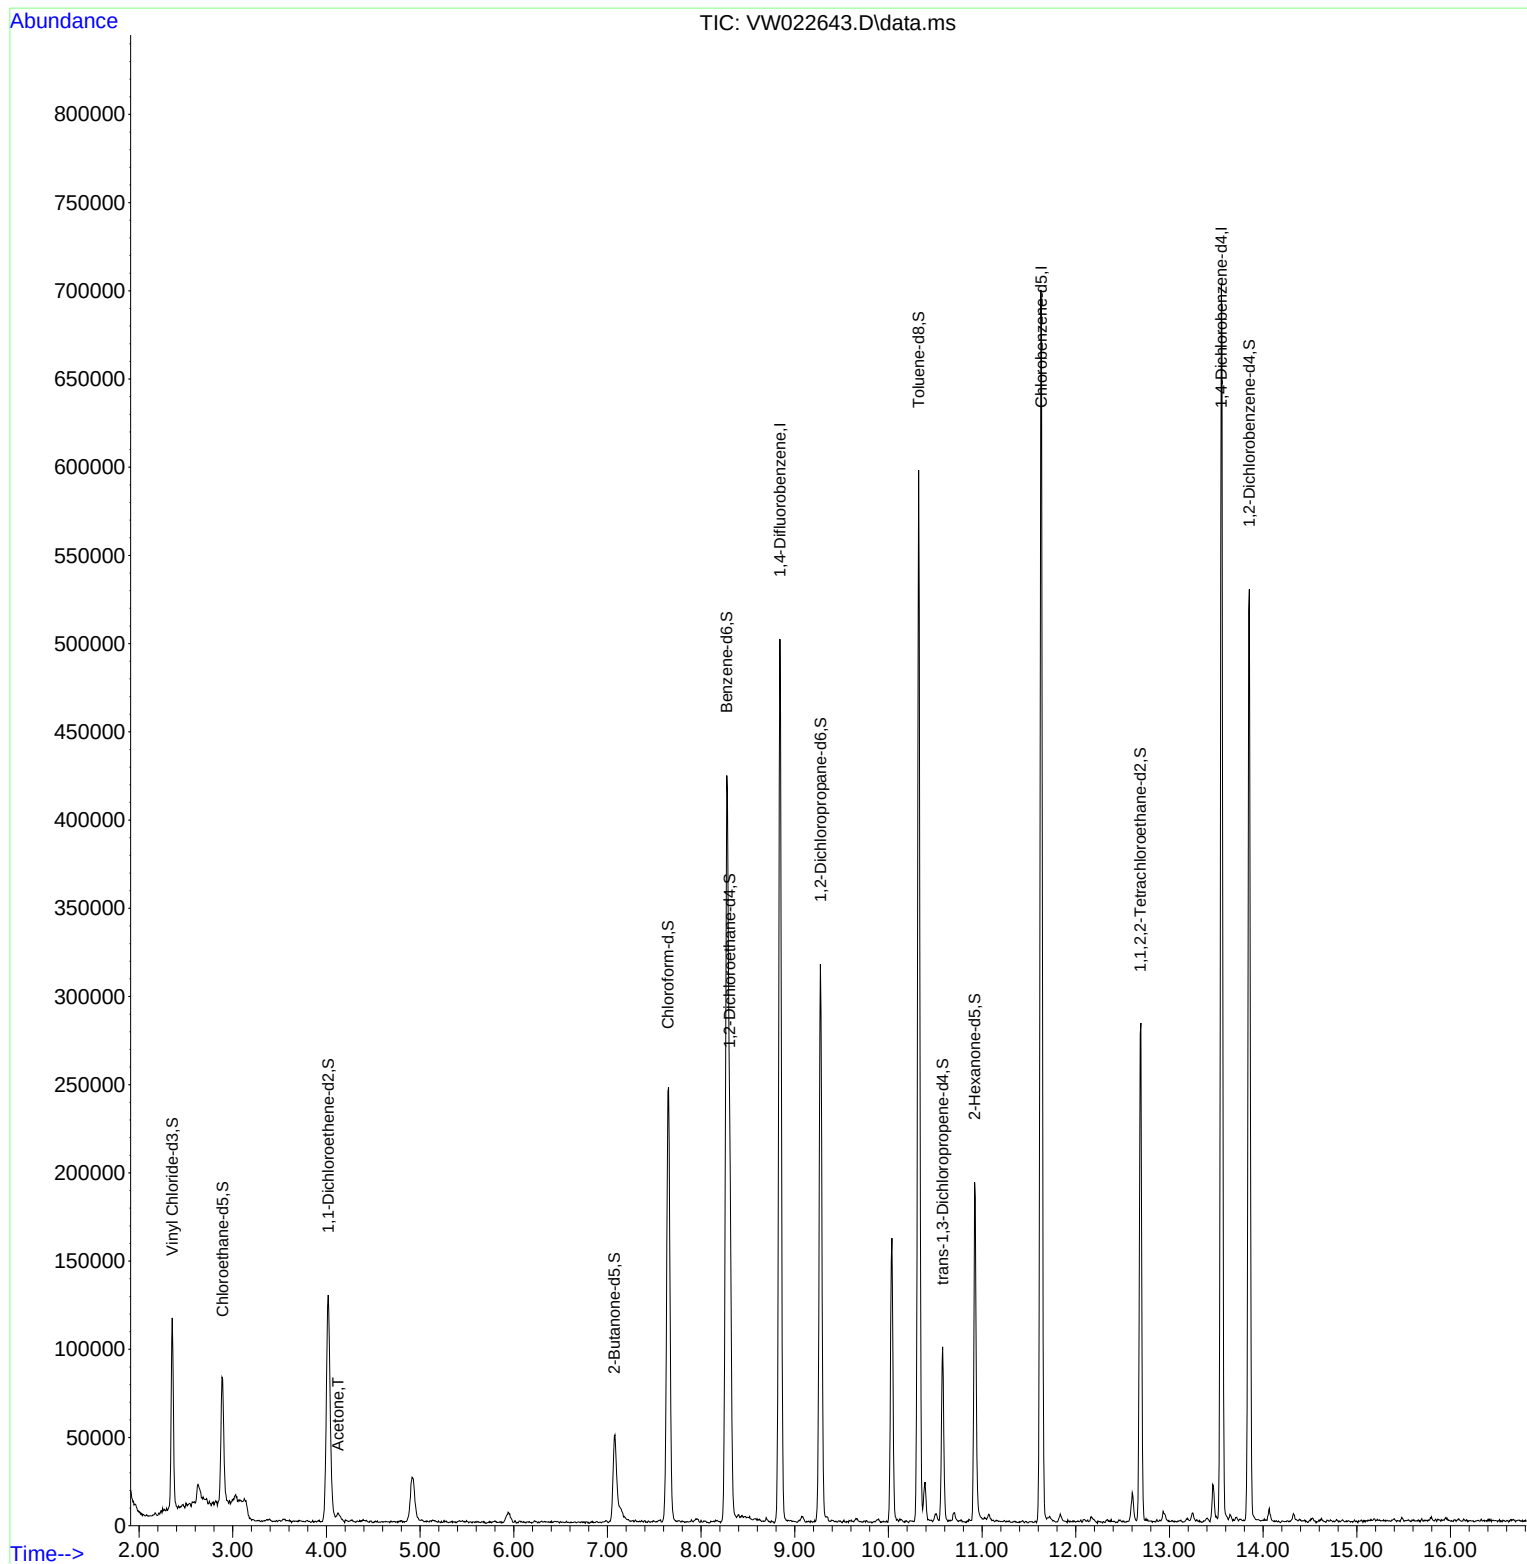

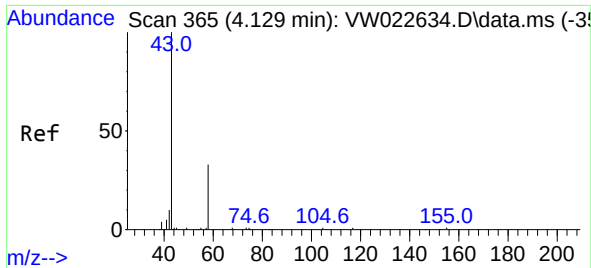

#13
 Acetone
 Concen: 6.484 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022643.D
 Acq: 27 Apr 2022 15:32

Instrument :
 MSVOA_W
 ClientSampleId :
 EW470

Tgt Ion: 43 Resp: 7028
 Ion Ratio Lower Upper
 43 100
 58 39.0 0.0 57.0

